

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
 Data File : BM014903.D
 Acq On : 02 May 2018 01:50
 Operator : SJ/JU
 Sample : J2638-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA5

Quant Time: May 02 04:59:56 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	403527	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1720372	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	906448	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1905643	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1760219	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1666796	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	65360	7.07	ng/uL	0.00
5) Phenol-d5	7.62	99	218083	6.99	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	701518	35.07	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	690890	26.48	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	393430	15.81	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	400713	32.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	419044	33.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	705098	28.02	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	2449	0.10	ng/ul	0.01
43) Dimethylphthalate-d6	14.49	166	2307584	32.61	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2683495	30.71	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	61758	4.70	ng/ul	0.00
57) Fluorene-d10	16.08	176	1944482	31.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	275361	26.70	ng/ul	0.00
70) Anthracene-d10	17.91	188	2880538	32.44	ng/ul	0.00
76) Pyrene-d10	20.15	212	2966811	35.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	2849710	34.80	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.54	163	182387	2.666 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
Data File : BM014903.D
Acq On : 02 May 2018 01:50
Operator : SJ/JU
Sample : J2638-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA5

Quant Time: May 02 04:59:56 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

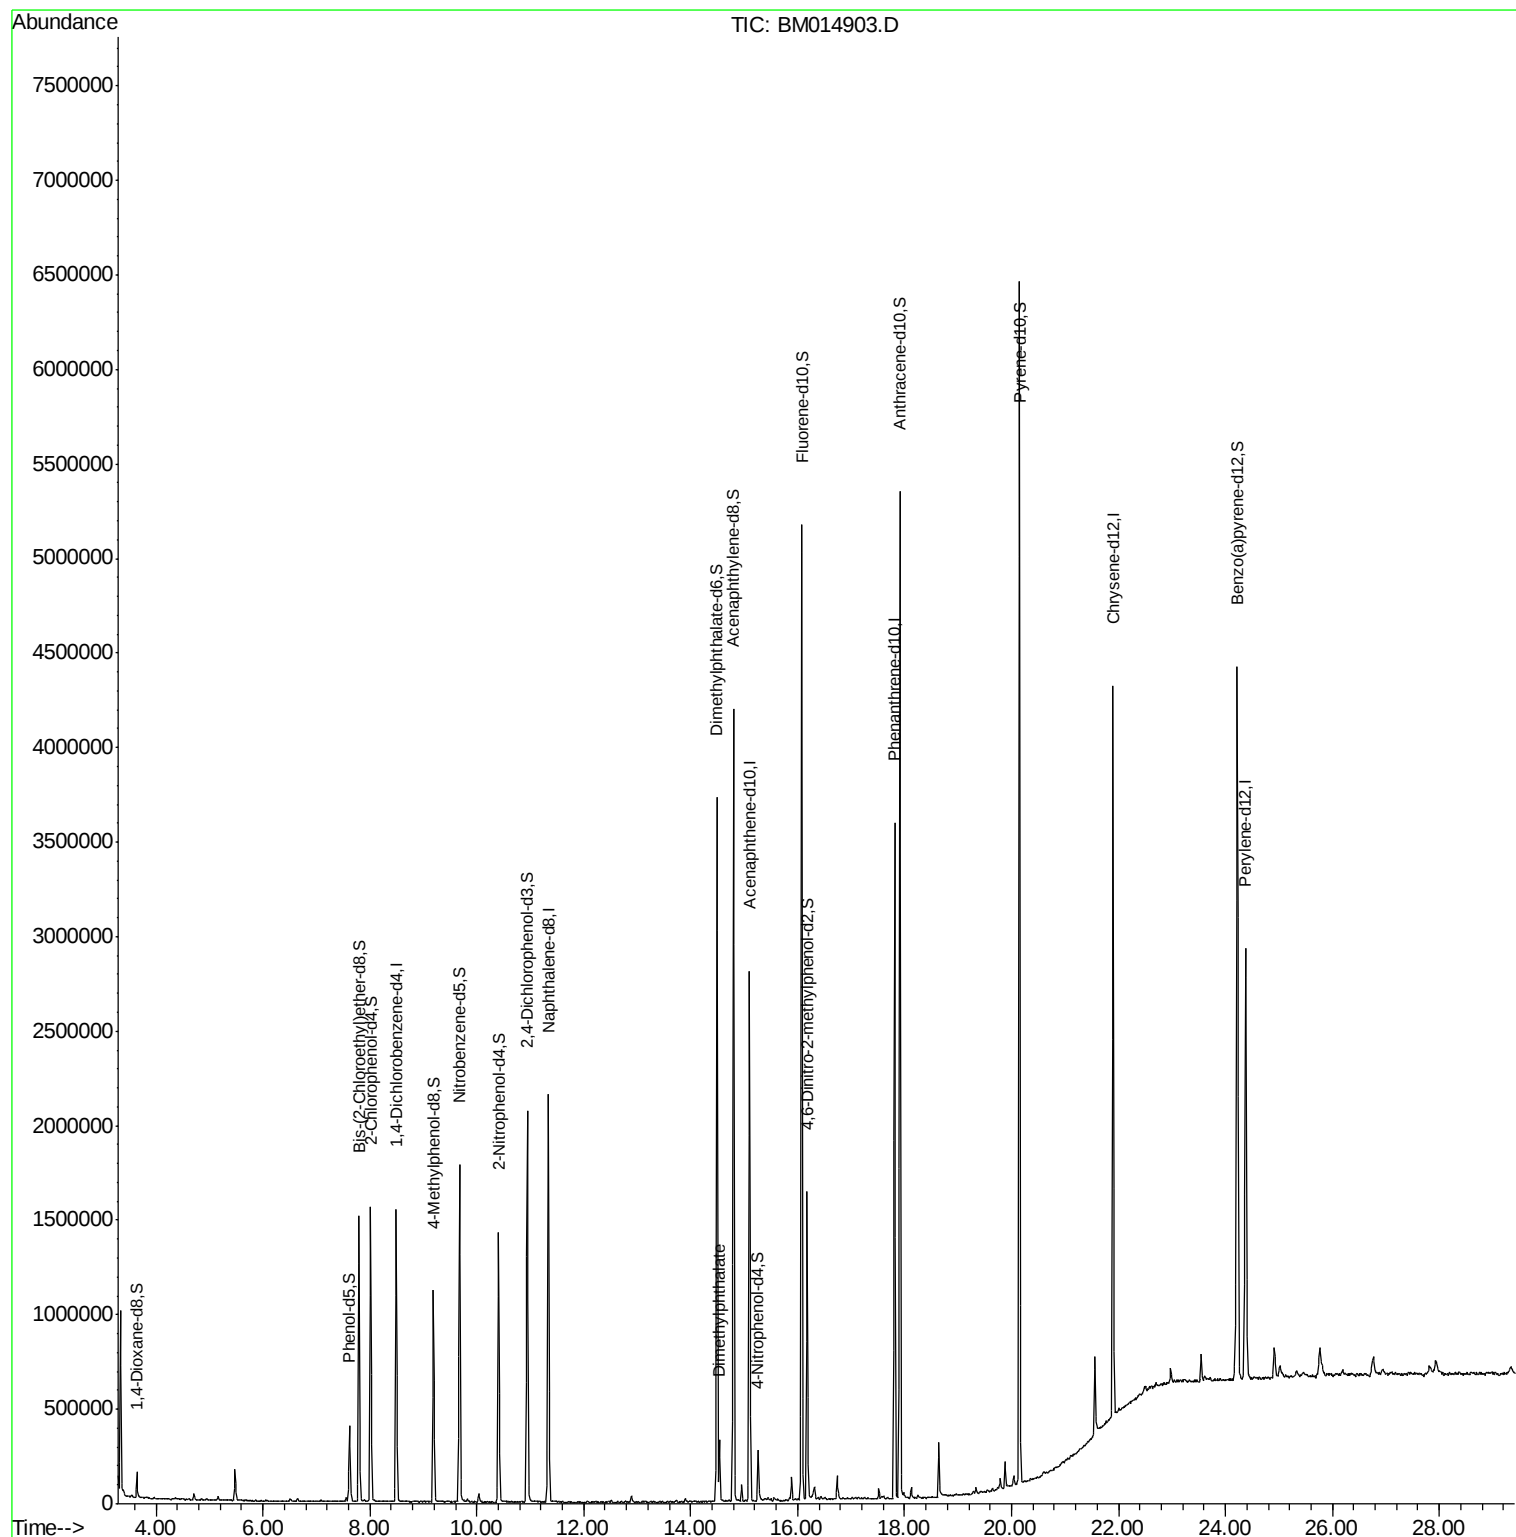

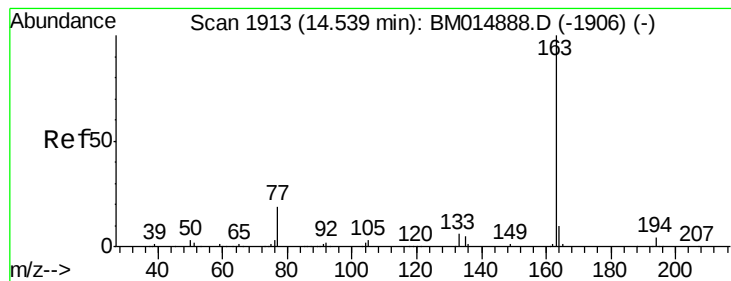

#44

Dimethylphthalate

Concen: 2.666 ng/ul

RT: 14.54 min Scan# 1913

Delta R.T. 0.00 min

Lab File: BM014903.D

Acq: 02 May 2018 01:50

Instrument :

BNA_M

ClientSampleId :

C0AA5


Tgt Ion:163 Resp: 182387

Ion Ratio Lower Upper

163 100

194 3.5 3.5 5.3#

164 9.9 8.2 12.4

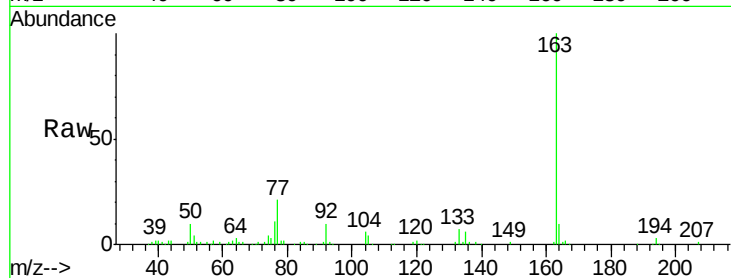

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

