

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
 Data File : BM014904.D
 Acq On : 02 May 2018 02:27
 Operator : SJ/JU
 Sample : J2638-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AA4

Quant Time: May 02 05:00:10 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 02 04:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	378259	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1538985	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	765545	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1556375	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1545168	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1638459	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	64865	7.49	ng/uL	0.00
5) Phenol-d5	7.62	99	200746	6.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	642967	34.29	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	639536	26.14	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	365124	15.66	ng/ul	0.00
19) Nitrobenzene-d5	9.67	128	362486	32.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	371784	33.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	628344	27.91	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	28754	1.29	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	1930918	32.31	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2301181	31.18	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	49037	4.42	ng/ul	0.00
57) Fluorene-d10	16.08	176	1636678	31.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	221951	26.35	ng/ul	0.00
70) Anthracene-d10	17.91	188	2390865	32.96	ng/ul	0.00
76) Pyrene-d10	20.15	212	2459599	33.64	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	2812919	34.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.54	163	87810	1.520	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050118\
Data File : BM014904.D
Acq On : 02 May 2018 02:27
Operator : SJ/JU
Sample : J2638-13
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AA4

Quant Time: May 02 05:00:10 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 02 04:52:22 2018
Response via : Initial Calibration

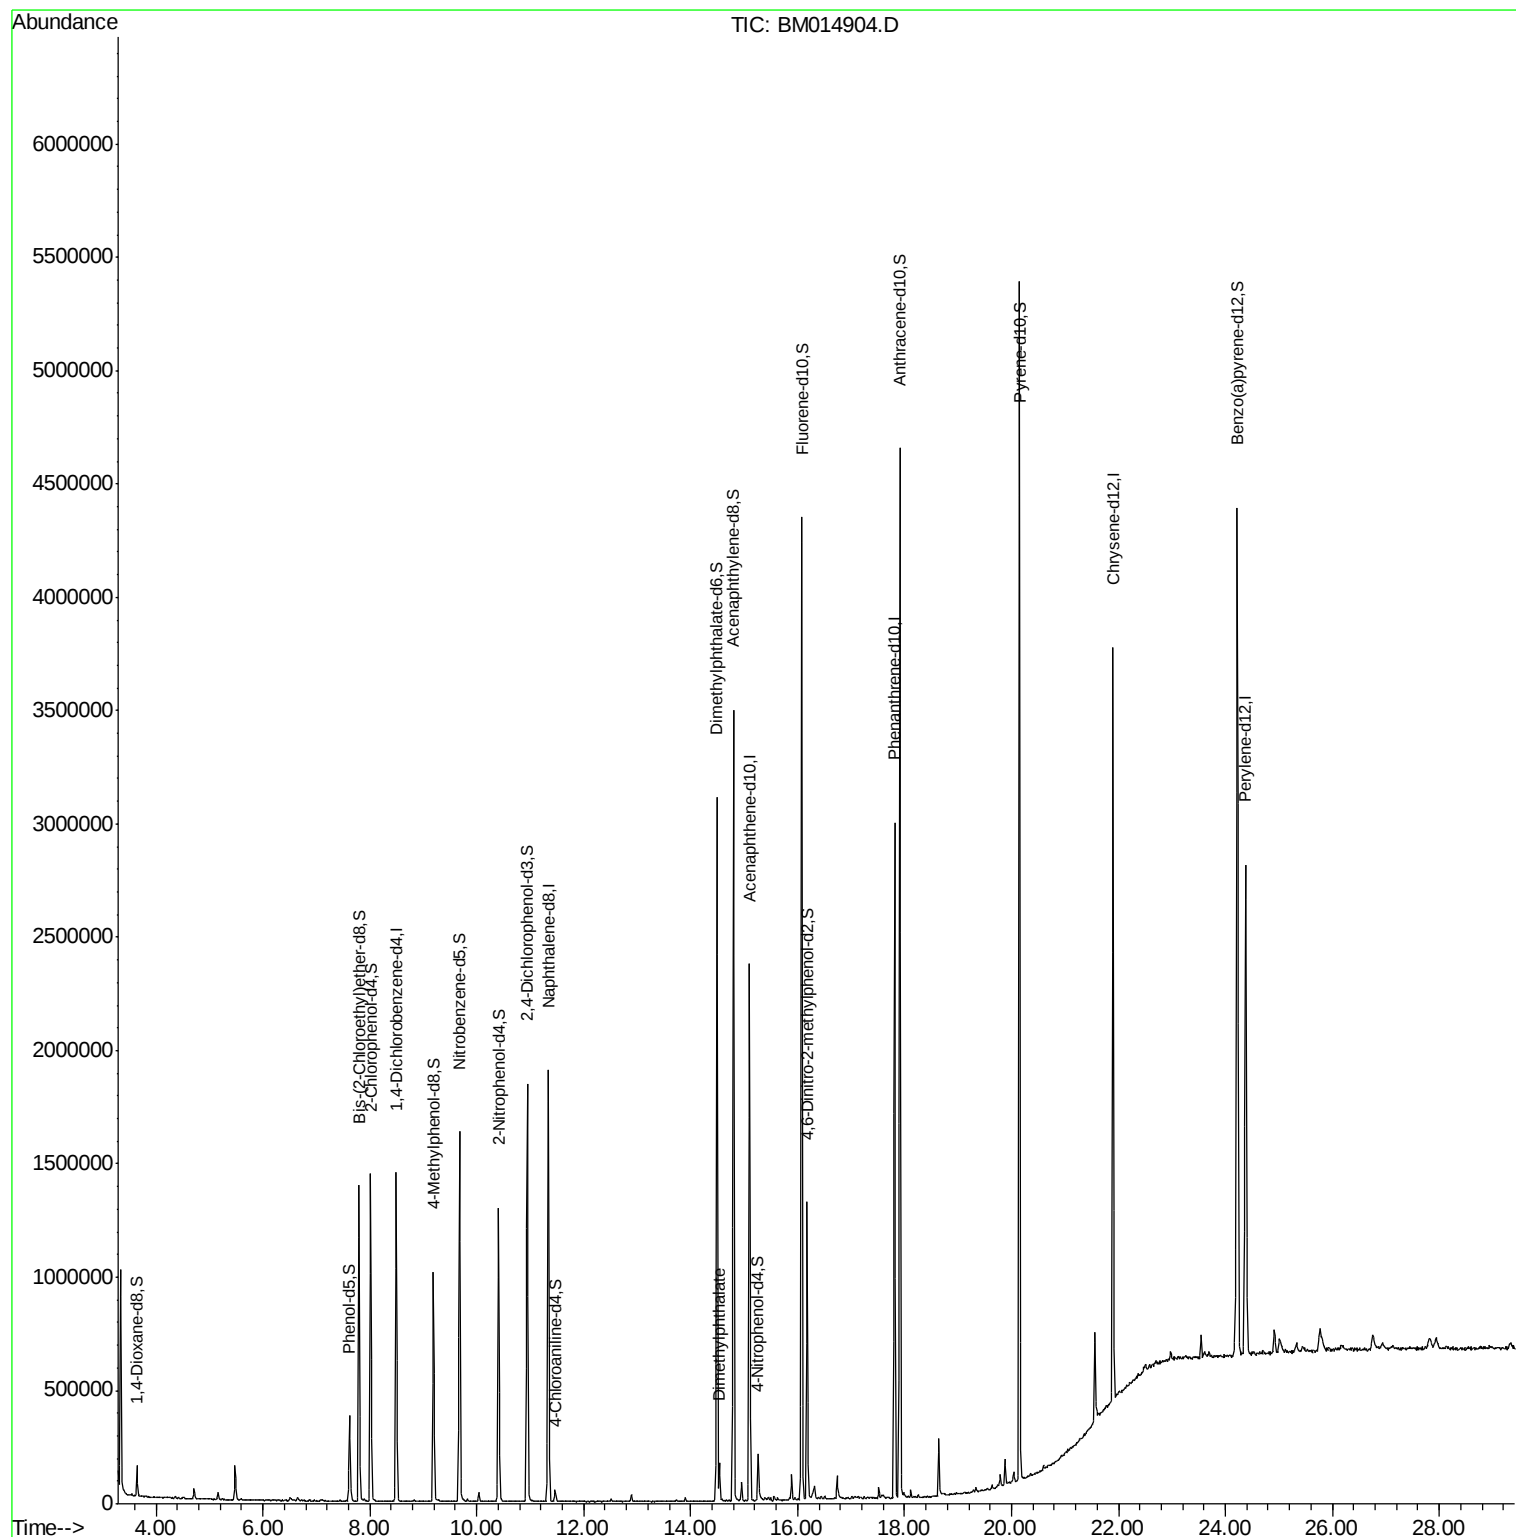

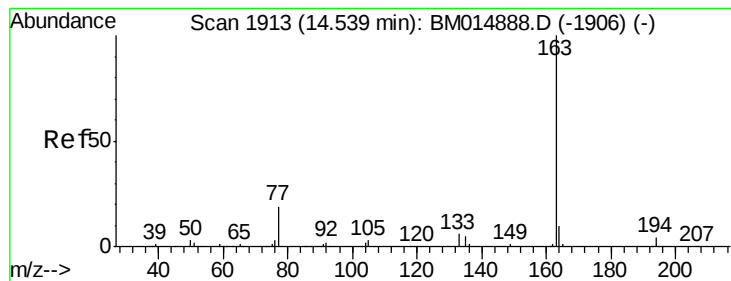

#44
 Dimethylphthalate
 Concen: 1.520 ng/ul
 RT: 14.54 min Scan# 1913
 Delta R.T. 0.00 min
 Lab File: BM014904.D
 Acq: 02 May 2018 02:27

Instrument :
 BNA_M
 ClientSampleId :
 C0AA4

Tgt Ion:163 Resp: 87810
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.5 5.3
 164 10.6 8.2 12.4

