

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050125\
 Data File : BM050067.D
 Acq On : 01 May 2025 16:44
 Operator : RC/JU
 Sample : Q1914-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SS-91

Quant Time: May 01 18:06:39 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	241297	20.000	ng	-0.02
21) Naphthalene-d8	10.539	136	826545	20.000	ng	-0.02
39) Acenaphthene-d10	14.392	164	542720	20.000	ng	-0.02
64) Phenanthrene-d10	17.139	188	1075472	20.000	ng	-0.02
76) Chrysene-d12	21.380	240	1169707	20.000	ng	-0.02
86) Perylene-d12	24.374	264	1275485	20.000	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	1842545	133.712	ng	-0.02
7) Phenol-d6	6.934	99	2344634	135.375	ng	-0.02
23) Nitrobenzene-d5	8.904	82	1372632	81.833	ng	-0.02
42) 2,4,6-Tribromophenol	15.886	330	1143242	142.463	ng	-0.02
45) 2-Fluorobiphenyl	13.010	172	3546344	77.301	ng	-0.02
79) Terphenyl-d14	19.768	244	6306366	79.779	ng	-0.01
Target Compounds						
						Qvalue
60) Diethylphthalate	15.215	149	137565	3.681	ng	98
74) Di-n-butylphthalate	18.109	149	225196	3.550	ng	99
75) Fluoranthene	19.203	202	152568	2.142	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050125\
Data File : BM050067.D
Acq On : 01 May 2025 16:44
Operator : RC/JU
Sample : Q1914-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SS-91

Quant Time: May 01 18:06:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

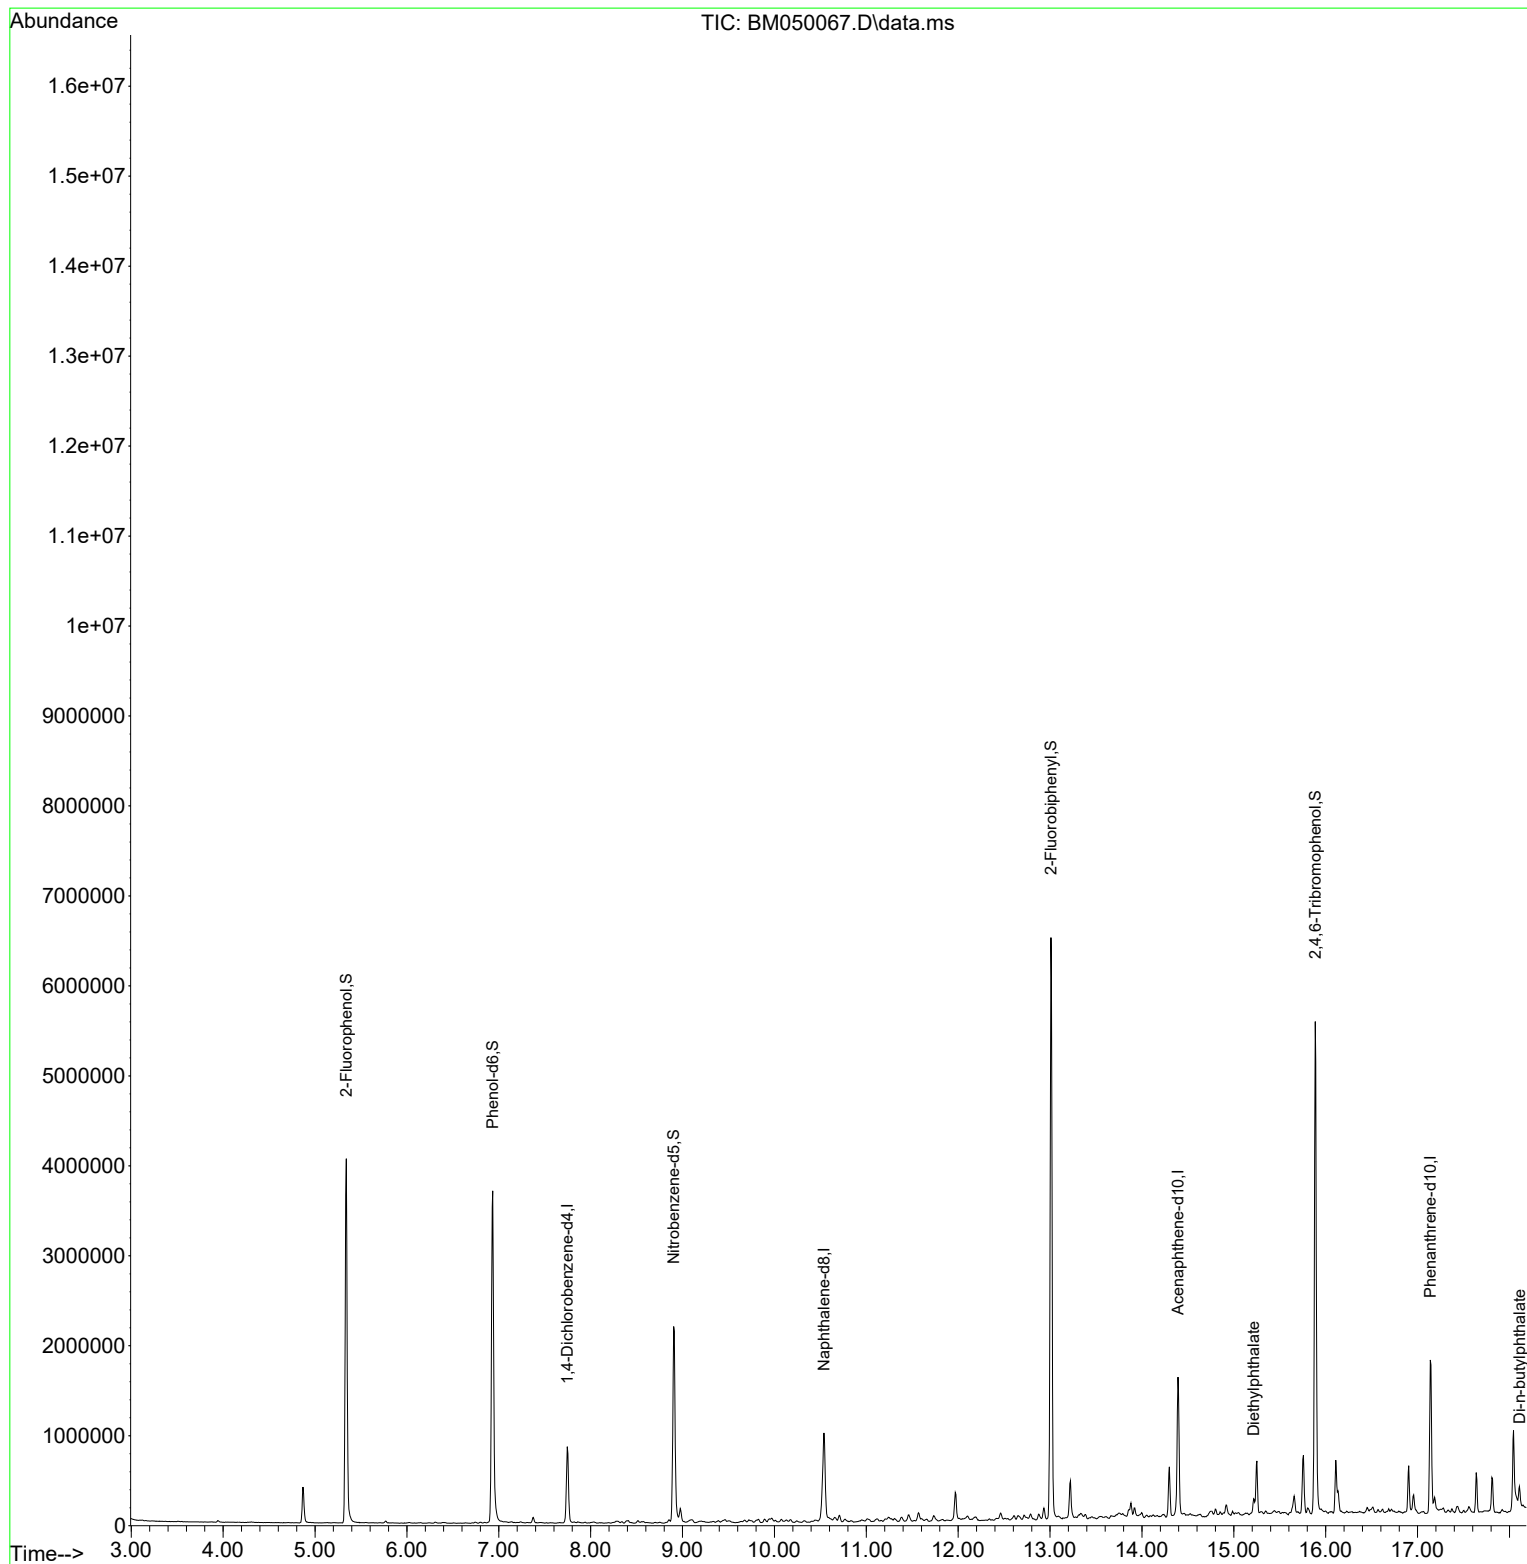

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050125\
Data File : BM050067.D
Acq On : 01 May 2025 16:44
Operator : RC/JU
Sample : Q1914-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SS-91

Quant Time: May 01 18:06:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

