

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050125\  
 Data File : BM050077.D  
 Acq On : 01 May 2025 23:15  
 Operator : RC/JU  
 Sample : Q1906-09 5X  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 WC-6

Quant Time: May 02 01:14:10 2025  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042825.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Apr 28 18:09:16 2025  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|--------|------|----------|--------|-------|----------|
| -----                       |        |      |          |        |       |          |
| Internal Standards          |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.751  | 152  | 260963   | 20.000 | ng    | -0.02    |
| 21) Naphthalene-d8          | 10.540 | 136  | 956596   | 20.000 | ng    | -0.02    |
| 39) Acenaphthene-d10        | 14.392 | 164  | 662166   | 20.000 | ng    | -0.02    |
| 64) Phenanthrene-d10        | 17.145 | 188  | 1355794  | 20.000 | ng    | -0.01    |
| 76) Chrysene-d12            | 21.380 | 240  | 1317336  | 20.000 | ng    | -0.02    |
| 86) Perylene-d12            | 24.374 | 264  | 1346752  | 20.000 | ng    | -0.03    |
| System Monitoring Compounds |        |      |          |        |       |          |
| 5) 2-Fluorophenol           | 5.346  | 112  | 219213   | 14.709 | ng    | -0.01    |
| 7) Phenol-d6                | 6.940  | 99   | 293970   | 15.694 | ng    | -0.01    |
| 23) Nitrobenzene-d5         | 8.910  | 82   | 158699   | 8.175  | ng    | -0.02    |
| 42) 2,4,6-Tribromophenol    | 15.892 | 330  | 142542   | 14.558 | ng    | -0.01    |
| 45) 2-Fluorobiphenyl        | 13.016 | 172  | 481951   | 8.610  | ng    | -0.02    |
| 79) Terphenyl-d14           | 19.768 | 244  | 715529   | 8.037  | ng    | -0.01    |
| Target Compounds            |        |      |          |        |       |          |
|                             |        |      |          |        |       | Qvalue   |
| 75) Fluoranthene            | 19.204 | 202  | 180287   | 2.008  | ng    | 99       |
| 78) Pyrene                  | 19.568 | 202  | 228962   | 2.475  | ng    | 100      |
| 88) Benzo(b)fluoranthene    | 23.433 | 252  | 222746   | 2.543  | ng    | # 95     |
| -----                       |        |      |          |        |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050125\  
Data File : BM050077.D  
Acq On : 01 May 2025 23:15  
Operator : RC/JU  
Sample : Q1906-09 5X  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
WC-6

Quant Time: May 02 01:14:10 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042825.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 28 18:09:16 2025  
Response via : Initial Calibration

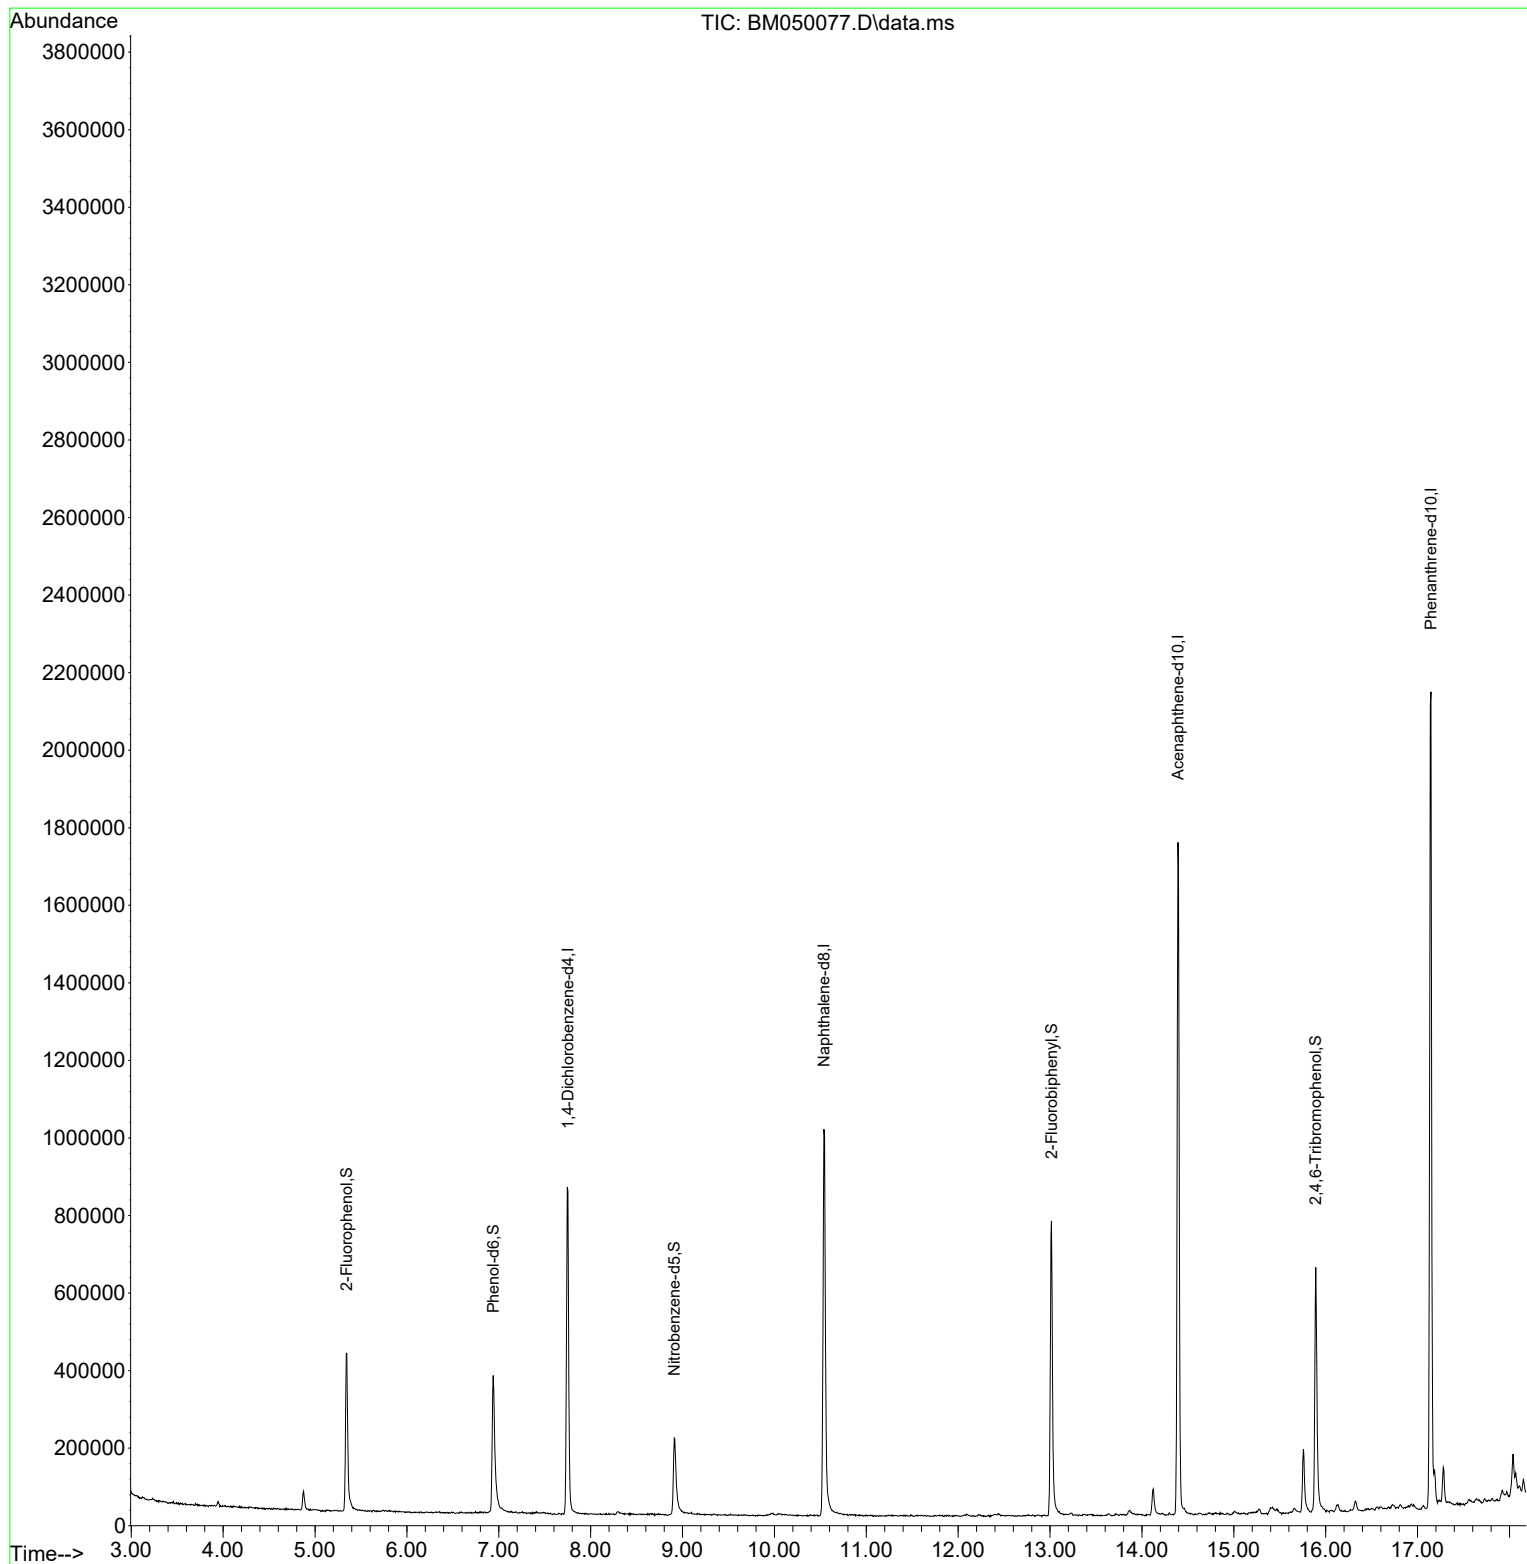

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050125\  
Data File : BM050077.D  
Acq On : 01 May 2025 23:15  
Operator : RC/JU  
Sample : Q1906-09 5X  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
WC-6

Quant Time: May 02 01:14:10 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042825.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 28 18:09:16 2025  
Response via : Initial Calibration

