

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005197.D
 Acq On : 02 May 2016 17:45
 Operator : UM/SJ
 Sample : H2772-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3A9

Quant Time: May 03 03:25:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	42427	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	203237	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	127908	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	277097	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	243018	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	210833	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	2113	2.53	ng/uL	0.00
5) Phenol-d5	6.96	99	42873	12.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	29461	14.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	35834	12.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	26814	9.01	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	17656	12.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	19600	12.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	36286	12.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	46292	13.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	148370	14.69	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	168064	13.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	13030	7.38	ng/ul	0.00
57) Fluorene-d10	15.42	176	127840	14.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	13177	8.36	ng/ul	0.00
70) Anthracene-d10	17.27	188	203259	16.36	ng/ul	0.00
76) Pyrene-d10	19.57	212	227388	20.55	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	170819	18.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.88	163	30302	2.99	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005197.D
Acq On : 02 May 2016 17:45
Operator : UM/SJ
Sample : H2772-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3A9

Quant Time: May 03 03:25:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

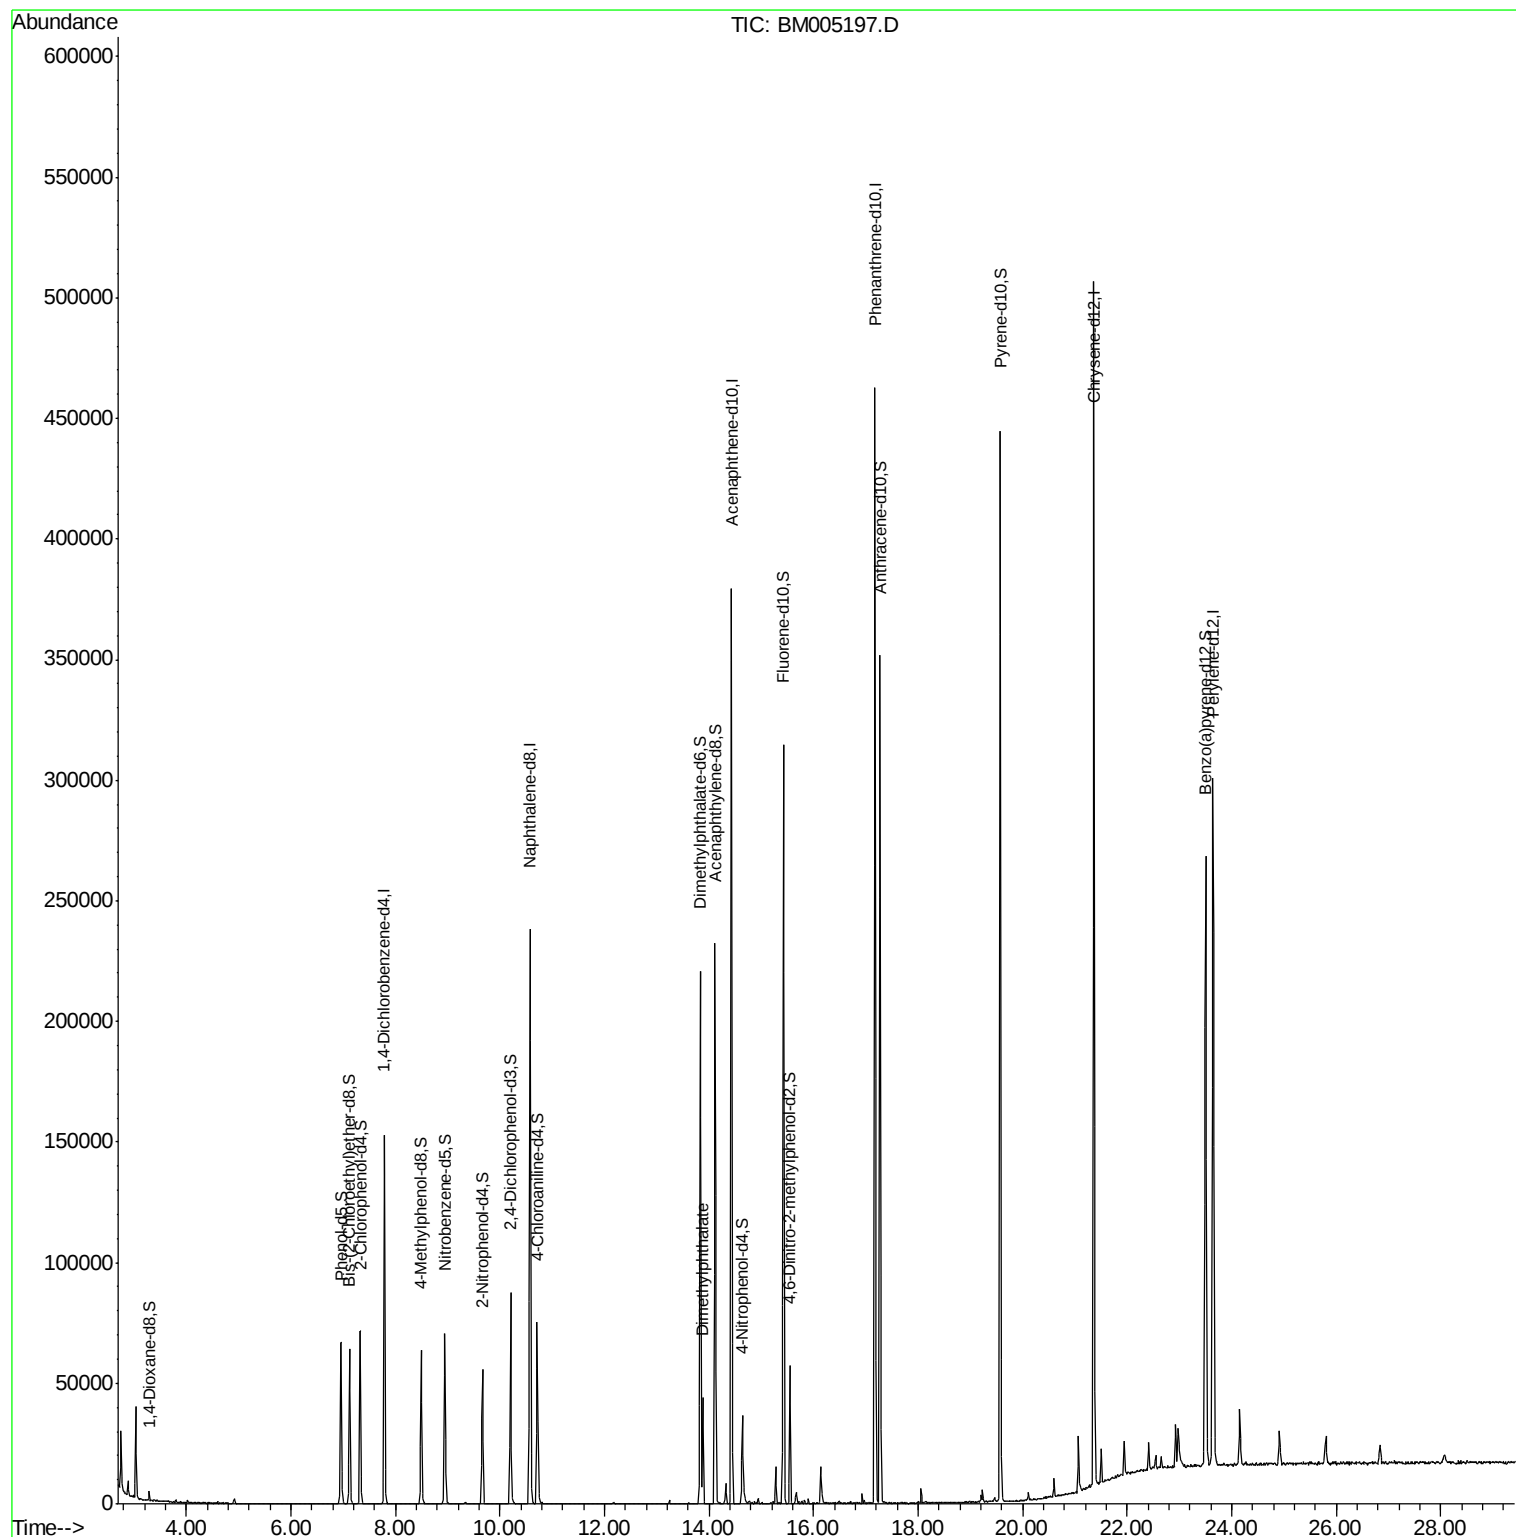

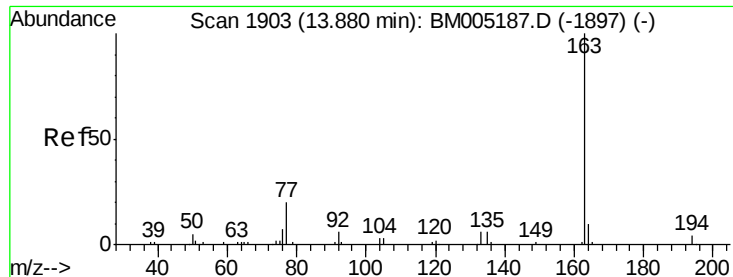

#44

Dimethylphthalate

Concen: 2.99 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. 0.00 min

Lab File: BM005197.D


Acq: 02 May 2016 17:45

Instrument :

BNA_M

ClientSampleId :

BD3A9

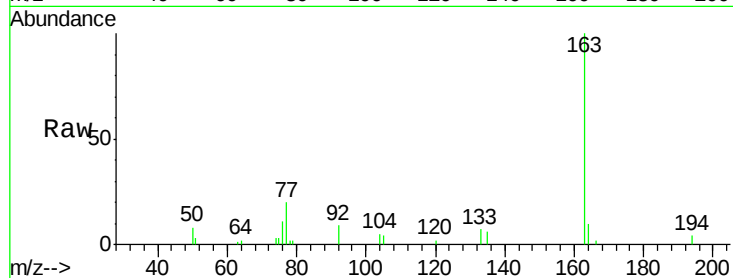

Tgt Ion:163 Resp: 30302

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.1 8.2 12.2

