

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005191.D
Acq On : 02 May 2016 14:08
Operator : UM/SJ
Sample : H2772-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD381

Manual Integrations
APPROVED

sohil
5/3/2016 6:32:56 PM

Quant Time: May 03 03:48:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
Qlast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

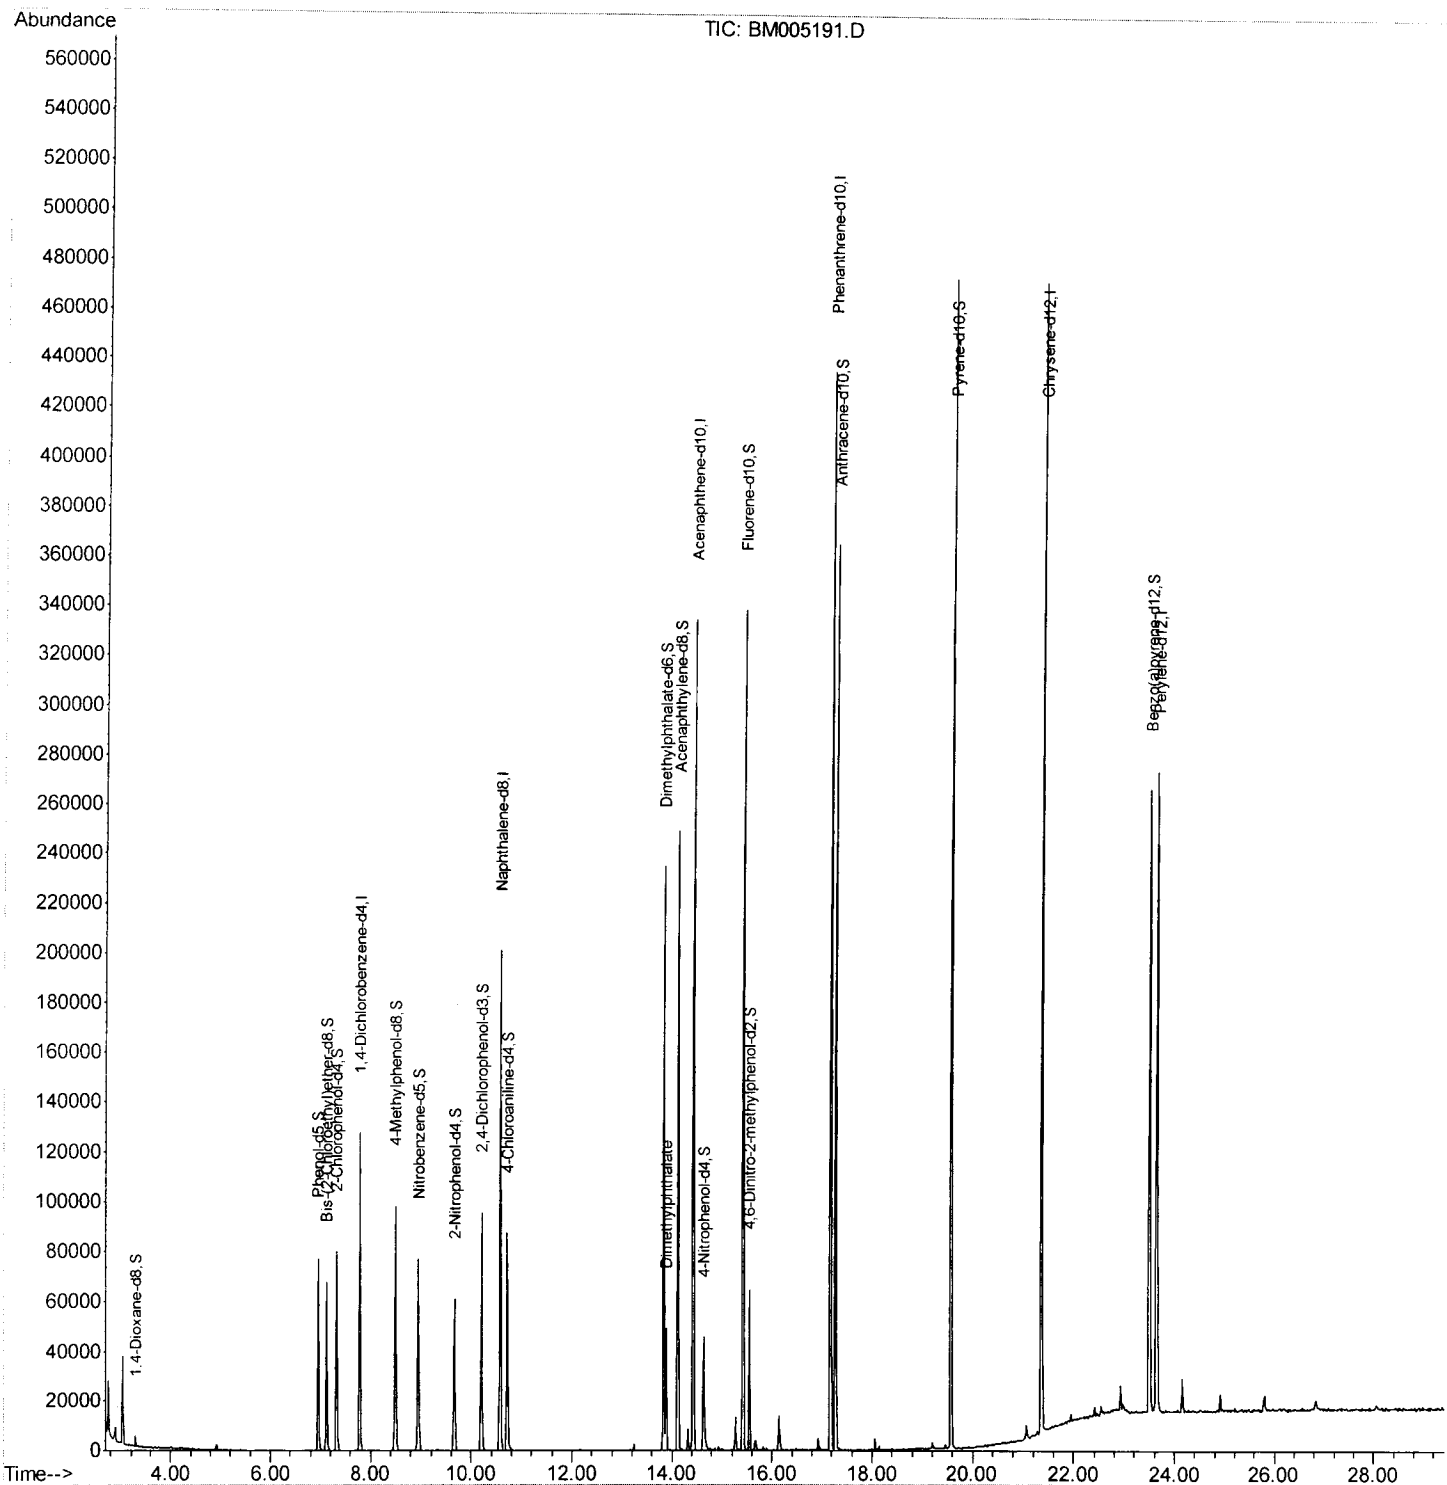

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005191.D
 Acq On : 02 May 2016 14:08
 Operator : UM/SJ
 Sample : H2772-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD381

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:32:56 PM

Quant Time: May 03 03:24:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

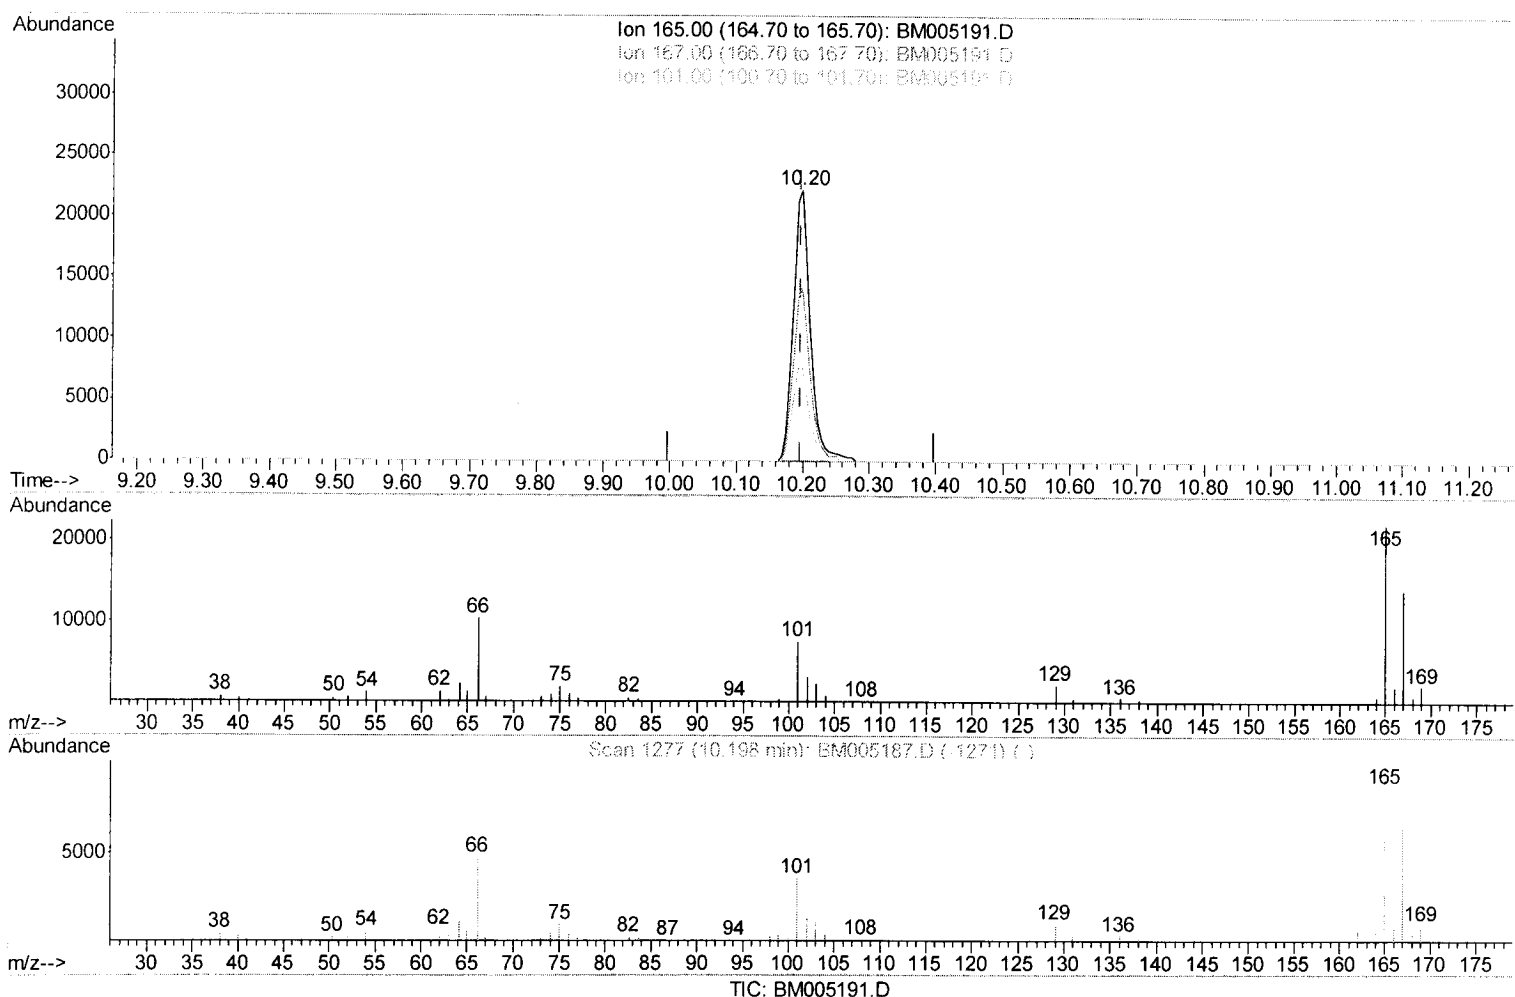

(26) 2,4-Dichlorophenol-d3 (S)

10.198min (+0.000) 15.64ng/ul m

response 39534

Ion	Exp%	Act%
165.00	100	100
167.00	65.90	64.21
101.00	34.10	34.67
0.00	0.00	0.00

UM
 05/04/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005191.D
Acq On : 02 May 2016 14:08
Operator : UM/SJ
Sample : H2772-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD381

Manual Integrations
APPROVED

sohil
5/3/2016 6:32:56 PM

Quant Time: May 03 03:24:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

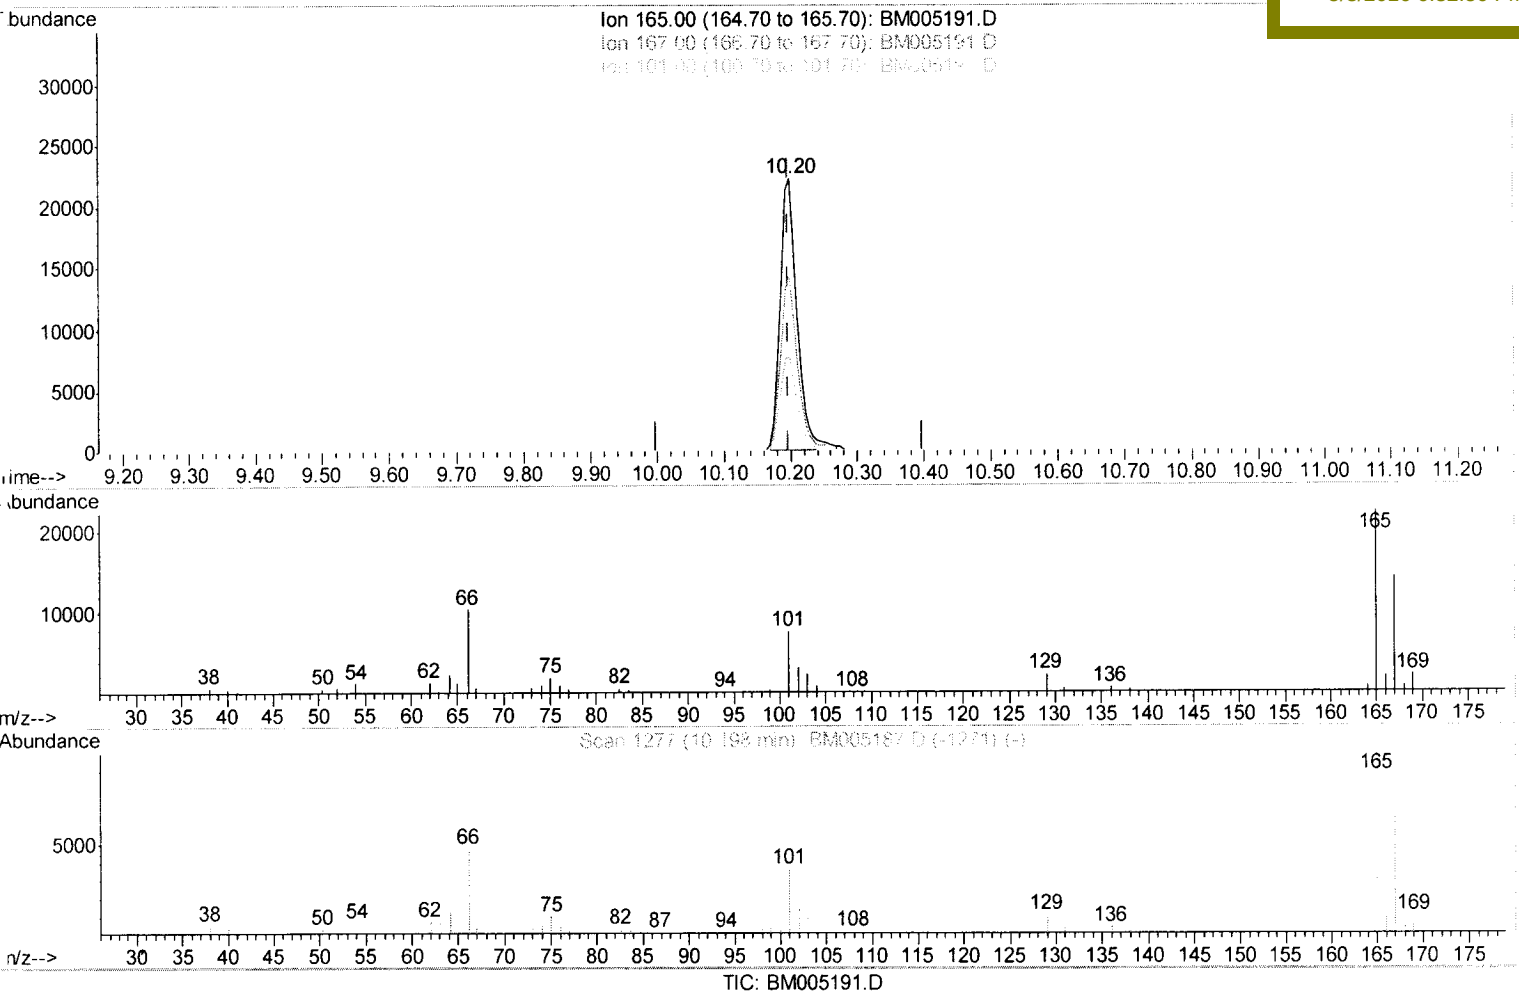

(26) 2,4-Dichlorophenol-d3 (S)

10.198min (+0.000) 15.60ng/ul

response 39426

Ion	Exp%	Act%
165.00	100	100
167.00	65.90	64.21
101.00	34.10	34.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005191.D
 Acq On : 02 May 2016 14:08
 Operator : UM/SJ
 Sample : H2772-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD381

Quant Time: May 03 03:48:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:32:56 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	35579	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	172147	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	112486	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	253088	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	226305	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	192586	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	2216	3.17	ng/uL	0.00
5) Phenol-d5	6.95	99	48379	16.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	31697	18.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	39583	17.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	39058	15.65	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	18927	15.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	21159	15.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	39534m	15.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	53501	18.06	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	156119	17.57	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	177200	16.75	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	15721	10.12	ng/ul	0.00
57) Fluorene-d10	15.42	176	137412	17.60	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	14560	10.11	ng/ul	0.00
70) Anthracene-d10	17.27	188	217483	19.16	ng/ul	0.00
76) Pyrene-d10	19.57	212	242504	23.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	177979	20.63	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	13.88	163	33636	3.78	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 05/04/16