

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005194.D
 Acq On : 02 May 2016 15:56
 Operator : UM/SJ
 Sample : H2772-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3E0

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:33:18 PM

Quant Time: May 03 04:02:35 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

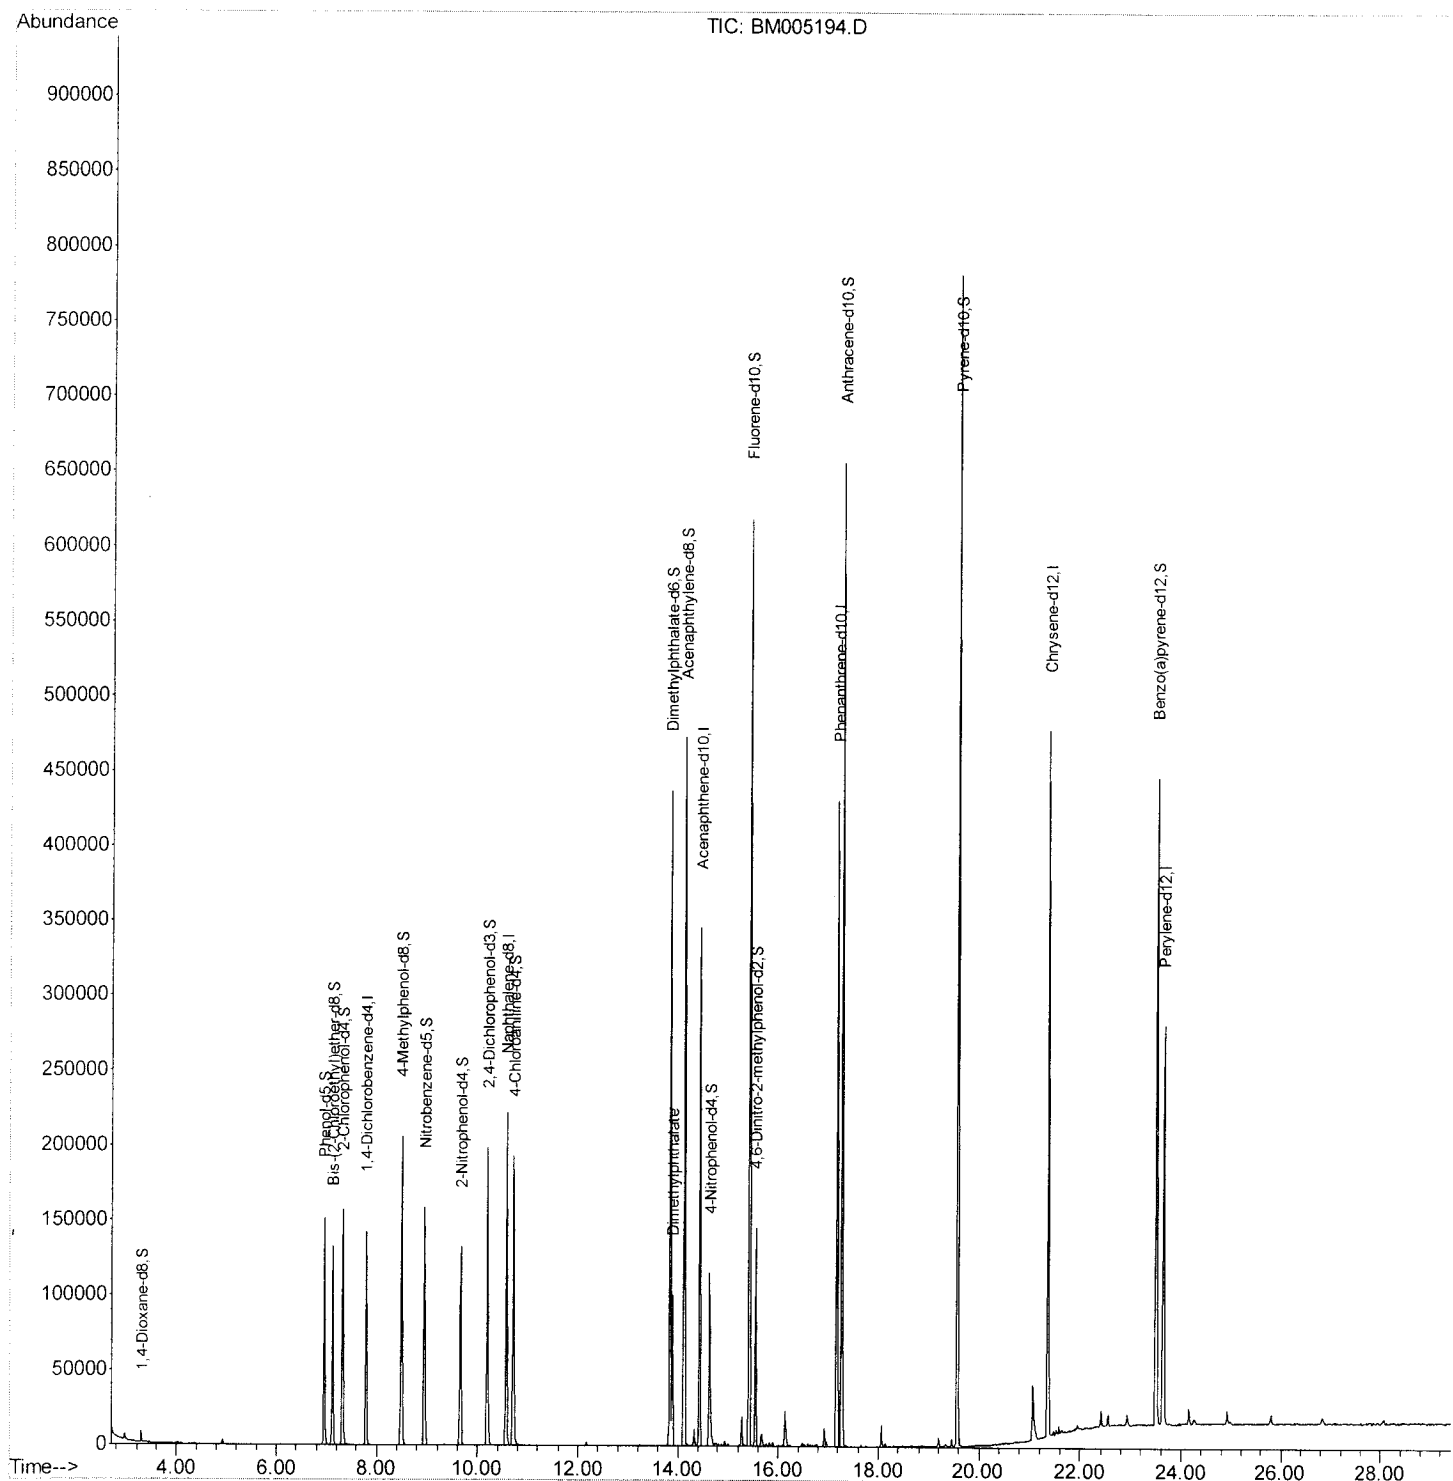

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005194.D
 Acq On : 02 May 2016 15:56
 Operator : UM/SJ
 Sample : H2772-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3E0

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:33:18 PM

Quant Time: May 03 03:24:53 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

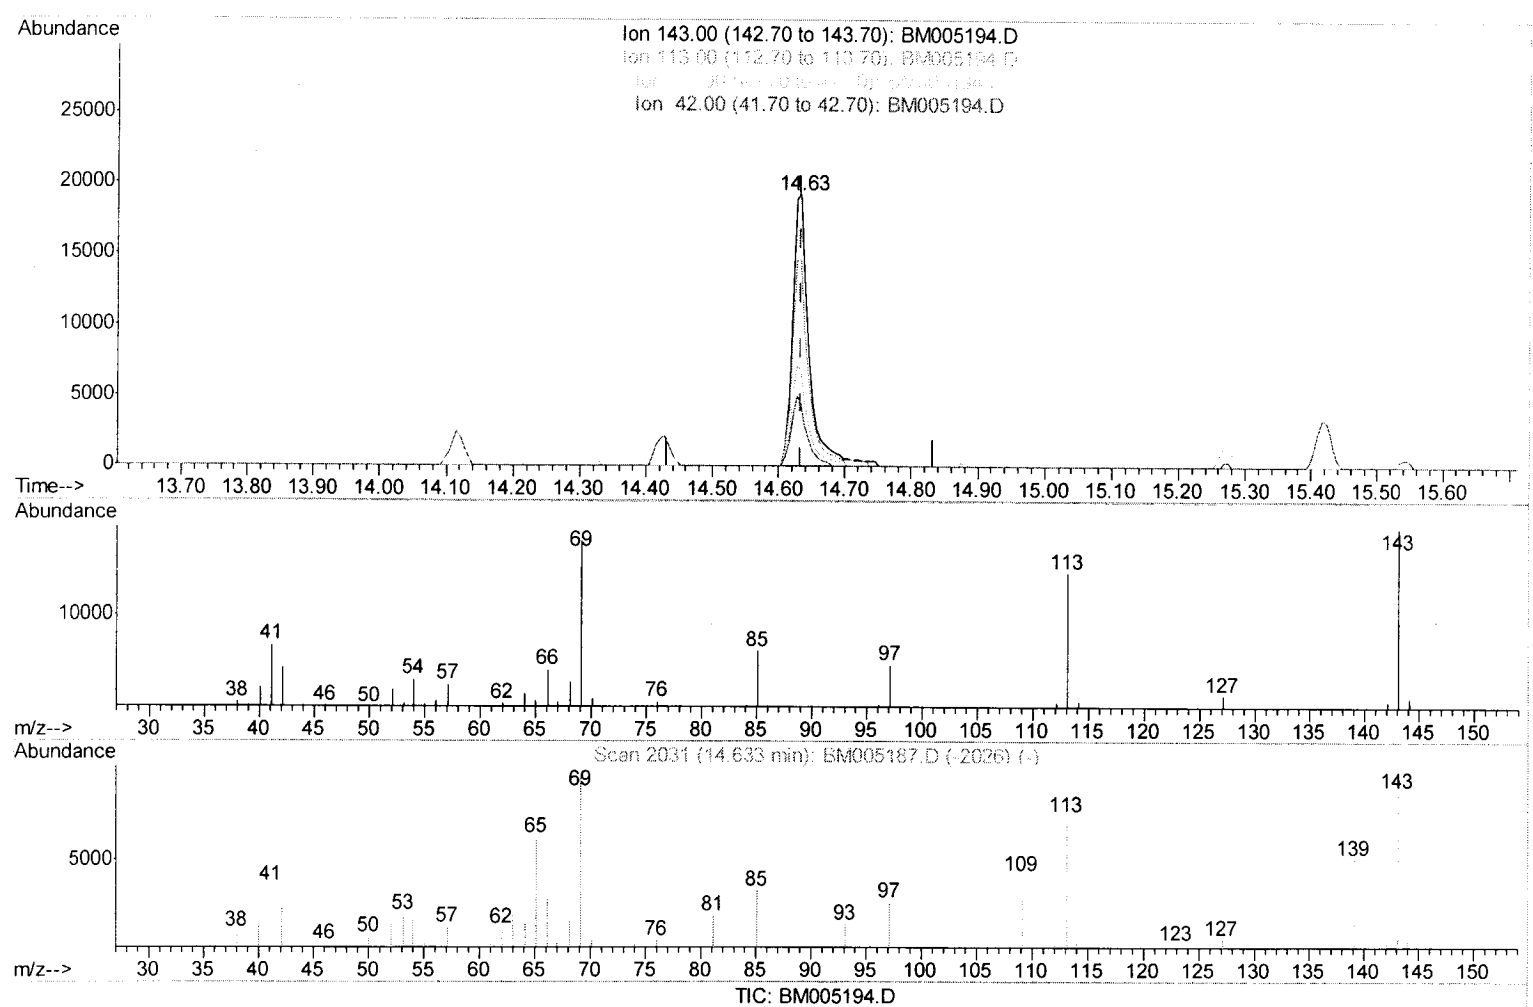

(51) 4-Nitrophenol-d4 (S)

14.633min (+0.000) 20.93ng/ul m

response 34031

Ion	Exp%	Act%
143.00	100	100
113.00	75.50	75.73
41.00	35.90	35.43
42.00	22.90	23.35

UM
 05/04/16


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005194.D
Acq On : 02 May 2016 15:56
Operator : UM/SJ
Sample : H2772-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3E0

Manual Integrations
APPROVED

sohil
5/3/2016 6:33:18 PM

Quant Time: May 03 03:24:53 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

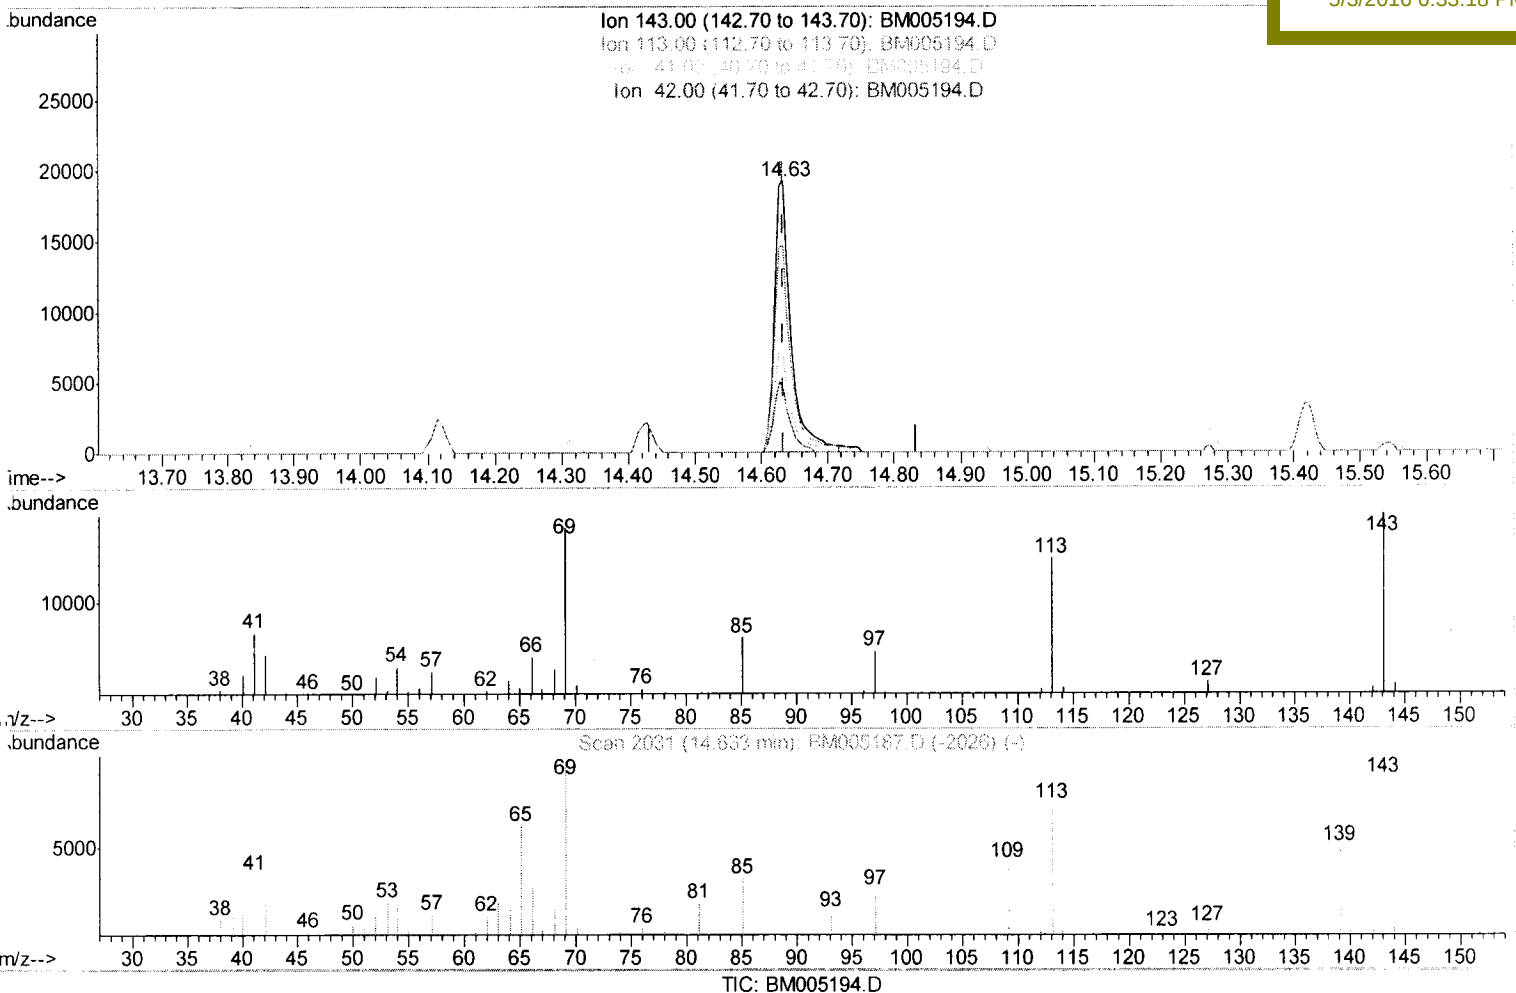

(51) 4-Nitrophenol-d4 (S)

14.633min (+0.000) 20.52ng/ul

response 33362

Ion	Exp%	Act%
143.00	100	100
113.00	75.50	75.73
41.00	35.90	35.43
42.00	22.90	23.35

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005194.D
Acq On : 02 May 2016 15:56
Operator : UM/SJ
Sample : H2772-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3E0

Quant Time: May 03 04:02:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
5/3/2016 6:33:18 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	38695	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	188487	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	117768	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	258727	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	227996	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	197969	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	4028	5.29	ng/uL	0.00
5) Phenol-d5	6.95	99	94696	29.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	59992	32.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	76167	30.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	79488	29.29	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	39103	29.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	44401	30.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	79120	28.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	112776	34.78	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	290653	31.25	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	342882	30.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	34031m	20.93	ng/ul	0.00
57) Fluorene-d10	15.42	176	251752	30.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	30647	20.83	ng/ul	0.00
70) Anthracene-d10	17.27	188	388231	33.46	ng/ul	0.00
76) Pyrene-d10	19.57	212	404617	38.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	304414	34.32	ng/ul	0.00

UM
05/04/16

Target Compounds					Qvalue
44) Dimethylphthalate	13.88	163	64017	6.86 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed