

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005195.D
 Acq On : 02 May 2016 16:33
 Operator : UM/SJ
 Sample : H2772-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD384

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:33:41 PM

Quant Time: May 03 04:04:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

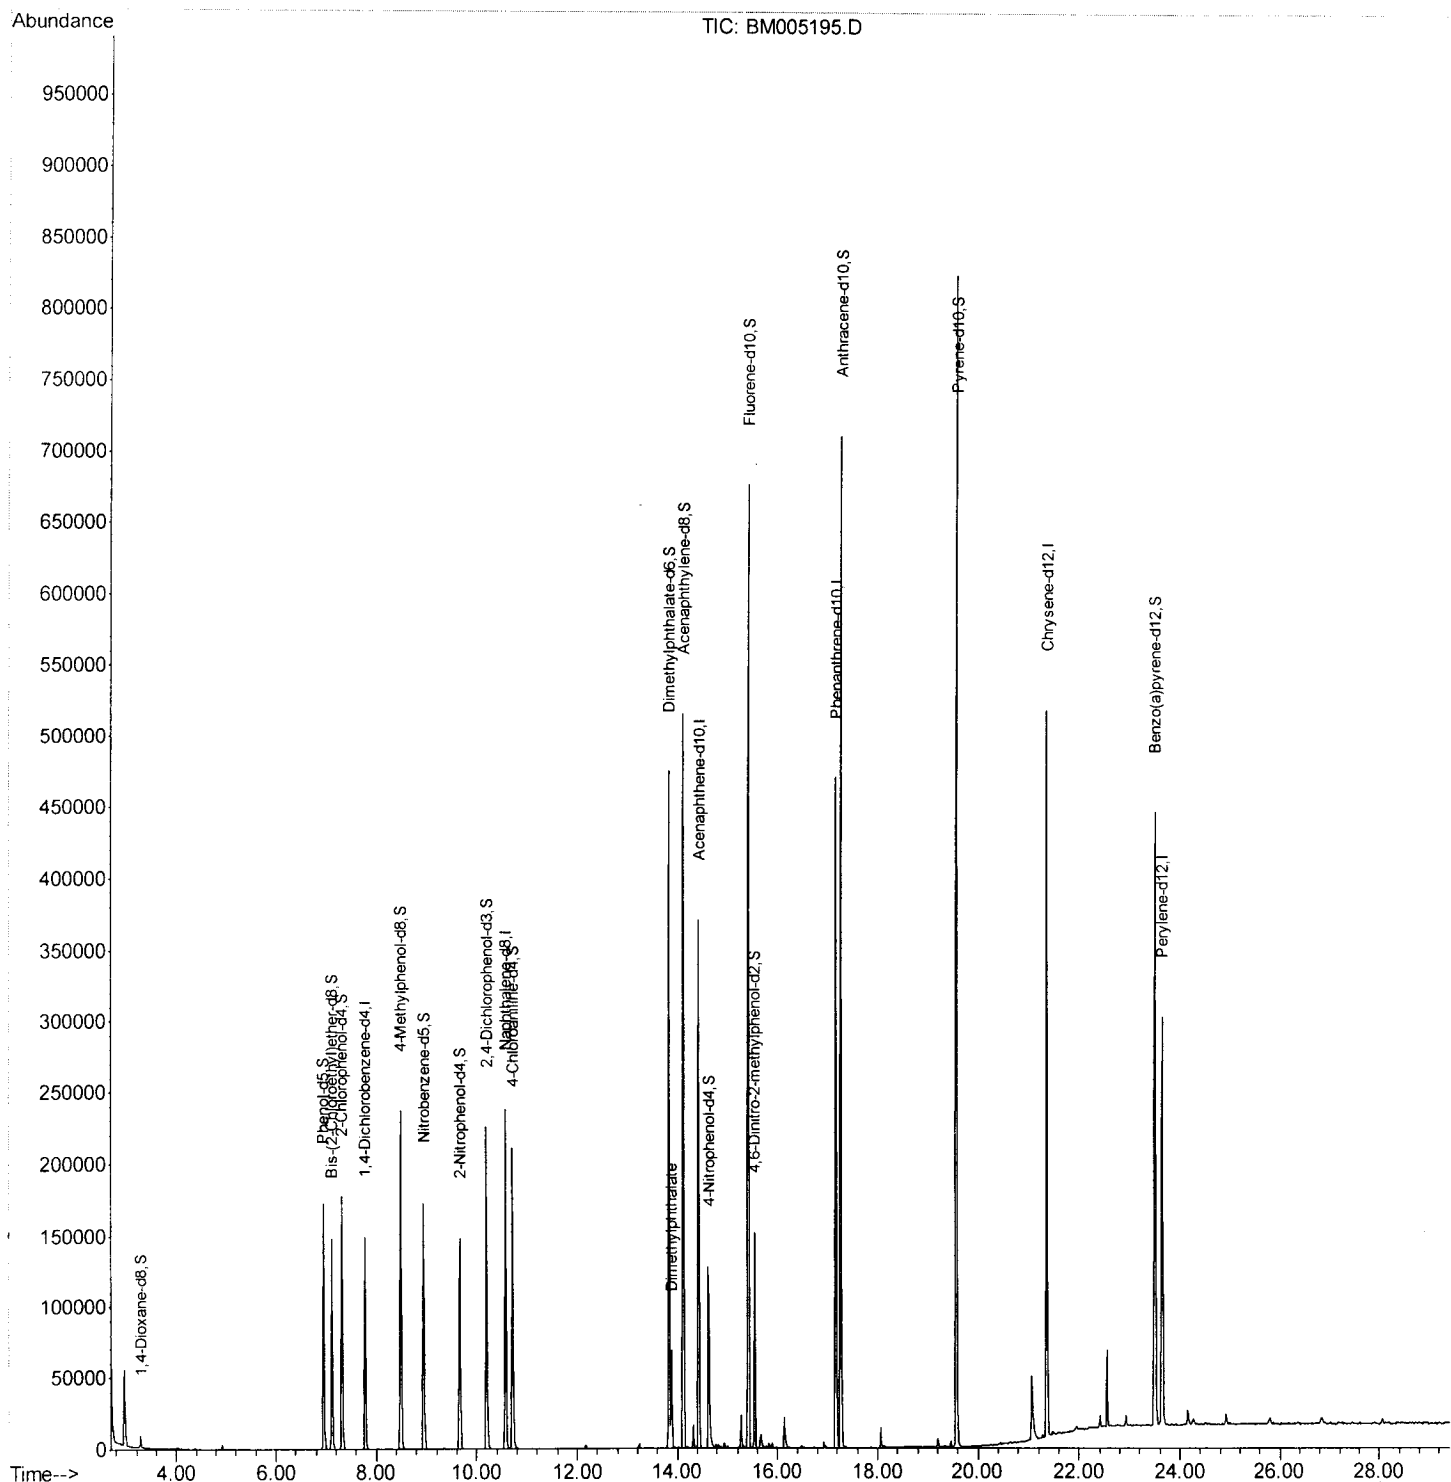

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005195.D
 Acq On : 02 May 2016 16:33
 Operator : UM/SJ
 Sample : H2772-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD384

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:33:41 PM

Quant Time: May 03 03:25:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

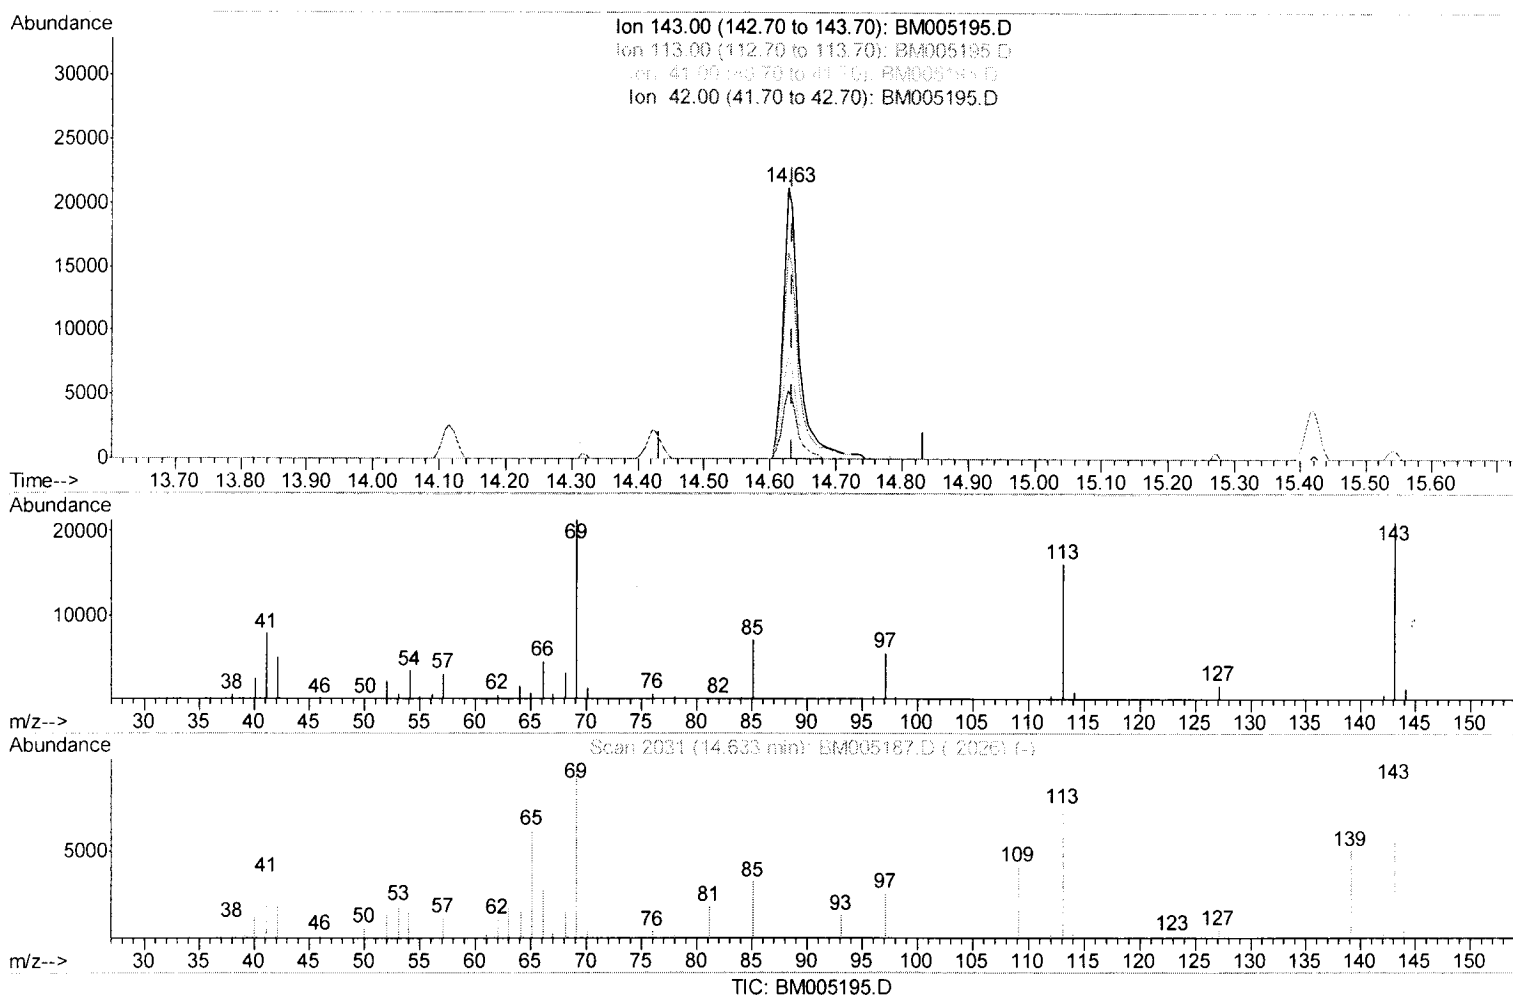

(51) 4-Nitrophenol-d4 (S)

14.627min (-0.006) 20.83ng/ul m

response 36100

Ion	Exp%	Act%
143.00	100	100
113.00	75.50	76.43
41.00	35.90	37.46
42.00	22.90	25.00

U.S.
 05/04/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005195.D
Acq On : 02 May 2016 16:33
Operator : UM/SJ
Sample : H2772-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD384

Manual Integrations
APPROVED

sohil
5/3/2016 6:33:41 PM

Quant Time: May 03 03:25:00 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

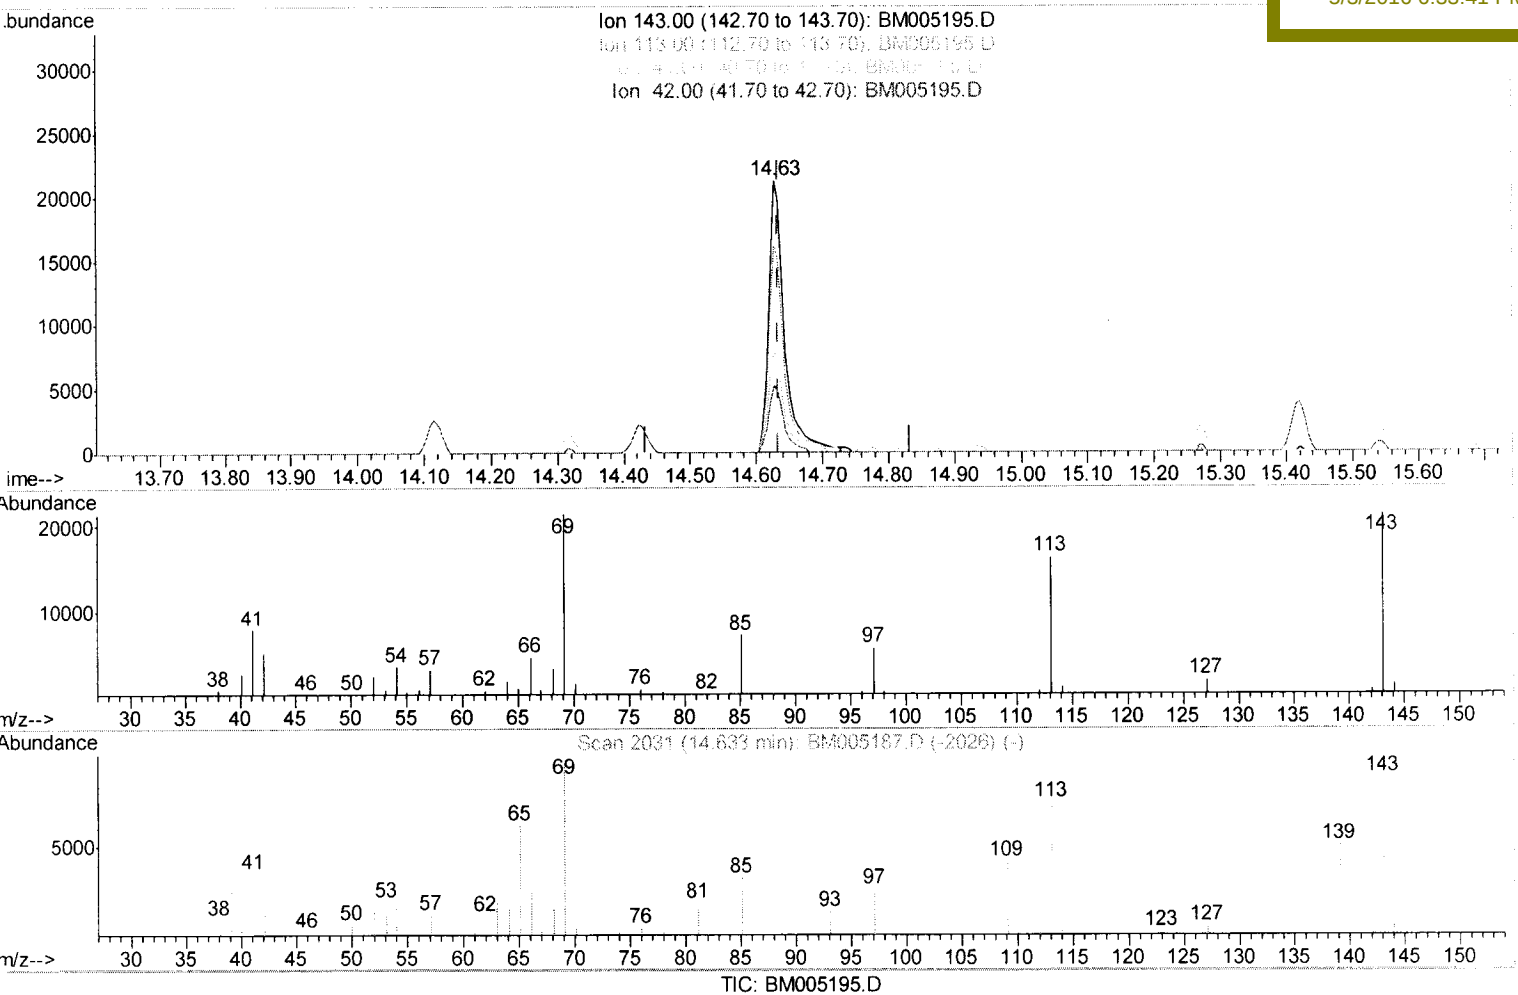

(51) 4-Nitrophenol-d4 (S)

14.627min (-0.006) 20.69ng/ul

response 35853

Ion	Exp%	Act%
143.00	100	100
113.00	75.50	76.43
41.00	35.90	37.46
42.00	22.90	25.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
 Data File : BM005195.D
 Acq On : 02 May 2016 16:33
 Operator : UM/SJ
 Sample : H2772-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD384

Quant Time: May 03 04:04:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:33:41 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	41082	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	198906	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	125547	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	281031	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	249844	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	214341	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	4726	5.85	ng/uL	0.00
5) Phenol-d5	6.95	99	107190	31.54	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.12	67	66955	34.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	85217	31.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	90724	31.49	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	43494	31.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	49652	32.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	88541	30.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	120827	35.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	313820	31.65	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	374090	31.68	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	36100m	20.83	ng/ul	0.00
57) Fluorene-d10	15.42	176	270210	31.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	32329	20.22	ng/ul	0.00
70) Anthracene-d10	17.27	188	414585	32.90	ng/ul	0.00
76) Pyrene-d10	19.57	212	432316	38.01	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	318876	33.20	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	13.88	163	45357	4.56 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

6.21
 05/04/16