

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005201.D
 Acq On : 02 May 2016 20:38
 Operator : UM/SJ
 Sample : H2772-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B2

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:34:23 PM

Quant Time: May 03 04:23:26 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	47774	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	237642	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	153649	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	348813	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	333045	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	269850	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	3701	3.94	ng/uL	0.00
5) Phenol-d5	6.95	99	91493	23.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	56607	25.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	72198	23.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	67263	20.08	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	36688	22.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	42488	23.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	76878	22.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	90585	22.16	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	275251	22.68	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	325609	22.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	34413m	16.22	ng/ul	0.00
57) Fluorene-d10	15.42	176	236959	22.22	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	33293	16.78	ng/ul	0.00
70) Anthracene-d10	17.27	188	361145	23.09	ng/ul	0.00
76) Pyrene-d10	19.57	212	402615	26.55	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	290110	23.99	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.88	163	60503	4.97	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005201.D
Acq On : 02 May 2016 20:38
Operator : UM/SJ
Sample : H2772-13
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BD3B2

Manual Integrations
APPROVED

sohil
5/3/2016 6:34:23 PM

Quant Time: May 03 04:23:26 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

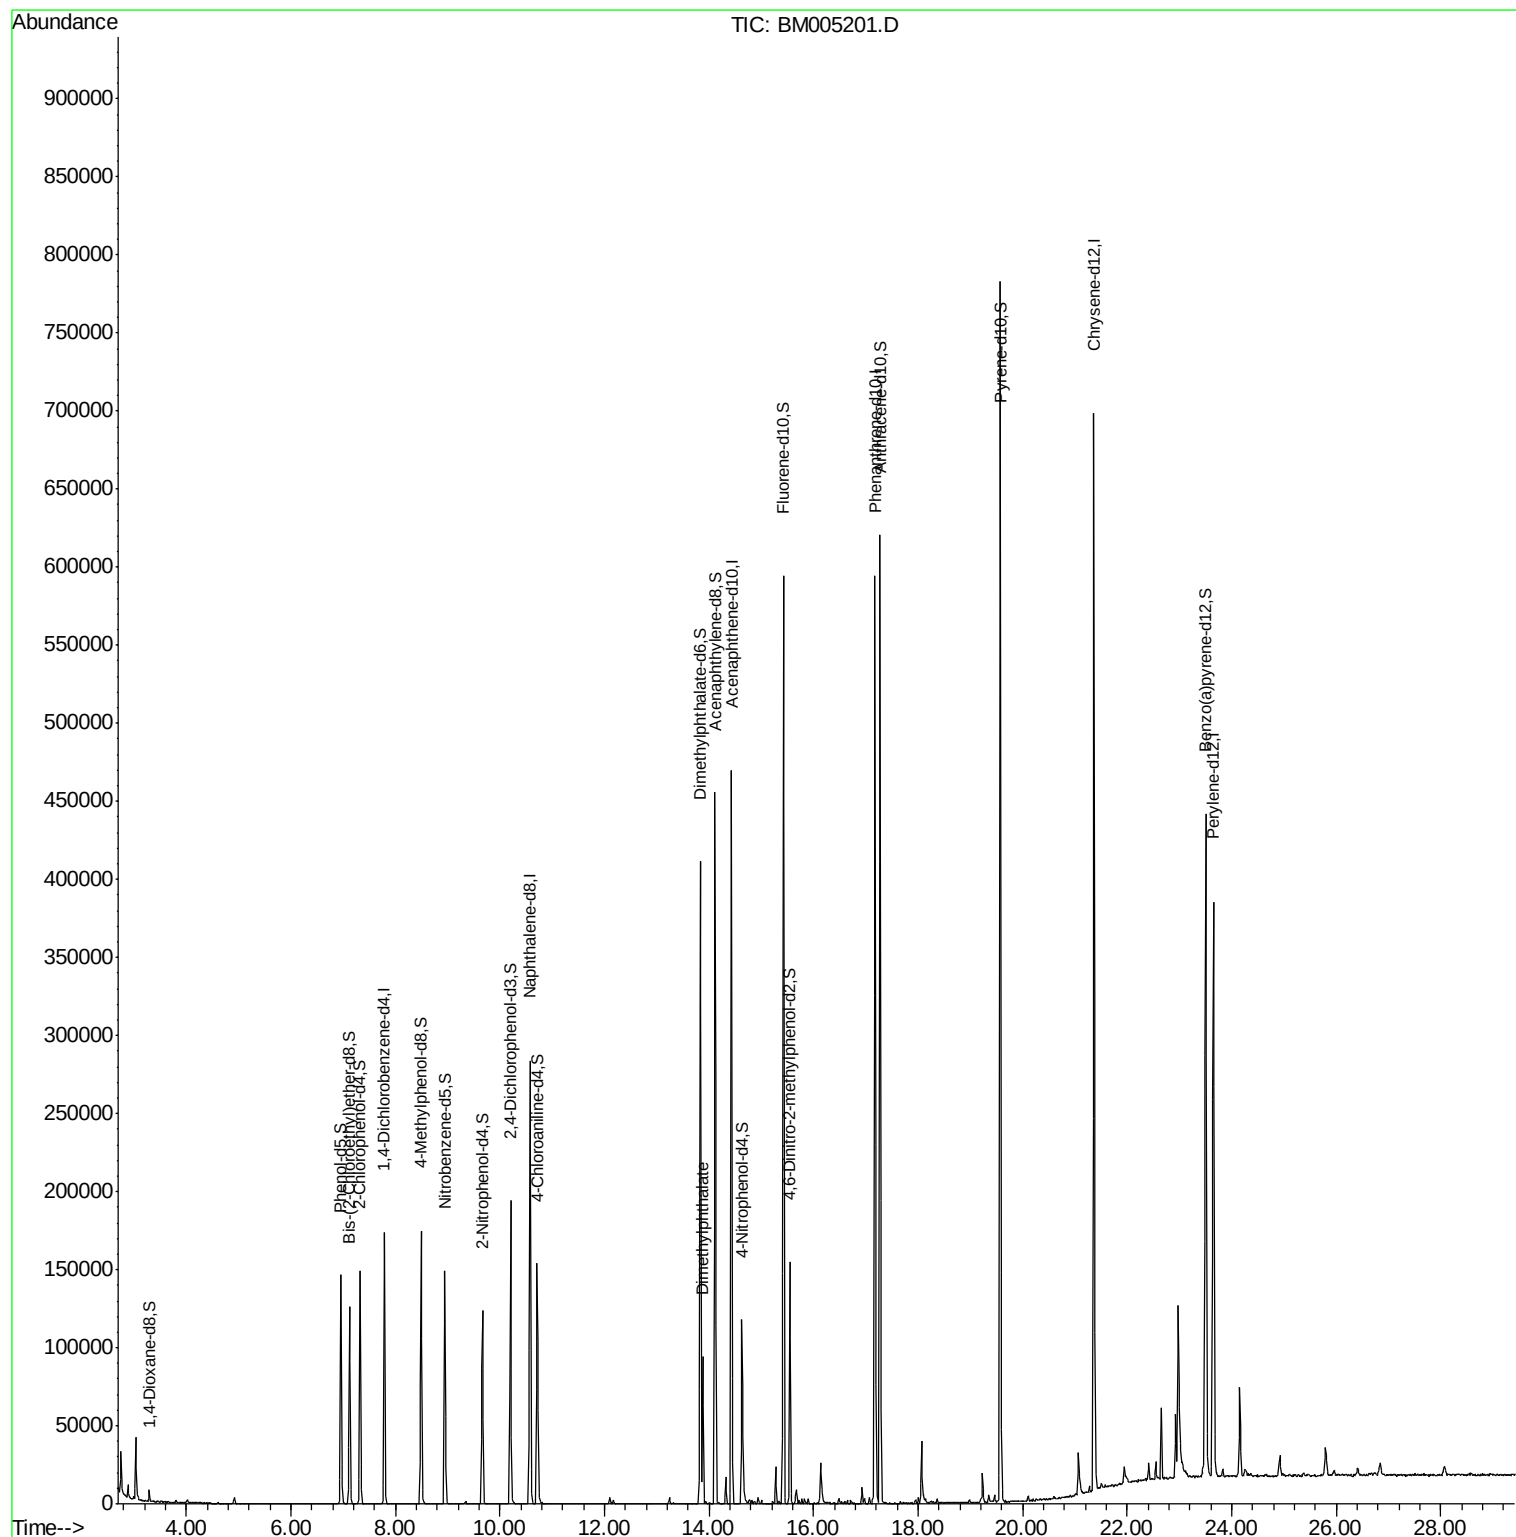

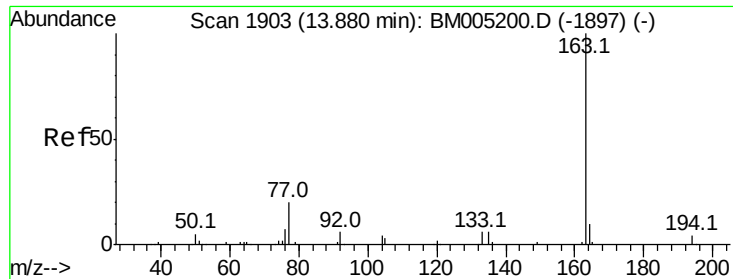

#44

Dimethylphthalate

Concen: 4.97 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. 0.00 min

Lab File: BM005201.D


Acq: 02 May 2016 20:38

Instrument :

BNA_M

ClientSampleId :

BD3B2

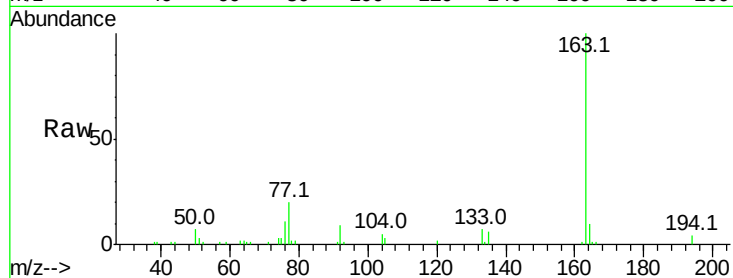

Tot Ion:	163	Resp:	60503
Ion Ratio	Lower	Upper	
163	100		
194	4.3	3.3	4.9
164	10.2	8.2	12.2

Manual Integrations
APPROVED

sohil
5/3/2016 6:34:23 PM

