

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005202.D
 Acq On : 02 May 2016 21:14
 Operator : UM/SJ
 Sample : H2772-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B3

Quant Time: May 03 03:26:04 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	47427	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	225402	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	144285	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	335059	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	320317	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	258744	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	5217	5.59	ng/uL	0.00
5) Phenol-d5	6.96	99	130363	33.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	75032	33.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	100840	32.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	104206	31.33	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	49439	31.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	57186	32.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	103747	31.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	141346	36.45	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	350643	30.77	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	419366	30.90	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	46185	23.19	ng/ul	0.00
57) Fluorene-d10	15.42	176	301681	30.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	41252	21.65	ng/ul	0.00
70) Anthracene-d10	17.27	188	465496	30.98	ng/ul	0.00
76) Pyrene-d10	19.57	212	502800	34.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	365423	31.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.88	163	80196	7.02	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005202.D
Acq On : 02 May 2016 21:14
Operator : UM/SJ
Sample : H2772-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B3

Quant Time: May 03 03:26:04 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

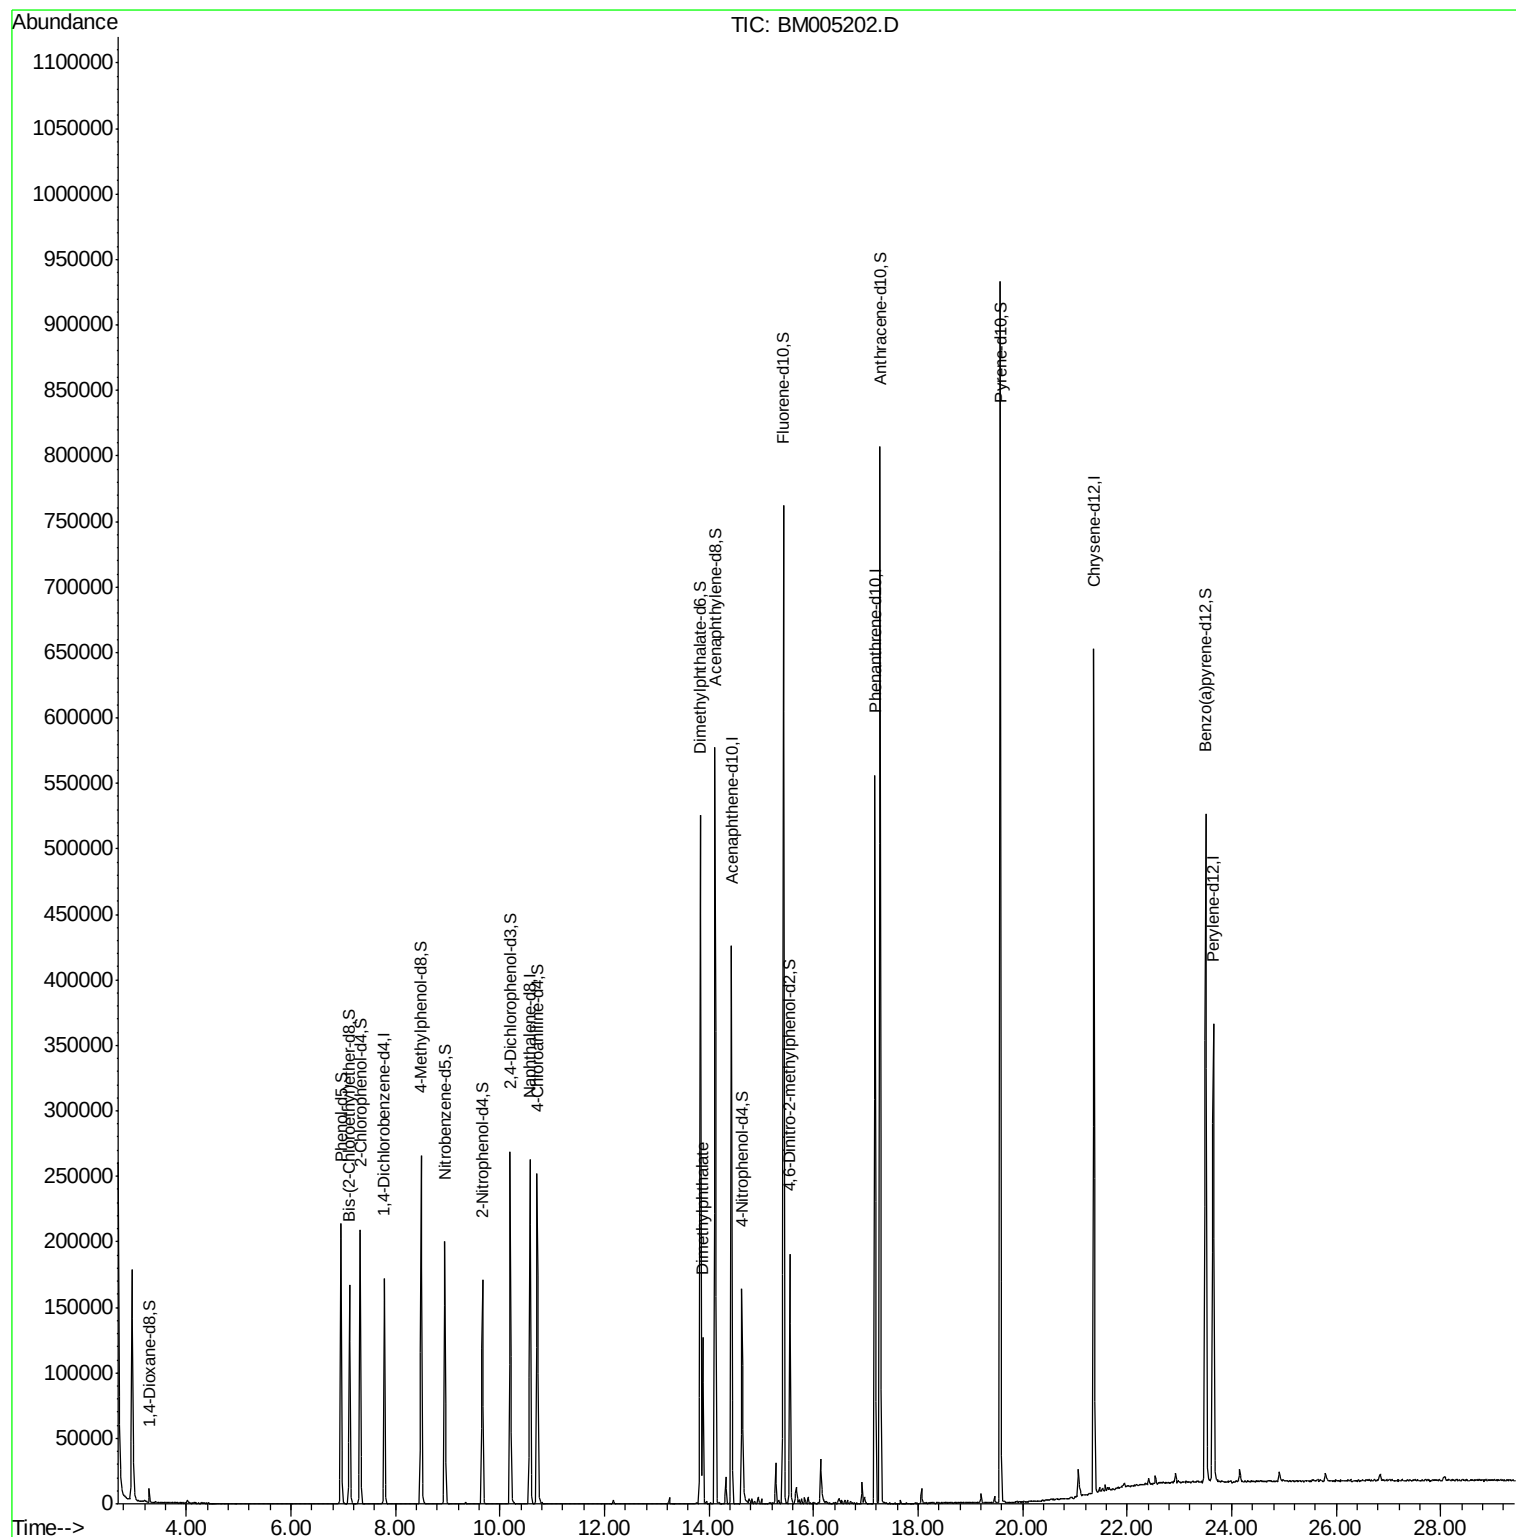

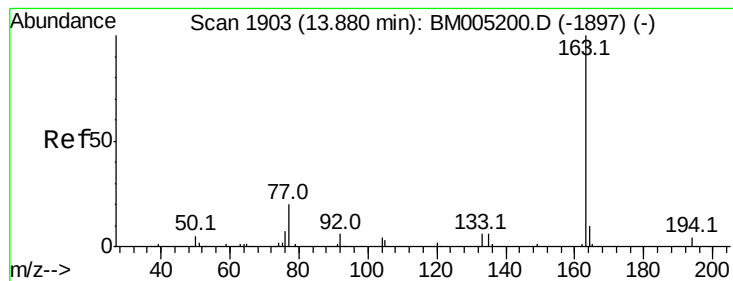

#44

Dimethylphthalate

Concen: 7.02 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. -0.00 min

Lab File: BM005202.D

Acq: 02 May 2016 21:14

Instrument :

BNA_M

ClientSampleId :

BD3B3


Tot Ion:163 Resp: 80196

Ion Ratio Lower Upper

163 100

194 4.1 3.3 4.9

164 9.8 8.2 12.2

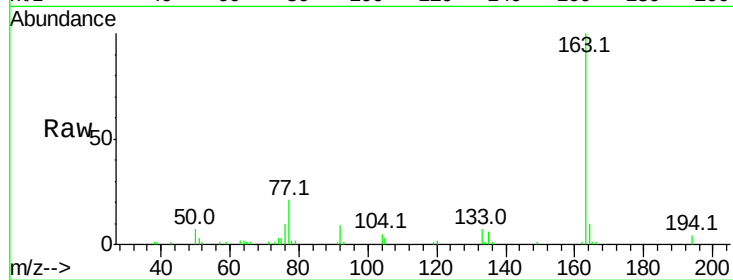

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

