

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005208.D
 Acq On : 03 May 2016 00:52
 Operator : UM/SJ
 Sample : H2772-22
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C6

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:35:03 PM

Quant Time: May 03 04:51:57 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	46100	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	221917	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	137249	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	307753	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	281005	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	227607	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	4933	5.44	ng/uL	0.00
5) Phenol-d5	6.95	99	111099	29.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	70334	32.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	89909	29.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	94671	29.28	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	46728	30.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	54213	31.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	93011	28.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	126825	33.22	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	324302	29.92	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	392112	30.38	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	41637m	21.98	ng/ul	0.00
57) Fluorene-d10	15.42	176	279901	29.39	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	37970	21.69	ng/ul	0.00
70) Anthracene-d10	17.27	188	423770	30.71	ng/ul	0.00
76) Pyrene-d10	19.57	212	449625	35.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.49	264	322352	31.61	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.88	163	46642	4.29	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005208.D
Acq On : 03 May 2016 00:52
Operator : UM/SJ
Sample : H2772-22
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BD3C6

Manual Integrations
APPROVED

sohil
5/3/2016 6:35:03 PM

Quant Time: May 03 04:51:57 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

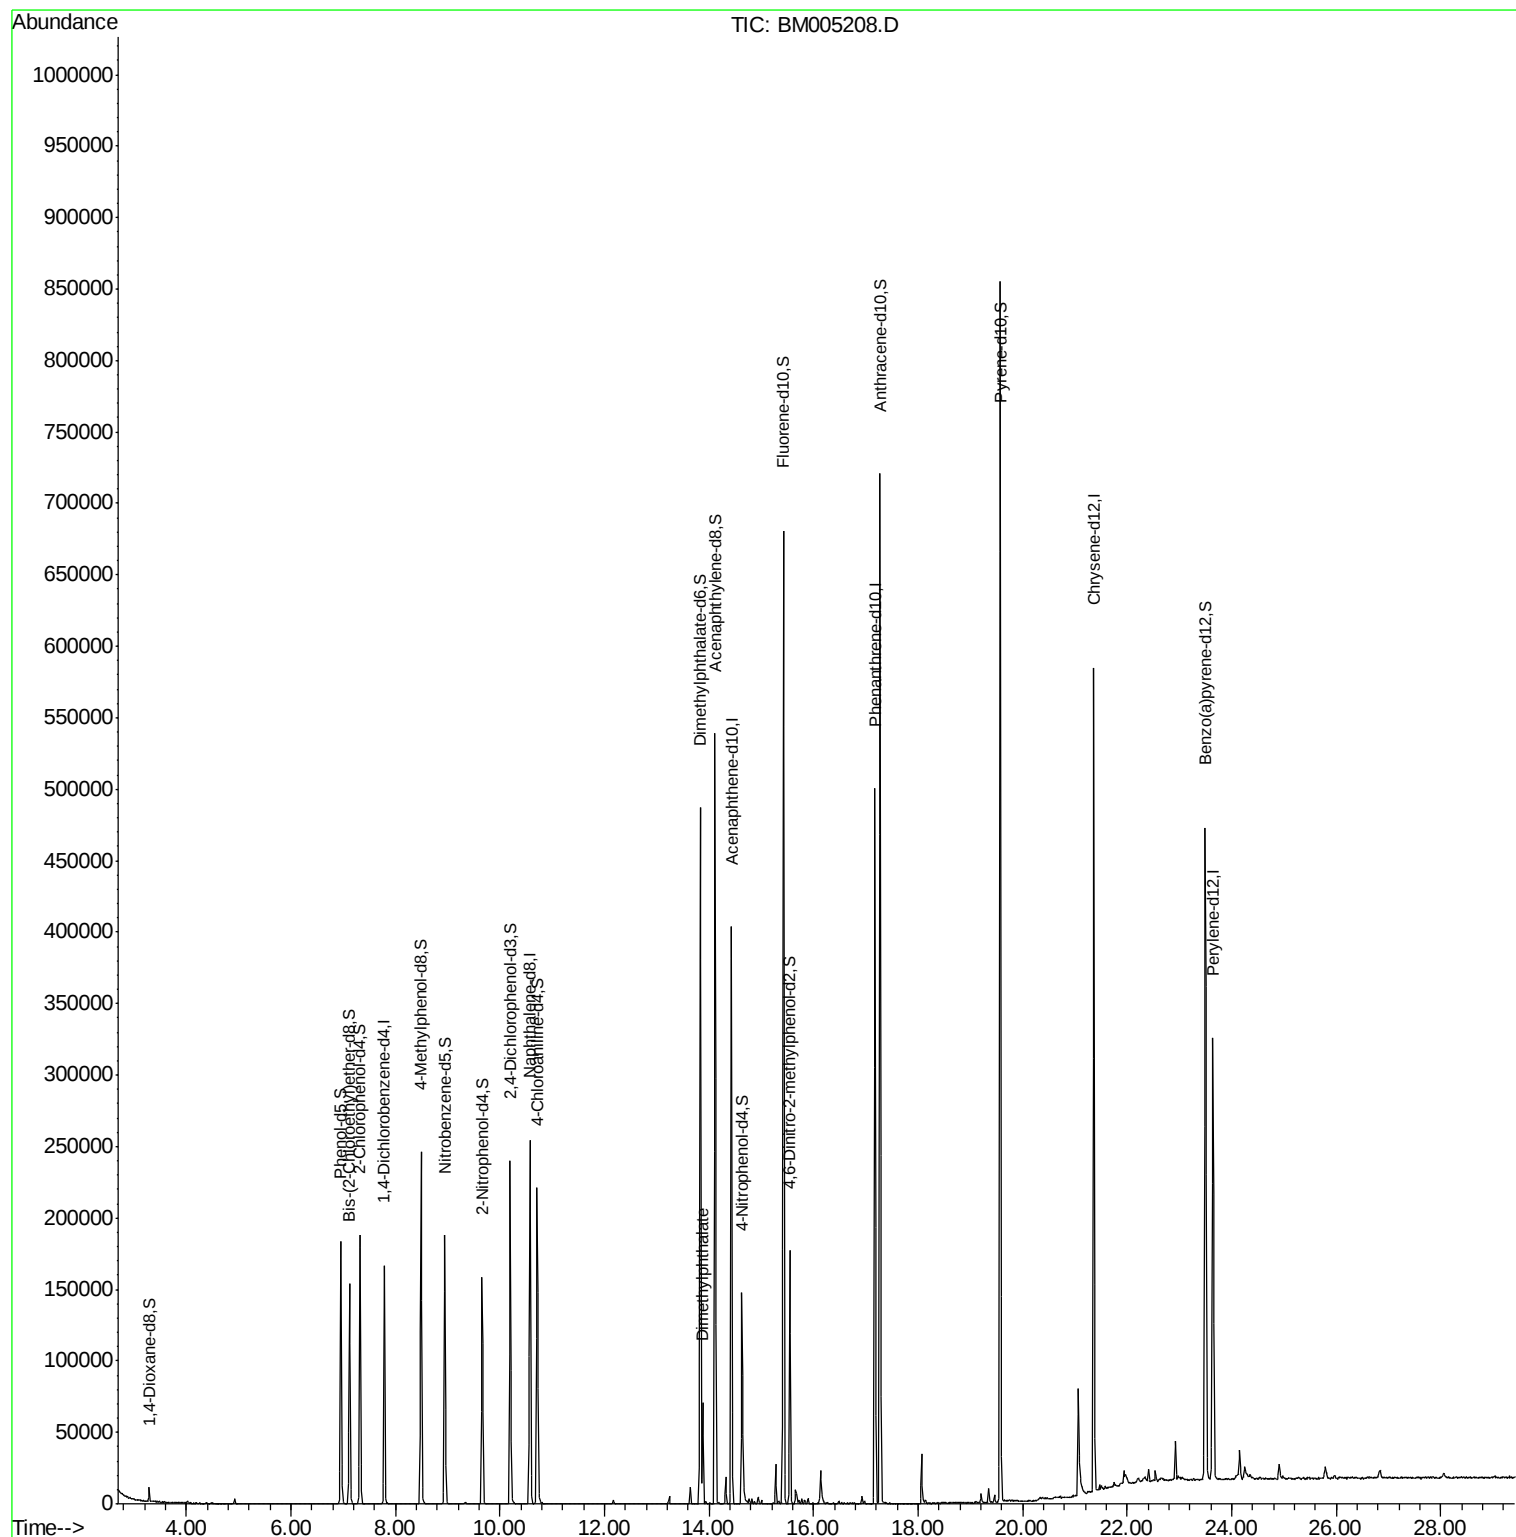

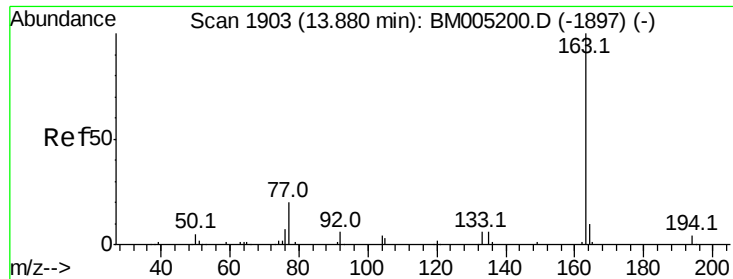

#44
 Dimethylphthalate
 Concen: 4.29 ng/ul
 RT: 13.88 min Scan# 1903
 Delta R.T. 0.00 min
 Lab File: BM005208.D
 Acq: 03 May 2016 00:52

Instrument :
 BNA_M
 ClientSampleId :
 BD3C6

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.1	3.3	4.9
164	10.3	8.2	12.2

Manual Integrations
 APPROVED

sohil
 5/3/2016 6:35:03 PM

