

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005209.D
 Acq On : 03 May 2016 01:29
 Operator : UM/SJ
 Sample : H2772-23
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C7

Quant Time: May 03 04:57:05 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 03 03:20:39 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	49202	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	235597	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	146481	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	330702	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	304191	20.00	ng/ul	0.00
83) Perylene-d12	23.64	264	247633	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	5625	5.81	ng/uL	0.00
5) Phenol-d5	6.95	99	126972	31.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	80151	34.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	102712	31.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	109887	31.85	ng/ul	0.00
19) Nitrobenzene-d5	8.94	128	54332	33.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	62502	34.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.19	165	107266	31.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.71	131	148994	36.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.83	166	381547	32.98	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	452945	32.88	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	46000	22.75	ng/ul	0.00
57) Fluorene-d10	15.42	176	324065	31.88	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	42250	22.46	ng/ul	0.00
70) Anthracene-d10	17.27	188	494318	33.33	ng/ul	0.00
76) Pyrene-d10	19.57	212	531464	38.38	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	388518	35.02	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.88	163	54750	4.72	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005209.D
Acq On : 03 May 2016 01:29
Operator : UM/SJ
Sample : H2772-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C7

Quant Time: May 03 04:57:05 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 03 03:20:39 2016
Response via : Initial Calibration

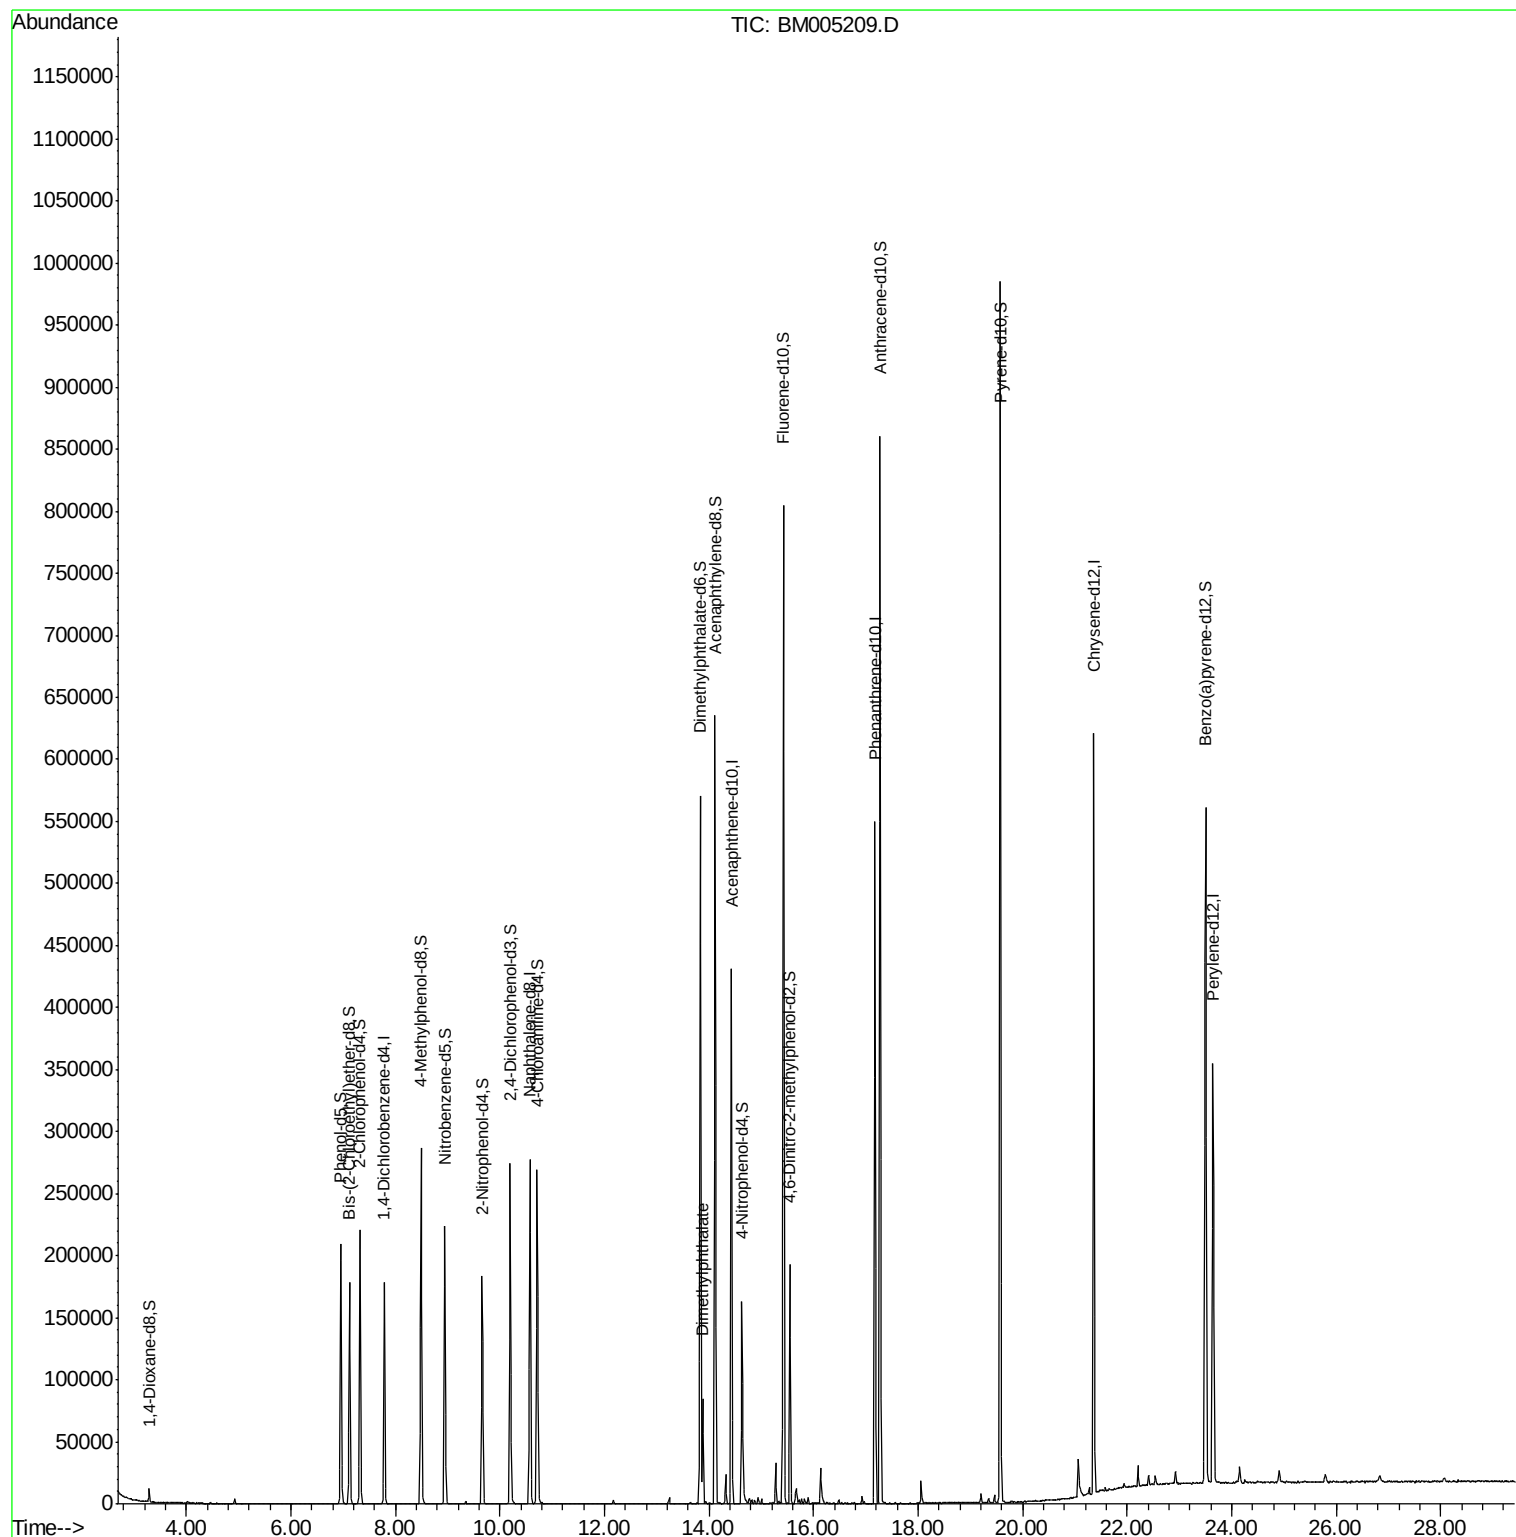

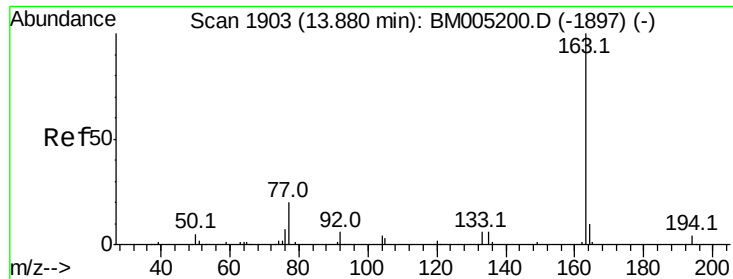

#44

Dimethylphthalate

Concen: 4.72 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. 0.00 min

Lab File: BM005209.D

Acq: 03 May 2016 01:29

Instrument :

BNA_M

ClientSampleId :

BD3C7


Tot Ion:163 Resp: 54750

Ion Ratio Lower Upper

163 100

194 3.8 3.3 4.9

164 10.0 8.2 12.2

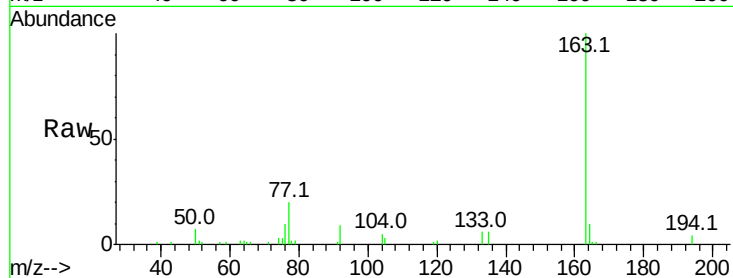

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

