

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005198.D
 Acq On : 02 May 2016 18:22
 Operator : UM/SJ
 Sample : H2772-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.957	41	46	56	rVB	36786	60024	8.26%	0.730%
2	3.287	99	102	108	rVB	6012	7369	1.01%	0.090%
3	6.951	720	725	739	rBB	107817	169323	23.30%	2.059%
4	7.122	748	754	764	rBB	96926	152009	20.92%	1.849%
5	7.316	782	787	797	rBB	113143	179964	24.77%	2.189%
6	7.787	861	867	876	rBB	129718	200747	27.63%	2.442%
7	8.487	981	986	998	rBB	148026	233689	32.16%	2.842%
8	8.939	1058	1063	1076	rBB	114085	185473	25.53%	2.256%
9	9.663	1180	1186	1194	rBB	89142	145484	20.02%	1.769%
10	10.198	1271	1277	1291	rBB	138329	234069	32.21%	2.847%
11	10.575	1334	1341	1350	rBB	205297	350189	48.19%	4.259%
12	10.710	1359	1364	1384	rBB	123506	217025	29.87%	2.640%
13	13.833	1889	1895	1899	rBV	315023	420923	57.93%	5.120%
14	13.880	1899	1903	1909	rVB	66689	90997	12.52%	1.107%
15	14.116	1937	1943	1960	rBB	348243	509818	70.16%	6.201%
16	14.316	1973	1977	1981	rBB	14640	16674	2.29%	0.203%
17	14.427	1989	1996	2003	rBB2	335148	508802	70.02%	6.188%
18	14.633	2026	2031	2045	rBV	44065	77744	10.70%	0.946%
19	15.004	2086	2094	2103	rBV2	4932	14868	2.05%	0.181%
20	15.268	2135	2139	2144	rBB	24821	30216	4.16%	0.368%
21	15.421	2159	2165	2174	rVB	461761	661580	91.05%	8.047%
22	15.545	2181	2186	2193	rBV	55409	76087	10.47%	0.925%
23	15.657	2202	2205	2213	rBV3	7248	16256	2.24%	0.198%
24	16.133	2282	2286	2299	rBV	23855	39640	5.46%	0.482%
25	17.174	2457	2463	2471	rBV	411119	587829	80.90%	7.150%
26	17.268	2473	2479	2491	rVV	457732	678314	93.35%	8.250%
27	19.568	2864	2870	2884	rVB	535525	726629	100.00%	8.838%
28	21.062	3120	3124	3132	rBV2	18522	31047	4.27%	0.378%
29	21.362	3170	3175	3185	rBV	445282	555957	76.51%	6.762%
30	22.927	3437	3441	3445	rVB2	7933	10823	1.49%	0.132%
31	23.497	3531	3538	3550	rVB2	294094	540168	74.34%	6.570%
32	23.644	3556	3563	3577	rVB2	241894	475624	65.46%	5.785%
33	24.156	3646	3650	3658	rVB2	9927	16470	2.27%	0.200%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005198.D
Acq On : 02 May 2016 18:22
Operator : UM/SJ
Sample : H2772-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Title : SVOA CALIBRATION


Sum of corrected areas: 8221831

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005198.D
Acq On : 02 May 2016 18:22
Operator : UM/SJ
Sample : H2772-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BD3B0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

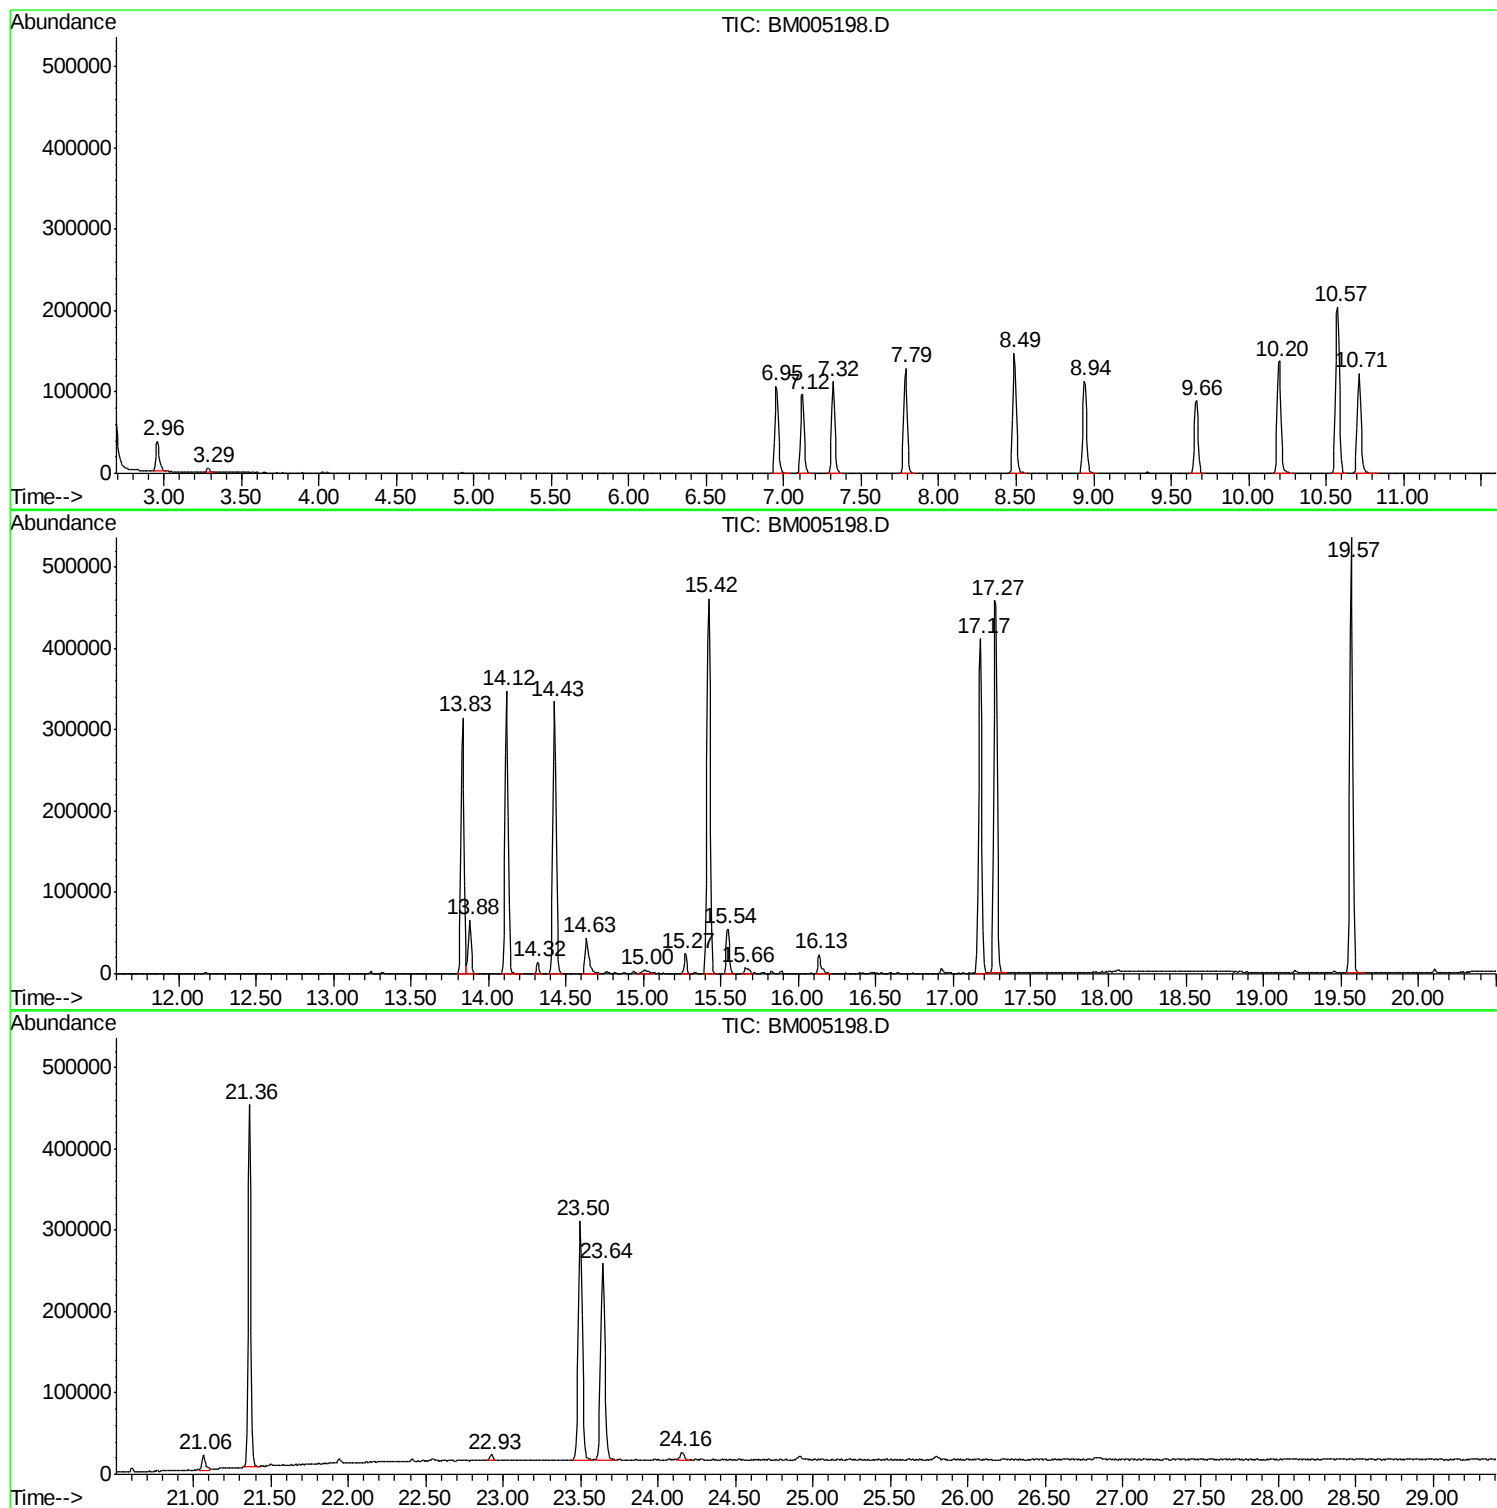

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005198.D
Acq On : 02 May 2016 18:22
Operator : UM/SJ
Sample : H2772-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005198.D
Acq On : 02 May 2016 18:22
Operator : UM/SJ
Sample : H2772-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc