

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005206.D
 Acq On : 02 May 2016 23:40
 Operator : UM/SJ
 Sample : H2772-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3B7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	99	102	109	rVB	9367	11274	1.06%	0.093%
2	6.951	720	725	742	rBB	180970	291567	27.29%	2.396%
3	7.122	748	754	765	rBB	151942	237227	22.21%	1.949%
4	7.316	782	787	799	rBB	184694	296374	27.74%	2.435%
5	7.786	861	867	876	rBB	184187	293093	27.44%	2.408%
6	8.486	980	986	1001	rBB	244673	385684	36.10%	3.169%
7	8.939	1057	1063	1073	rBV	180218	296294	27.74%	2.435%
8	9.657	1180	1185	1193	rBV	152048	247296	23.15%	2.032%
9	10.192	1271	1276	1290	rBV	231409	392247	36.72%	3.223%
10	10.574	1334	1341	1351	rBB	285695	479264	44.86%	3.938%
11	10.710	1358	1364	1379	rBV	239601	421526	39.46%	3.464%
12	13.833	1889	1895	1899	rBV	468707	639812	59.89%	5.258%
13	13.880	1899	1903	1909	rVB	76727	103160	9.66%	0.848%
14	14.115	1937	1943	1952	rBV	511679	765585	71.67%	6.291%
15	14.315	1973	1977	1981	rBB	18508	21794	2.04%	0.179%
16	14.427	1989	1996	2003	rVB2	431182	671037	62.81%	5.514%
17	14.627	2025	2030	2050	rBV	134130	222899	20.87%	1.832%
18	15.268	2134	2139	2144	rBV	26589	31743	2.97%	0.261%
19	15.421	2158	2165	2175	rVB	668063	966035	90.43%	7.938%
20	15.545	2181	2186	2194	rBB	160906	219661	20.56%	1.805%
21	15.662	2201	2206	2213	rBV3	9579	19850	1.86%	0.163%
22	16.133	2282	2286	2294	rBV	22351	35234	3.30%	0.290%
23	17.174	2456	2463	2469	rBV	545819	774952	72.54%	6.368%
24	17.274	2473	2480	2494	rVB	671464	992484	92.91%	8.156%
25	18.062	2610	2614	2620	rVB	13998	18337	1.72%	0.151%
26	19.568	2864	2870	2882	rBV2	784542	1068276	100.00%	8.778%
27	21.062	3120	3124	3134	rBV2	16846	30753	2.88%	0.253%
28	21.362	3169	3175	3185	rBV	586592	746131	69.84%	6.131%
29	22.921	3436	3440	3446	rVB	8775	11578	1.08%	0.095%
30	23.491	3530	3537	3546	rBV2	425752	798330	74.73%	6.560%
31	23.638	3555	3562	3571	rVB	333235	635514	59.49%	5.222%
32	24.150	3644	3649	3657	rVB2	13259	24773	2.32%	0.204%
33	24.903	3772	3777	3785	rBV4	8579	19517	1.83%	0.160%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005206.D
Acq On : 02 May 2016 23:40
Operator : UM/SJ
Sample : H2772-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Title : SVOA CALIBRATION


Sum of corrected areas: 12169301

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005206.D
Acq On : 02 May 2016 23:40
Operator : UM/SJ
Sample : H2772-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BD3B7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

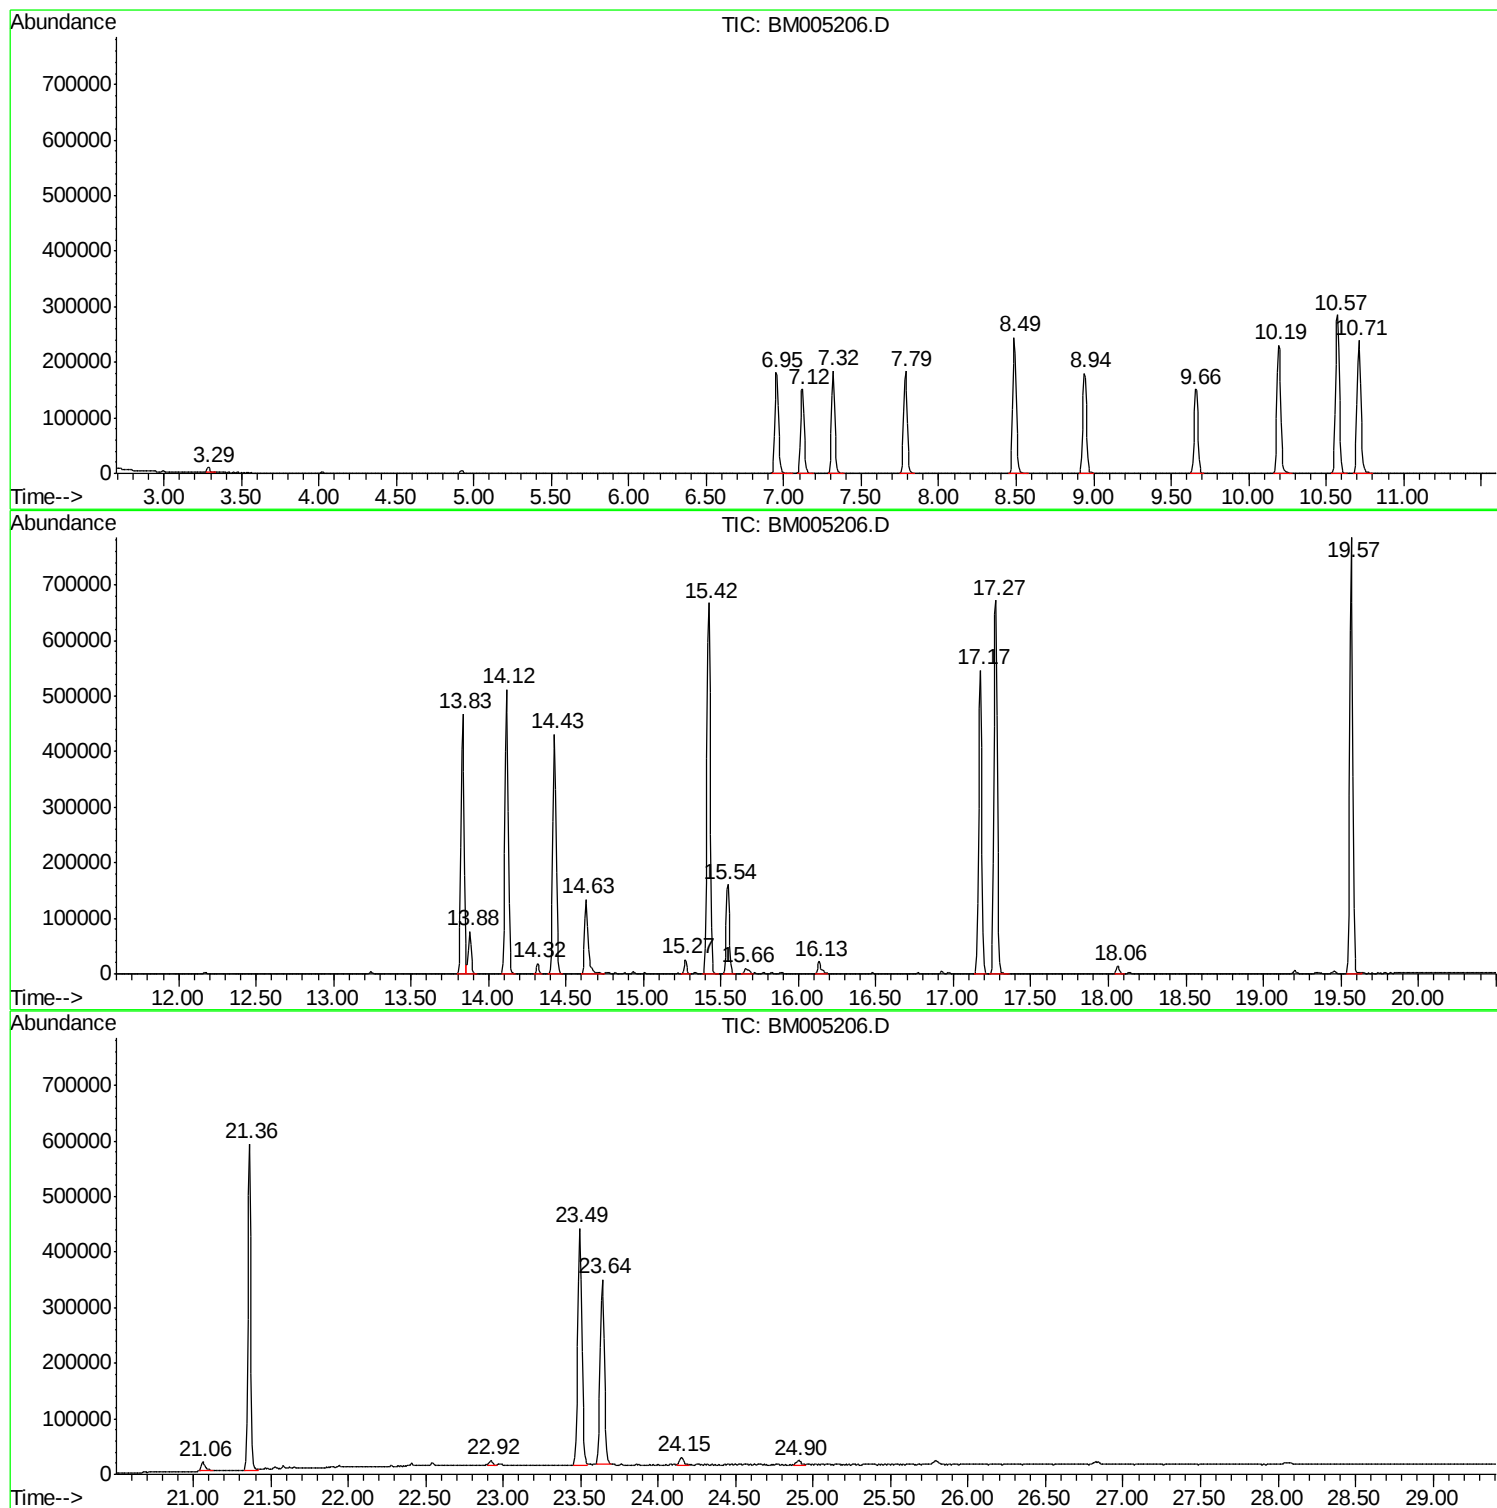

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005206.D
Acq On : 02 May 2016 23:40
Operator : UM/SJ
Sample : H2772-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005206.D
Acq On : 02 May 2016 23:40
Operator : UM/SJ
Sample : H2772-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3B7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc