

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005209.D
 Acq On : 03 May 2016 01:29
 Operator : UM/SJ
 Sample : H2772-23
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BD3C7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.951	720	725	740	rBB	209362	333444	23.60%	2.339%
2	7.122	748	754	765	rBB	178890	280618	19.86%	1.968%
3	7.316	782	787	798	rBB	220621	347384	24.58%	2.437%
4	7.787	861	867	875	rBV	178770	285187	20.18%	2.001%
5	8.487	980	986	999	rBB	287031	456792	32.33%	3.204%
6	8.940	1057	1063	1073	rBV	223727	360327	25.50%	2.528%
7	9.657	1180	1185	1193	rBV	183613	305474	21.62%	2.143%
8	10.192	1270	1276	1292	rBB	274760	470095	33.27%	3.298%
9	10.575	1334	1341	1350	rBB	277855	471032	33.34%	3.304%
10	10.710	1358	1364	1378	rBV	269670	456528	32.31%	3.202%
11	13.833	1889	1895	1899	rBV	570862	790835	55.97%	5.548%
12	13.880	1899	1903	1909	rVB	85174	116289	8.23%	0.816%
13	14.116	1937	1943	1955	rBV	635754	937988	66.38%	6.580%
14	14.316	1973	1977	1982	rBB	23513	28567	2.02%	0.200%
15	14.427	1989	1996	2003	rVB2	430851	669876	47.41%	4.699%
16	14.627	2025	2030	2049	rBV	163399	267897	18.96%	1.879%
17	15.269	2134	2139	2145	rVB	33090	40341	2.85%	0.283%
18	15.421	2158	2165	2175	rVB	804793	1183180	83.73%	8.300%
19	15.545	2181	2186	2196	rVB	193169	271636	19.22%	1.905%
20	15.663	2200	2206	2212	rBV4	12629	26253	1.86%	0.184%
21	16.133	2281	2286	2294	rBV	28285	44928	3.18%	0.315%
22	17.174	2456	2463	2471	rBV2	549877	799104	56.55%	5.606%
23	17.274	2473	2480	2493	rVB	860301	1261279	89.26%	8.848%
24	18.057	2609	2613	2621	rBV	18802	25668	1.82%	0.180%
25	19.568	2864	2870	2878	rBV2	984189	1413020	100.00%	9.912%
26	21.062	3119	3124	3136	rBV2	31162	64382	4.56%	0.452%
27	21.362	3169	3175	3182	rBV	612537	804183	56.91%	5.641%
28	22.203	3315	3318	3322	rVB	16660	19611	1.39%	0.138%
29	23.497	3530	3538	3548	rBV2	544251	1035323	73.27%	7.263%
30	23.639	3555	3562	3573	rVB2	337827	645775	45.70%	4.530%
31	24.144	3645	3648	3655	rVB3	12633	22720	1.61%	0.159%
32	24.909	3773	3778	3785	rVB3	9419	19962	1.41%	0.140%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005209.D
Acq On : 03 May 2016 01:29
Operator : UM/SJ
Sample : H2772-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Title : SVOA CALIBRATION


Sum of corrected areas: 14255698

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005209.D
Acq On : 03 May 2016 01:29
Operator : UM/SJ
Sample : H2772-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BD3C7

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

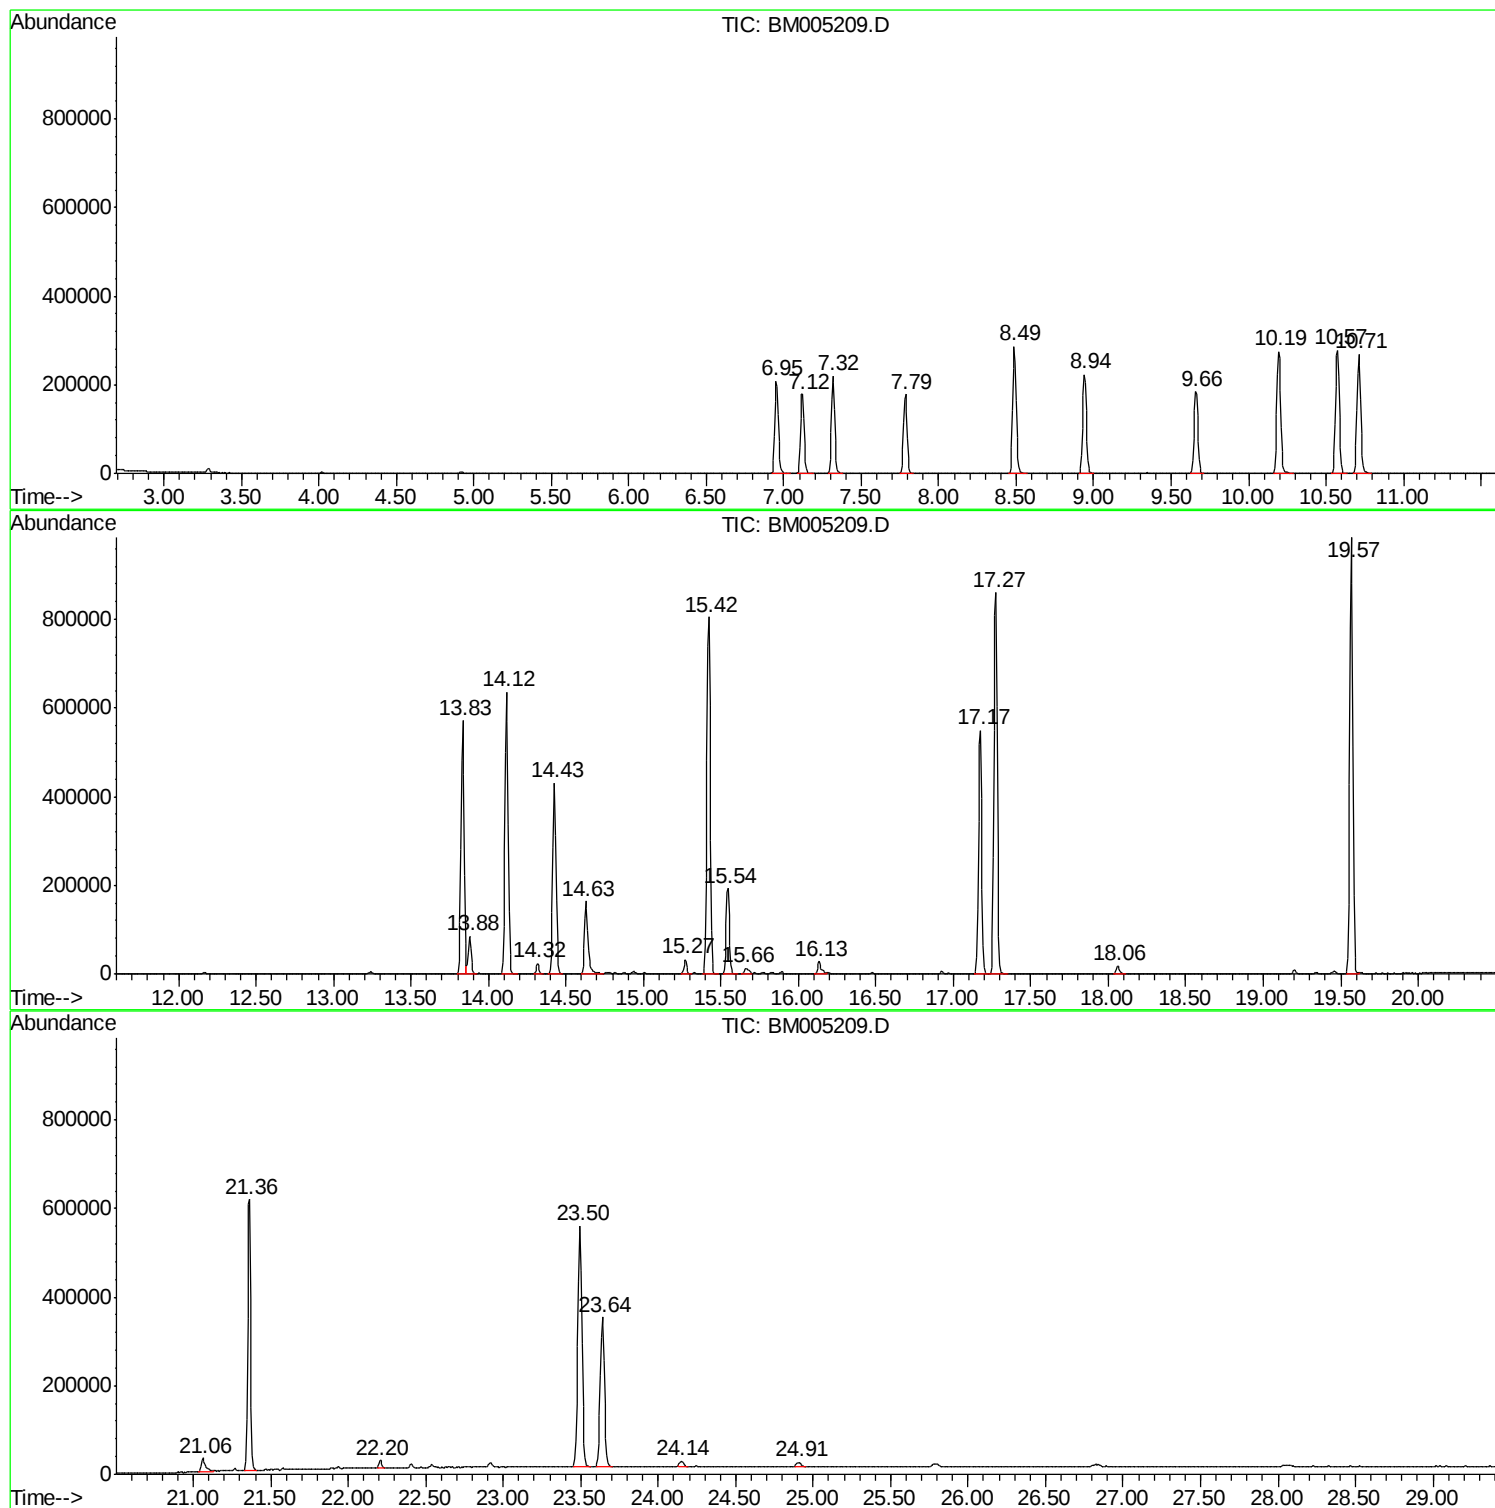

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005209.D
Acq On : 03 May 2016 01:29
Operator : UM/SJ
Sample : H2772-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005209.D
Acq On : 03 May 2016 01:29
Operator : UM/SJ
Sample : H2772-23
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BD3C7

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc