

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
 Data File : BM005210.D
 Acq On : 03 May 2016 02:05
 Operator : UM/SJ
 Sample : PB90243BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	98	102	108	rVB	11539	14381	1.05%	0.108%
2	6.951	720	725	741	rBB	205170	323834	23.75%	2.428%
3	7.122	747	754	764	rBV	170868	269333	19.75%	2.020%
4	7.316	782	787	799	rBB	209584	335227	24.58%	2.514%
5	7.787	861	867	876	rBB	168152	266538	19.54%	1.999%
6	8.487	980	986	1000	rBB	273059	435460	31.93%	3.265%
7	8.939	1057	1063	1074	rBV	210591	343603	25.20%	2.577%
8	9.657	1180	1185	1195	rBB	175413	290094	21.27%	2.175%
9	10.192	1270	1276	1291	rBV	266589	445118	32.64%	3.338%
10	10.575	1334	1341	1351	rBB	261083	442325	32.44%	3.317%
11	10.710	1358	1364	1384	rBV	261550	453255	33.24%	3.399%
12	13.833	1889	1895	1905	rBB	534673	742818	54.47%	5.570%
13	14.116	1937	1943	1963	rBB	591204	878625	64.43%	6.588%
14	14.427	1989	1996	2003	rBB2	397226	627318	46.00%	4.704%
15	14.627	2025	2030	2052	rBB	188908	299688	21.98%	2.247%
16	15.421	2158	2165	2175	rBB	760674	1110580	81.44%	8.328%
17	15.545	2181	2186	2193	rBV	209061	284749	20.88%	2.135%
18	17.174	2457	2463	2471	rBV	531298	754595	55.33%	5.658%
19	17.274	2473	2480	2490	rVV	815636	1206048	88.44%	9.044%
20	19.568	2864	2870	2882	rBV2	956938	1363723	100.00%	10.226%
21	21.362	3169	3175	3183	rBV	584804	784011	57.49%	5.879%
22	23.491	3529	3537	3548	rBV2	519550	1004869	73.69%	7.535%
23	23.638	3554	3562	3572	rBV2	324751	621424	45.57%	4.660%
24	24.150	3645	3649	3654	rVB	11637	19867	1.46%	0.149%
25	24.903	3774	3777	3784	rVB2	10345	18367	1.35%	0.138%


Sum of corrected areas: 13335850

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050216\
Data File : BM005210.D
Acq On : 03 May 2016 02:05
Operator : UM/SJ
Sample : PB90243BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

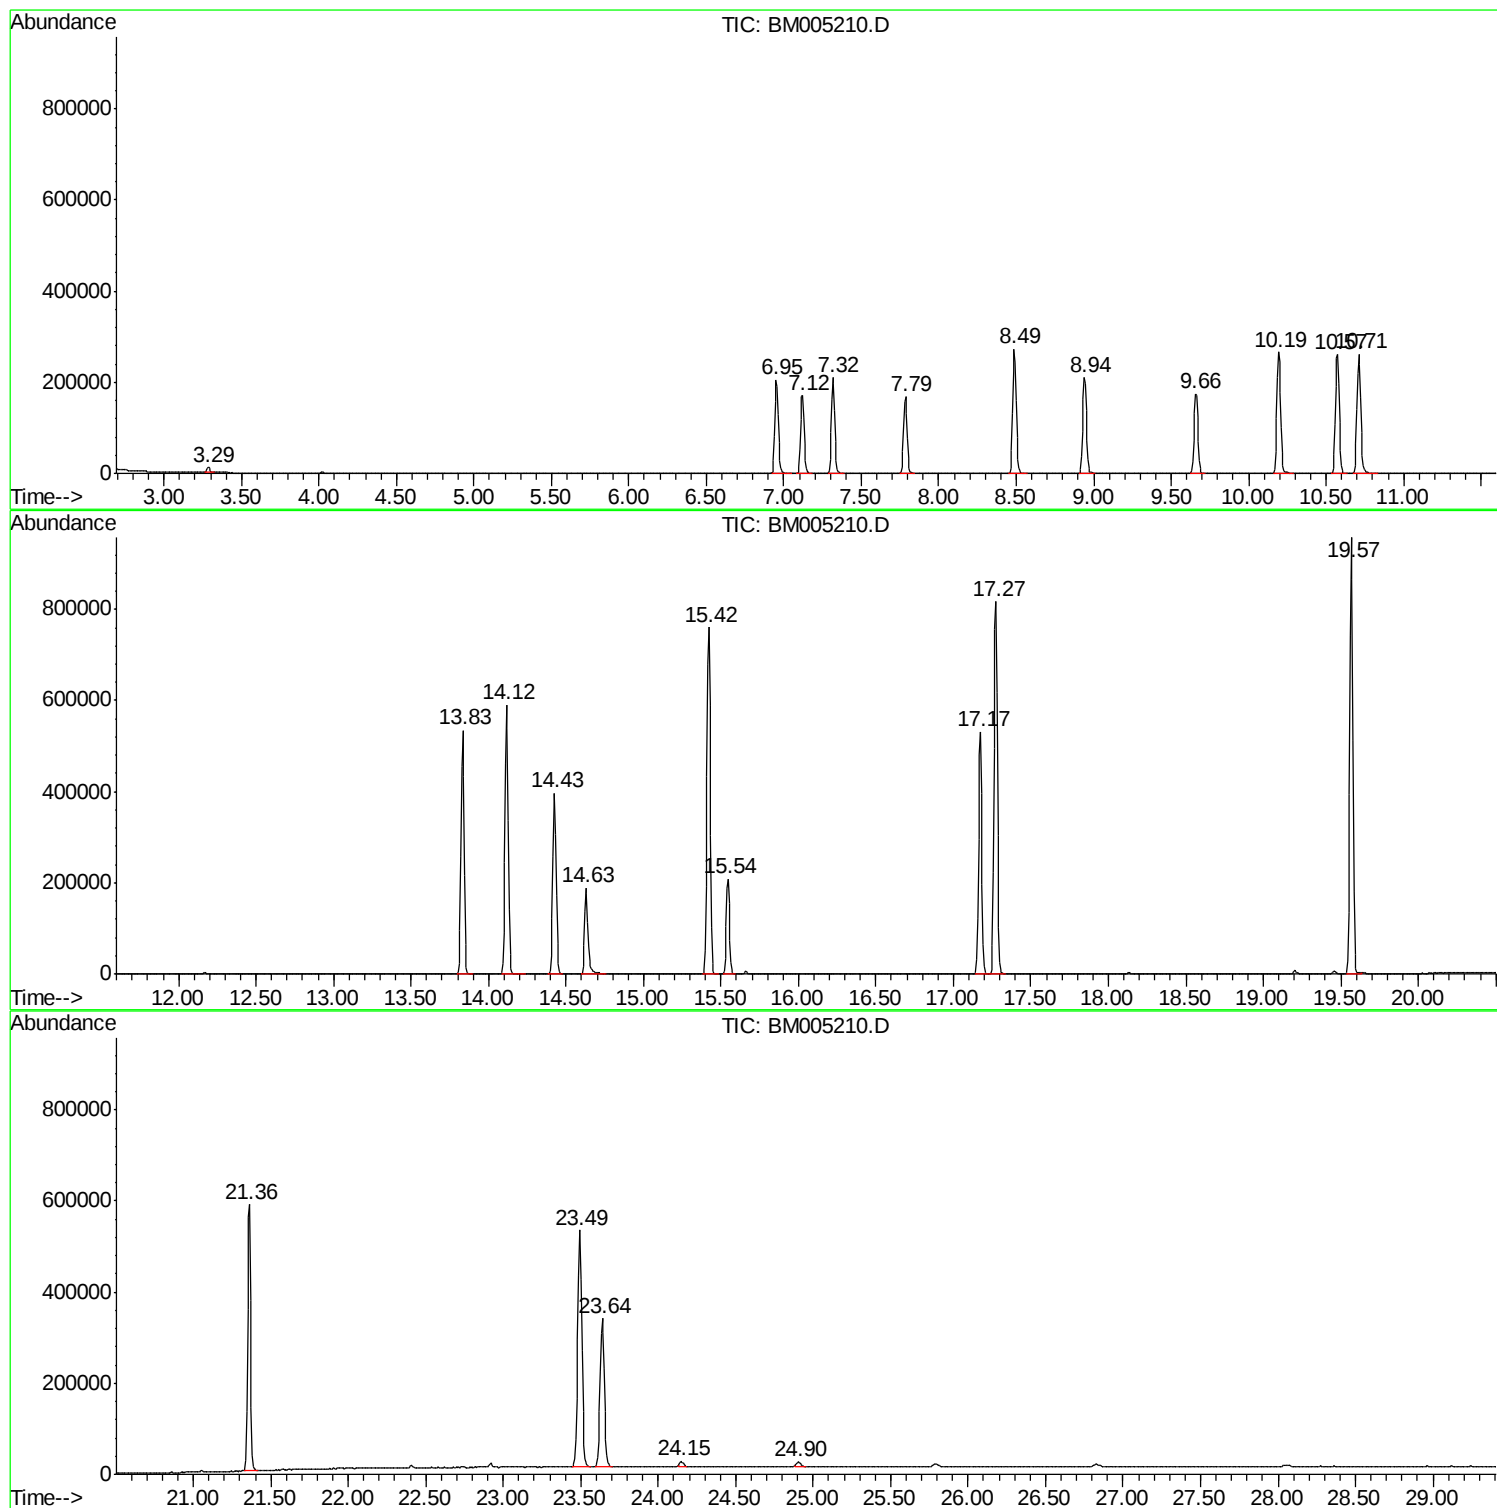

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005210.D
Acq On : 03 May 2016 02:05
Operator : UM/SJ
Sample : PB90243BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050216\
Data File : BM005210.D
Acq On : 03 May 2016 02:05
Operator : UM/SJ
Sample : PB90243BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc