

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050218\
 Data File : BM014934.D
 Acq On : 02 May 2018 22:09
 Operator : SJ/JU
 Sample : J2631-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 03 04:30:22 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 03 04:26:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.49	152	402917	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1680040	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	838803	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.81	188	1650964	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1469239	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1527902	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	72764	7.89	ng/uL	0.00
5) Phenol-d5	7.62	99	1381958	44.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	954201	47.77	ng/ul	0.00
9) 2-Chlorophenol-d4	8.01	132	1158586	44.46	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	1050966	42.31	ng/ul	0.00
19) Nitrobenzene-d5	9.67	128	539932	44.45	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	578602	47.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	1013791	41.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	1232300	50.80	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2882679	44.03	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	3472893	42.95	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	427481	35.18	ng/ul	0.00
57) Fluorene-d10	16.07	176	2415561	42.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	330468	36.99	ng/ul	0.00
70) Anthracene-d10	17.91	188	3409528	44.31	ng/ul	0.00
76) Pyrene-d10	20.15	212	3367415	48.44	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	3596962	47.92	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	7.65	94	74650	2.436 ng/ul#	82
15) N-Nitroso-di-n-propylamine	9.19	70	27016	1.430 ng/ul#	1
44) Dimethylphthalate	14.53	163	421289	6.656 ng/ul	99
81) Bis(2-ethylhexyl)phthalate	21.77	149	53655	1.044 ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050218\
Data File : BM014934.D
Acq On : 02 May 2018 22:09
Operator : SJ/JU
Sample : J2631-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :

Quant Time: May 03 04:30:22 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 03 04:26:19 2018
Response via : Initial Calibration

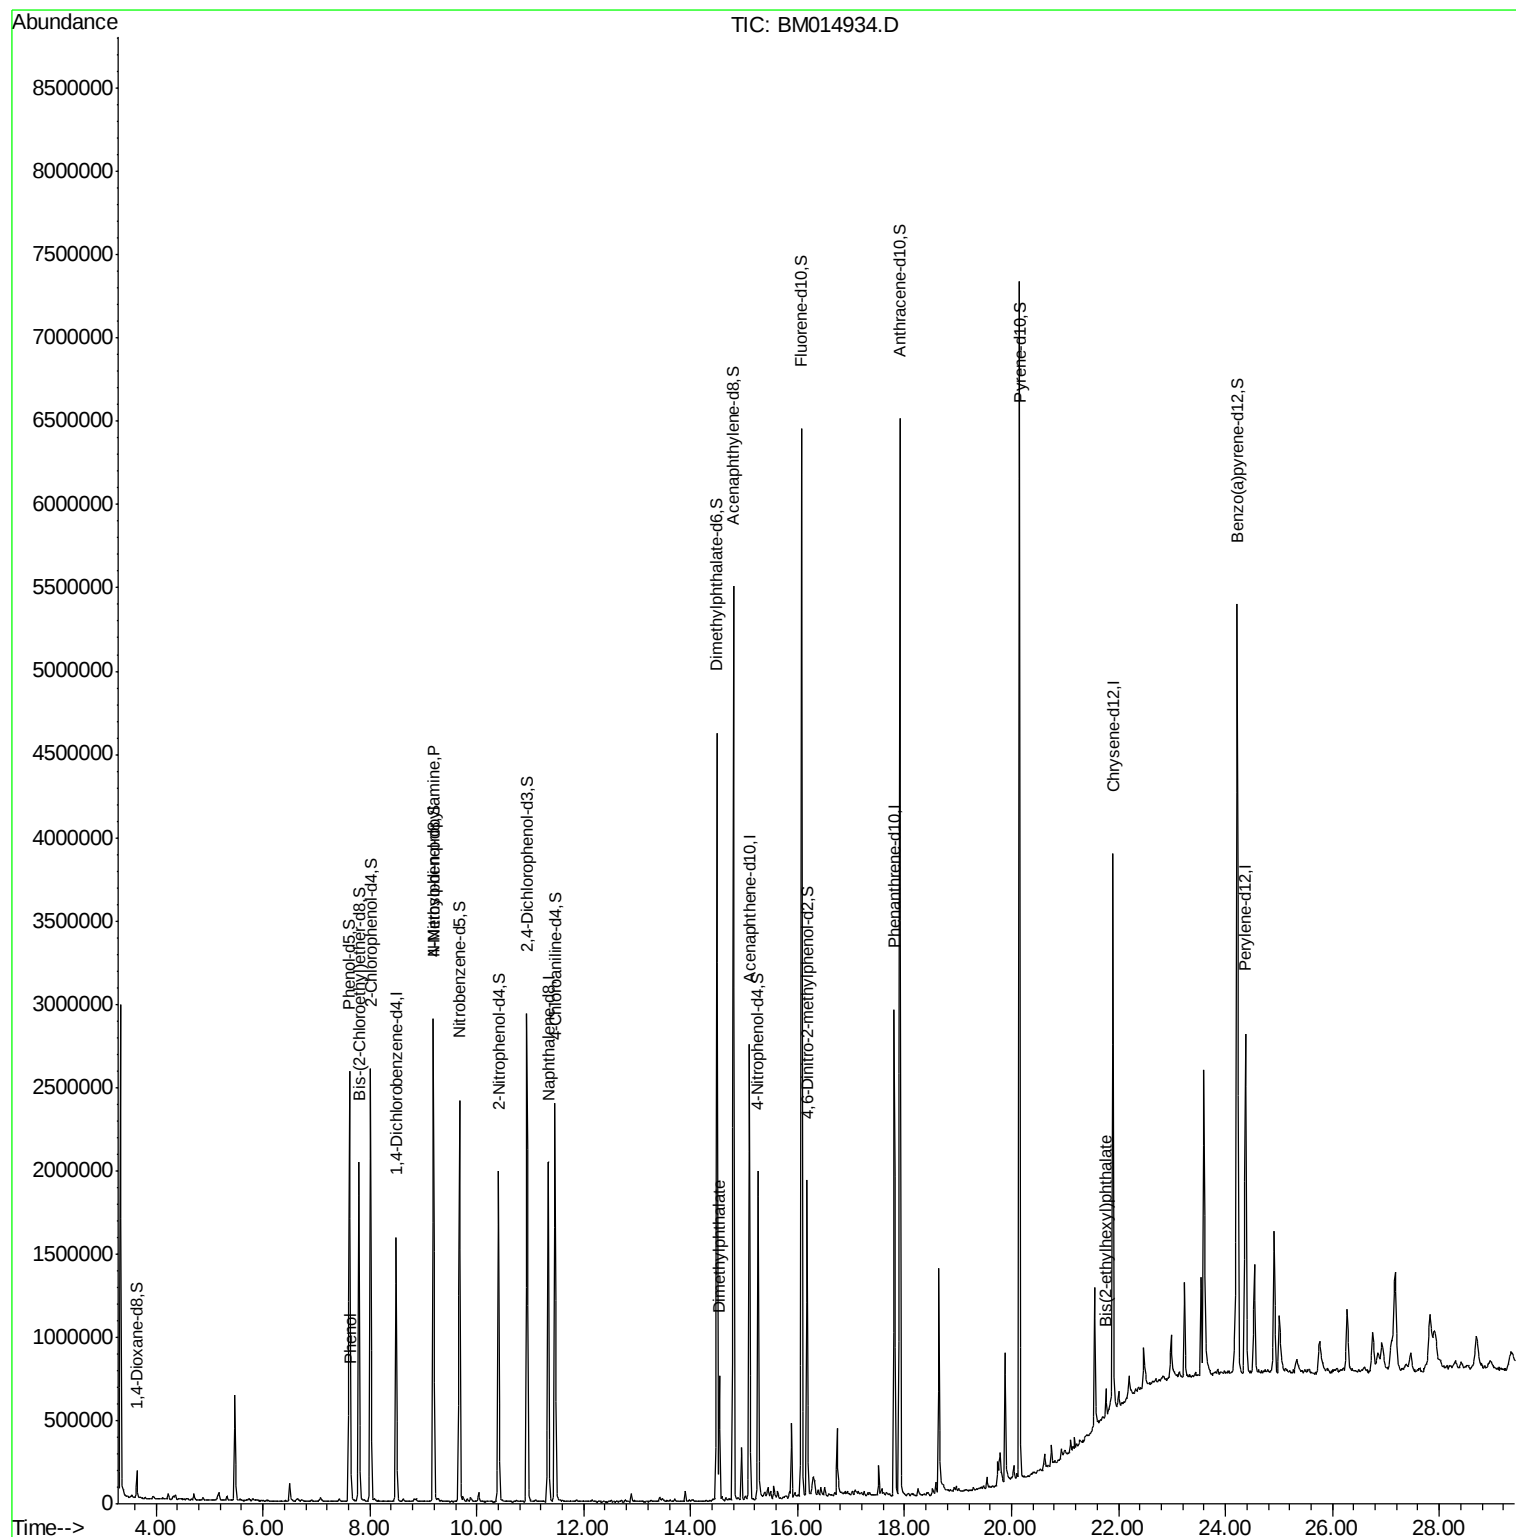

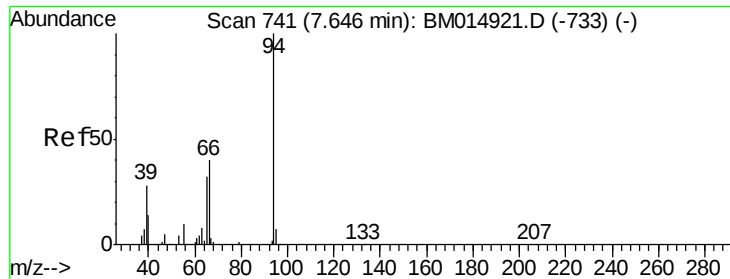





#6

Phenol

Concen: 2.436 ng/ul
 RT: 7.65 min Scan# 741
 Delta R.T. -0.00 min
 Lab File: BM014934.D
 Acq: 02 May 2018 22:09

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 94 Resp: 74650
 Ion Ratio Lower Upper
 94 100
 65 30.0 28.2 42.4
 66 41.3 47.2 70.8#

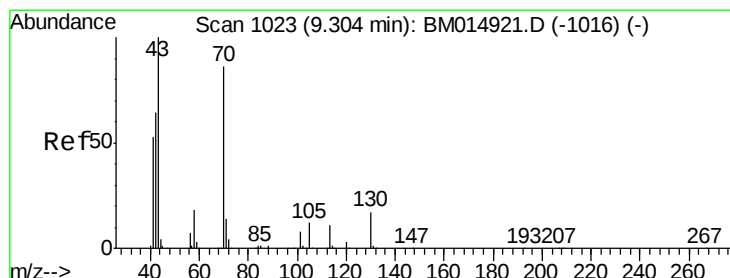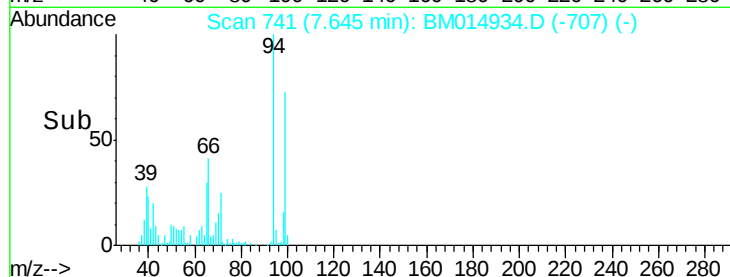
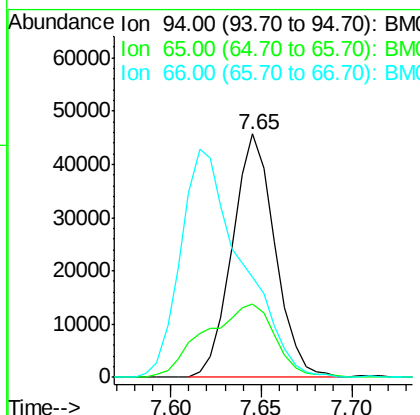
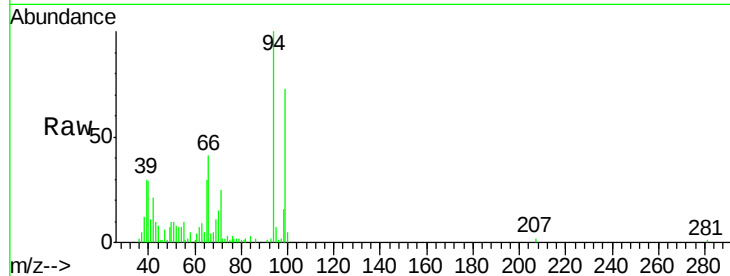



#15

N-Nitroso-di-n-propylamine

Concen: 1.430 ng/ul
 RT: 9.19 min Scan# 1004
 Delta R.T. -0.11 min
 Lab File: BM014934.D
 Acq: 02 May 2018 22:09

Tgt Ion: 70 Resp: 27016
 Ion Ratio Lower Upper
 70 100
 42 499.0 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

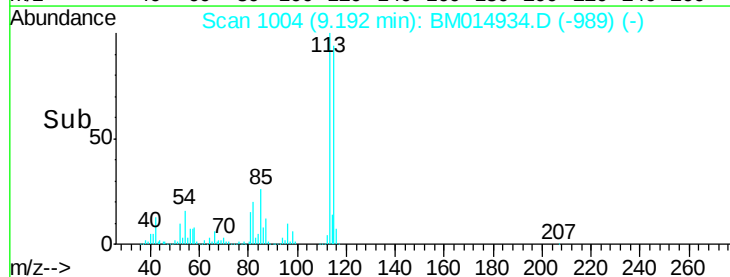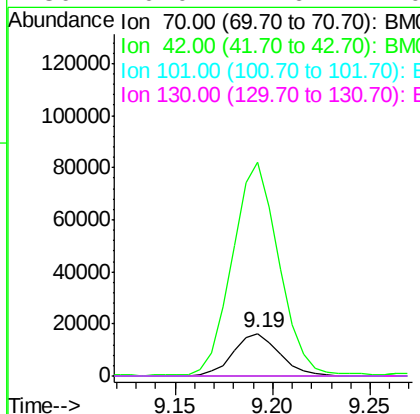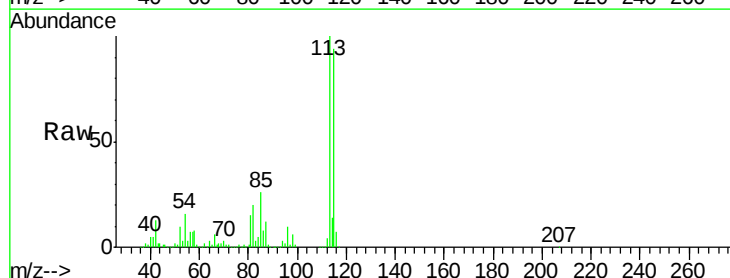

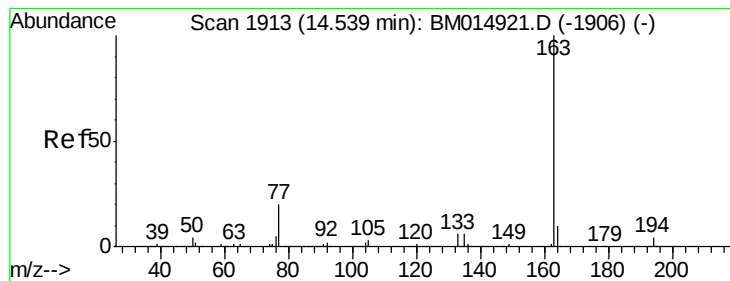

#44

Dimethylphthalate

Concen: 6.656 ng/ul

RT: 14.53 min Scan# 1912

Delta R.T. -0.01 min

Lab File: BM014934.D

Acq: 02 May 2018 22:09

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 421289

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3




164 9.9 8.2 12.4

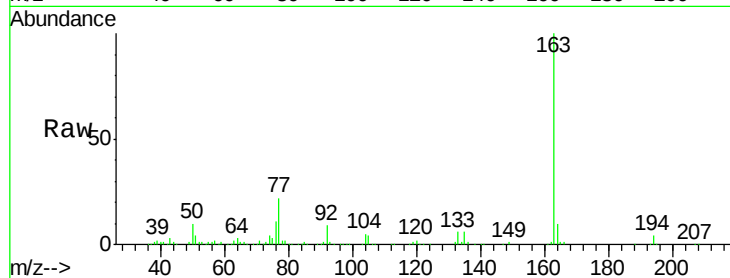

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

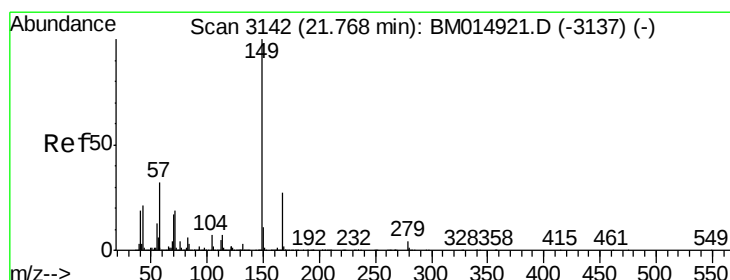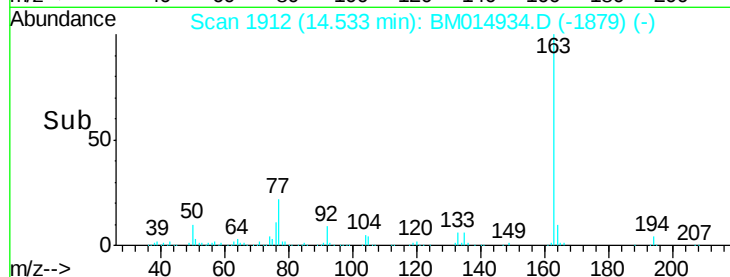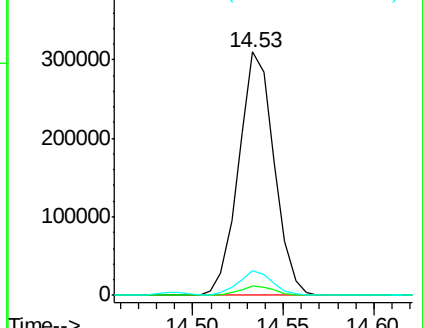

#81

Bis(2-ethylhexyl)phthalate

Concen: 1.044 ng/ul

RT: 21.77 min Scan# 3142

Delta R.T. -0.00 min

Lab File: BM014934.D

Acq: 02 May 2018 22:09


Tgt Ion:149 Resp: 53655

Ion Ratio Lower Upper

149 100

167 26.0 22.8 34.2

279 4.6 4.9 7.3#

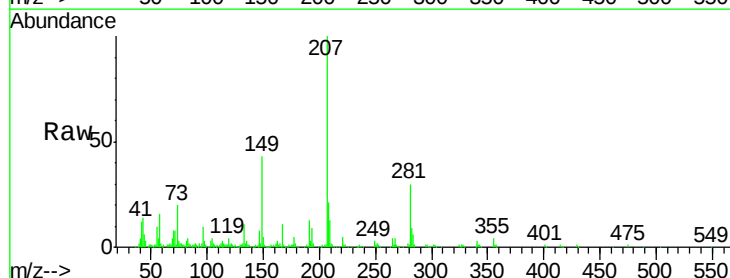

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

