

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050218\
 Data File : BM014939.D
 Acq On : 03 May 2018 01:16
 Operator : SJ/JU
 Sample : J2638-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 03 06:51:48 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 03 06:51:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.49	152	354308	20.00	ng/ul	0.00
18) Naphthalene-d8	11.33	136	1452407	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	723710	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.81	188	1457605	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1379185	20.00	ng/ul	0.00
83) Perylene-d12	24.37	264	1454046	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.64	96	59448	7.33	ng/uL	0.00
5) Phenol-d5	7.62	99	209980	7.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.79	67	633913	36.09	ng/ul	0.00
9) 2-Chlorophenol-d4	8.01	132	635950	27.76	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	364664	16.69	ng/ul	0.00
19) Nitrobenzene-d5	9.67	128	353397	33.65	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	367284	35.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	609330	28.68	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	7067	0.34	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	1873495	33.16	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2235533	32.05	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	54457	5.19	ng/ul	0.00
57) Fluorene-d10	16.07	176	1579610	32.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.17	200	213085	27.02	ng/ul	0.00
70) Anthracene-d10	17.91	188	2282170	33.60	ng/ul	0.00
76) Pyrene-d10	20.15	212	2320264	35.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	2560170	35.84	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.53	163	63470	1.162	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050218\
Data File : BM014939.D
Acq On : 03 May 2018 01:16
Operator : SJ/JU
Sample : J2638-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 03 06:51:48 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 03 06:51:06 2018
Response via : Initial Calibration

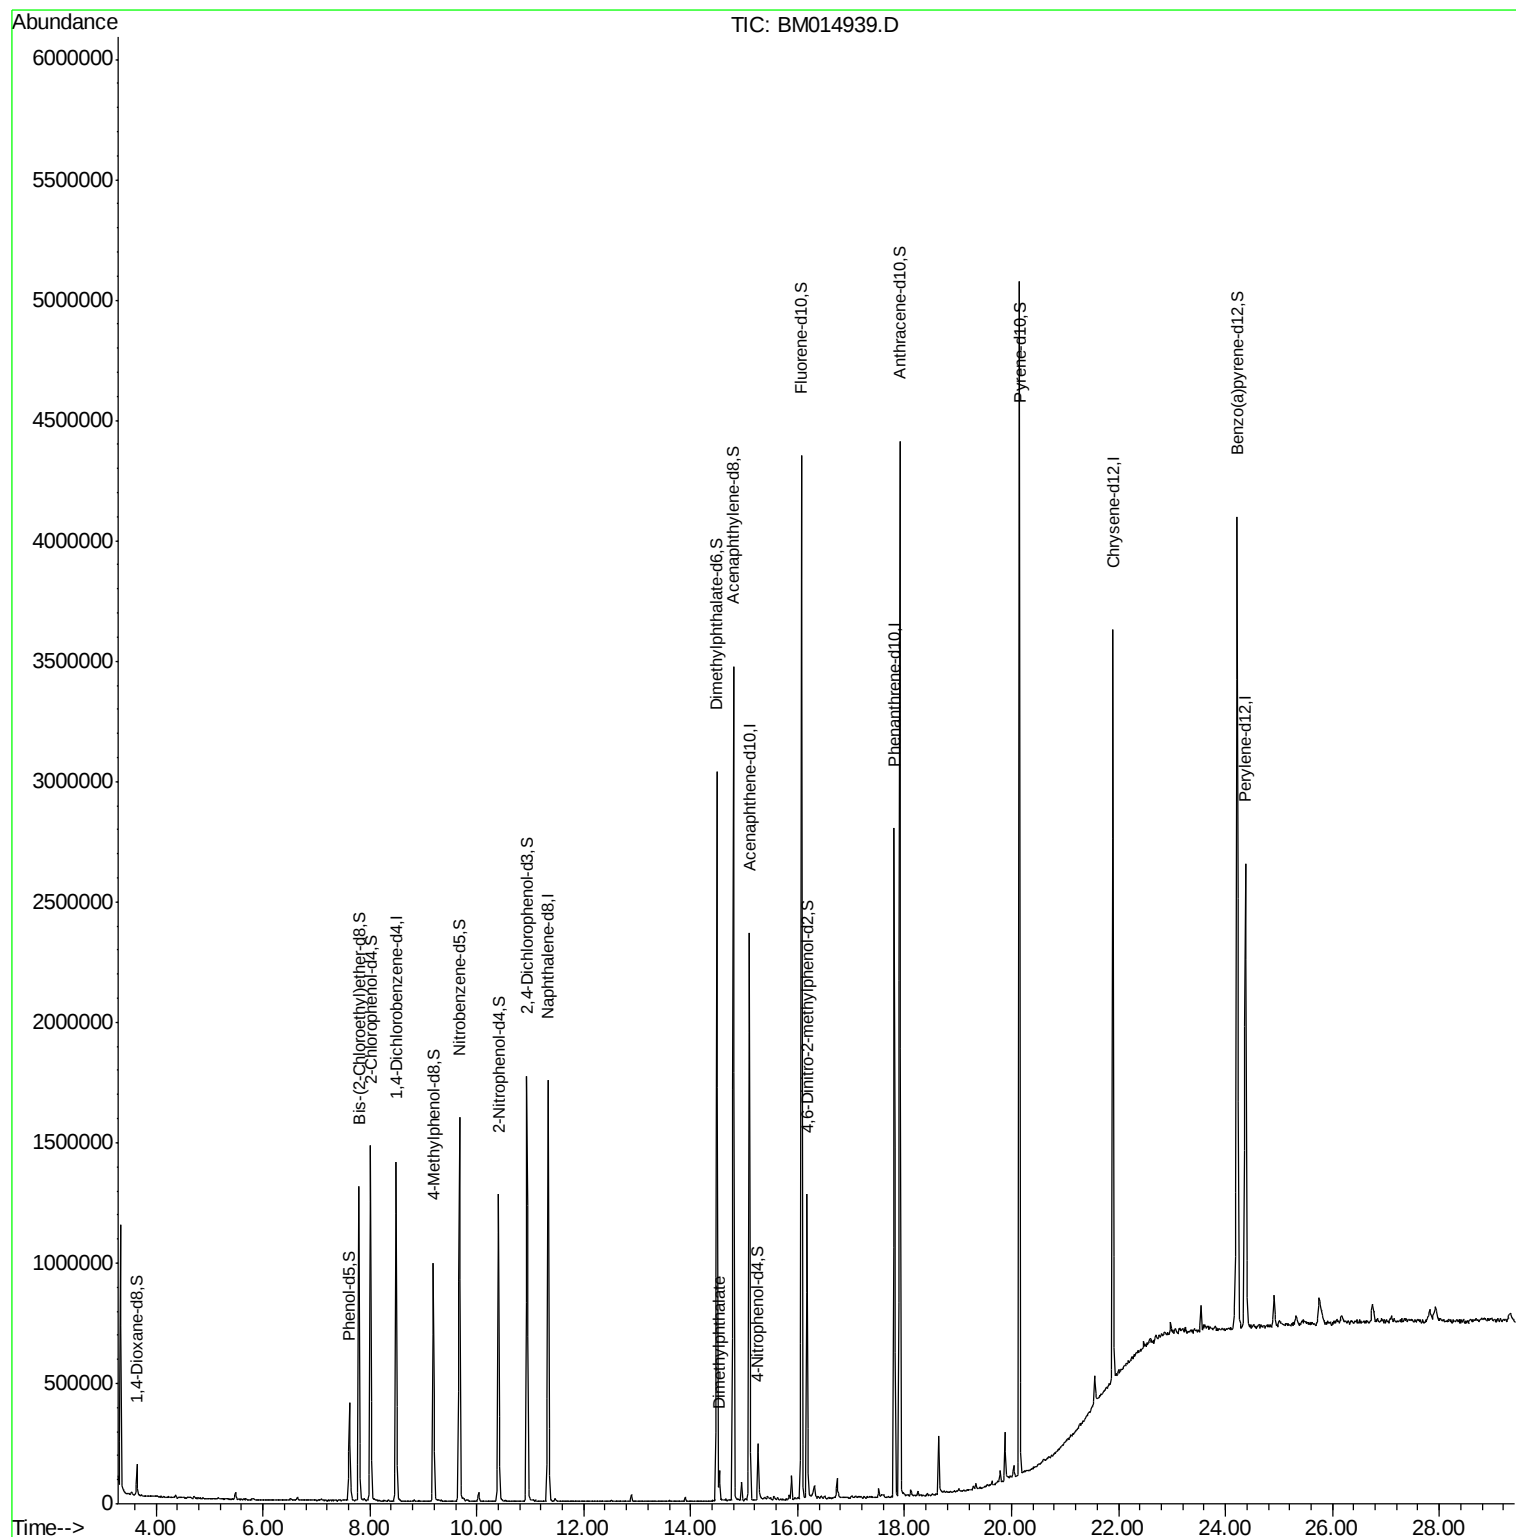

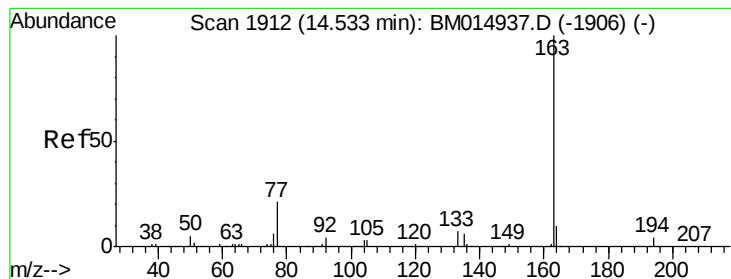

#44

Dimethylphthalate

Concen: 1.162 ng/ul

RT: 14.53 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BM014939.D

Acq: 03 May 2018 01:16

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 63470

Ion Ratio Lower Upper

163 100

194 3.4 3.5 5.3#

164 10.4 8.2 12.4

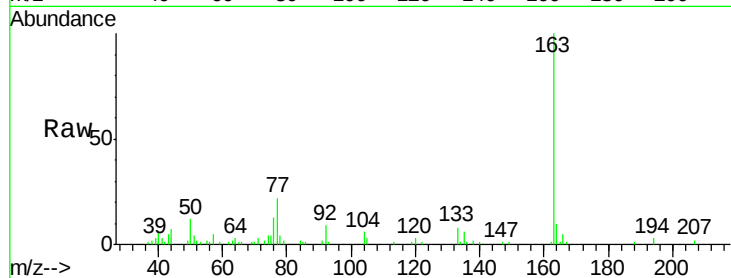

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

