

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050218\
 Data File : BM014934.D
 Acq On : 02 May 2018 22:09
 Operator : SJ/JU
 Sample : J2631-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AG9

Quant Time: May 03 06:38:26 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 03 04:26:19 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.49	152	402917	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	1680040	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	838803	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.81	188	1650964	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1469239	20.00	ng/ul	0.00
83) Perylene-d12	24.38	264	1527902	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	72764	7.89	ng/uL	0.00
5) Phenol-d5	7.62	99	1381958	44.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	954201	47.77	ng/ul	0.00
9) 2-Chlorophenol-d4	8.01	132	1158586	44.46	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	1050966	42.31	ng/ul	0.00
19) Nitrobenzene-d5	9.67	128	539932	44.45	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	578602	47.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	1013791	41.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	1232300	50.80	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2882679	44.03	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	3472893	42.95	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	427481	35.18	ng/ul	0.00
57) Fluorene-d10	16.07	176	2415561	42.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	330468	36.99	ng/ul	0.00
70) Anthracene-d10	17.91	188	3409528	44.31	ng/ul	0.00
76) Pyrene-d10	20.15	212	3367415	48.44	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	3596962	47.92	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.65	94	74650	2.436	ng/ul#	82
44) Dimethylphthalate	14.53	163	421289	6.656	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050218\
Data File : BM014934.D
Acq On : 02 May 2018 22:09
Operator : SJ/JU
Sample : J2631-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AG9

Quant Time: May 03 06:38:26 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 03 04:26:19 2018
Response via : Initial Calibration

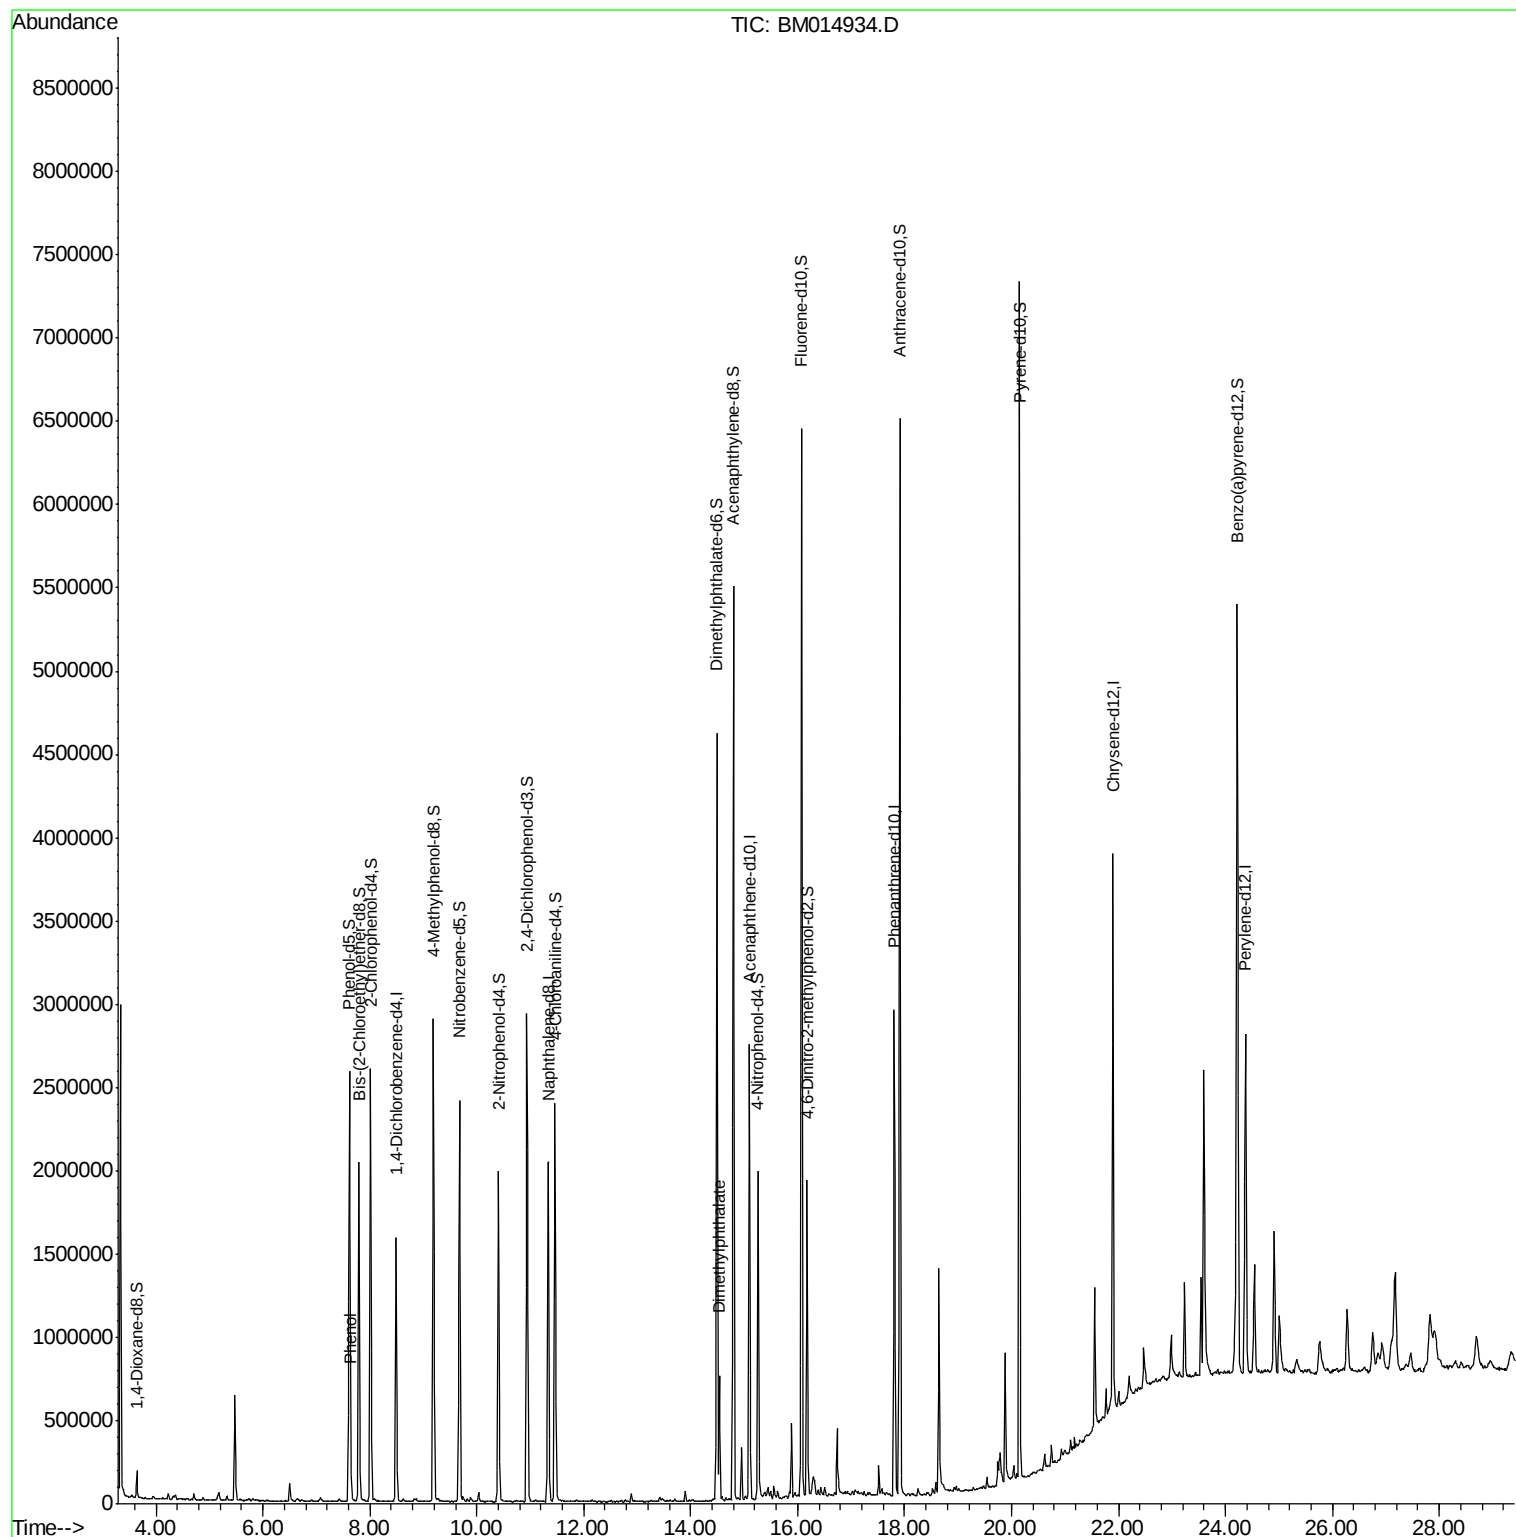

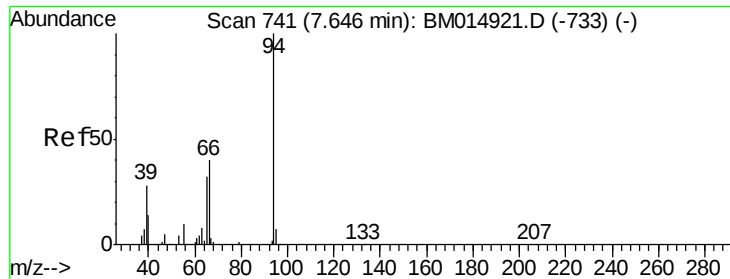





#6

Phenol

Concen: 2.436 ng/ul
 RT: 7.65 min Scan# 741
 Delta R.T. -0.00 min
 Lab File: BM014934.D
 Acq: 02 May 2018 22:09

Instrument :
 BNA_M
 ClientSampleId :
 C0AG9

Tot Ion: 94 Resp: 74650
 Ion Ratio Lower Upper
 94 100
 65 30.0 28.2 42.4
 66 41.3 47.2 70.8#

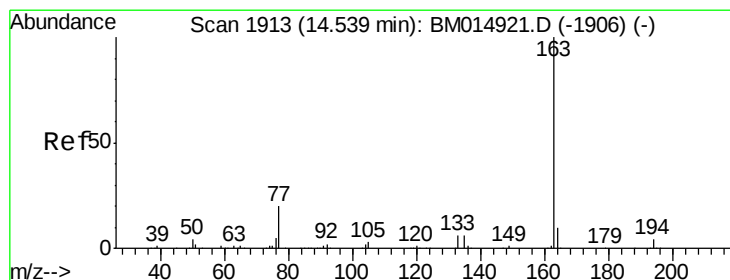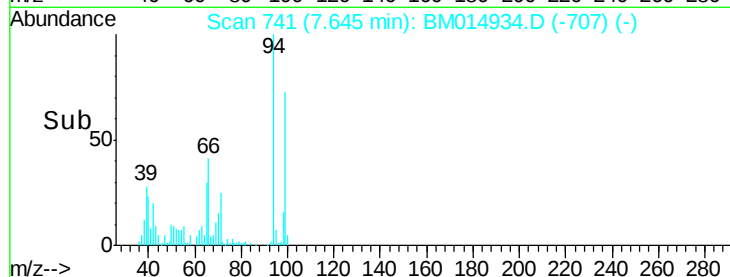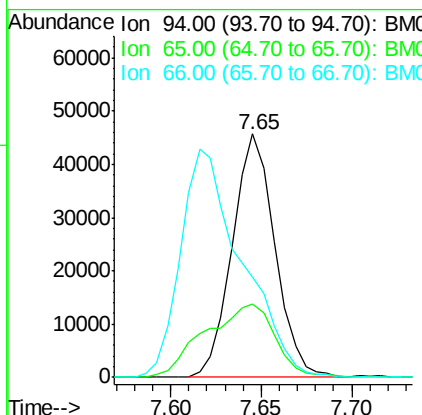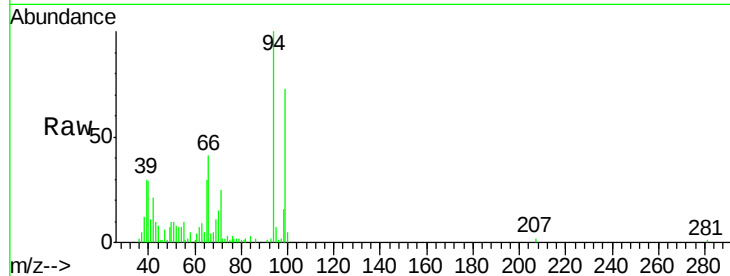

#44

Dimethylphthalate

Concen: 6.656 ng/ul
 RT: 14.53 min Scan# 1912
 Delta R.T. -0.01 min
 Lab File: BM014934.D
 Acq: 02 May 2018 22:09

Tgt Ion: 163 Resp: 421289
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.5 5.3
 164 9.9 8.2 12.4

