

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050219\
Data File : BM020103.D
Acq On : 02 May 2019 10:49
Operator : JU/SJ
Sample : PB119314BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119314BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.364	398	404	416	rVB	2808458	3890346	47.93%	9.124%
2	6.946	665	673	682	rBV	2571573	4066949	50.11%	9.538%
3	7.316	728	736	745	rBV	2759720	4272726	52.64%	10.020%
4	7.787	810	816	824	rVB	445065	682148	8.40%	1.600%
5	8.105	863	870	878	rVB	2080433	3255788	40.11%	7.635%
6	8.952	1006	1014	1022	rBV	1578084	2521062	31.06%	5.912%
7	10.581	1284	1291	1297	rBV	487464	805843	9.93%	1.890%
8	13.051	1704	1711	1720	rVB	3931255	5757592	70.94%	13.503%
9	14.428	1939	1945	1953	rBV2	716171	1037795	12.79%	2.434%
10	15.916	2192	2198	2219	rBV	3173411	4408424	54.32%	10.339%
11	17.175	2406	2412	2418	rBV	952475	1284870	15.83%	3.013%
12	19.804	2853	2859	2864	rBV	6757465	8116340	100.00%	19.035%
13	21.357	3118	3123	3130	rBV2	1058806	1317498	16.23%	3.090%
14	23.645	3505	3512	3519	rBV	650518	1222763	15.07%	2.868%


Sum of corrected areas: 42640144

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050219\
Data File : BM020103.D
Acq On : 02 May 2019 10:49
Operator : JU/SJ
Sample : PB119314BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119314BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

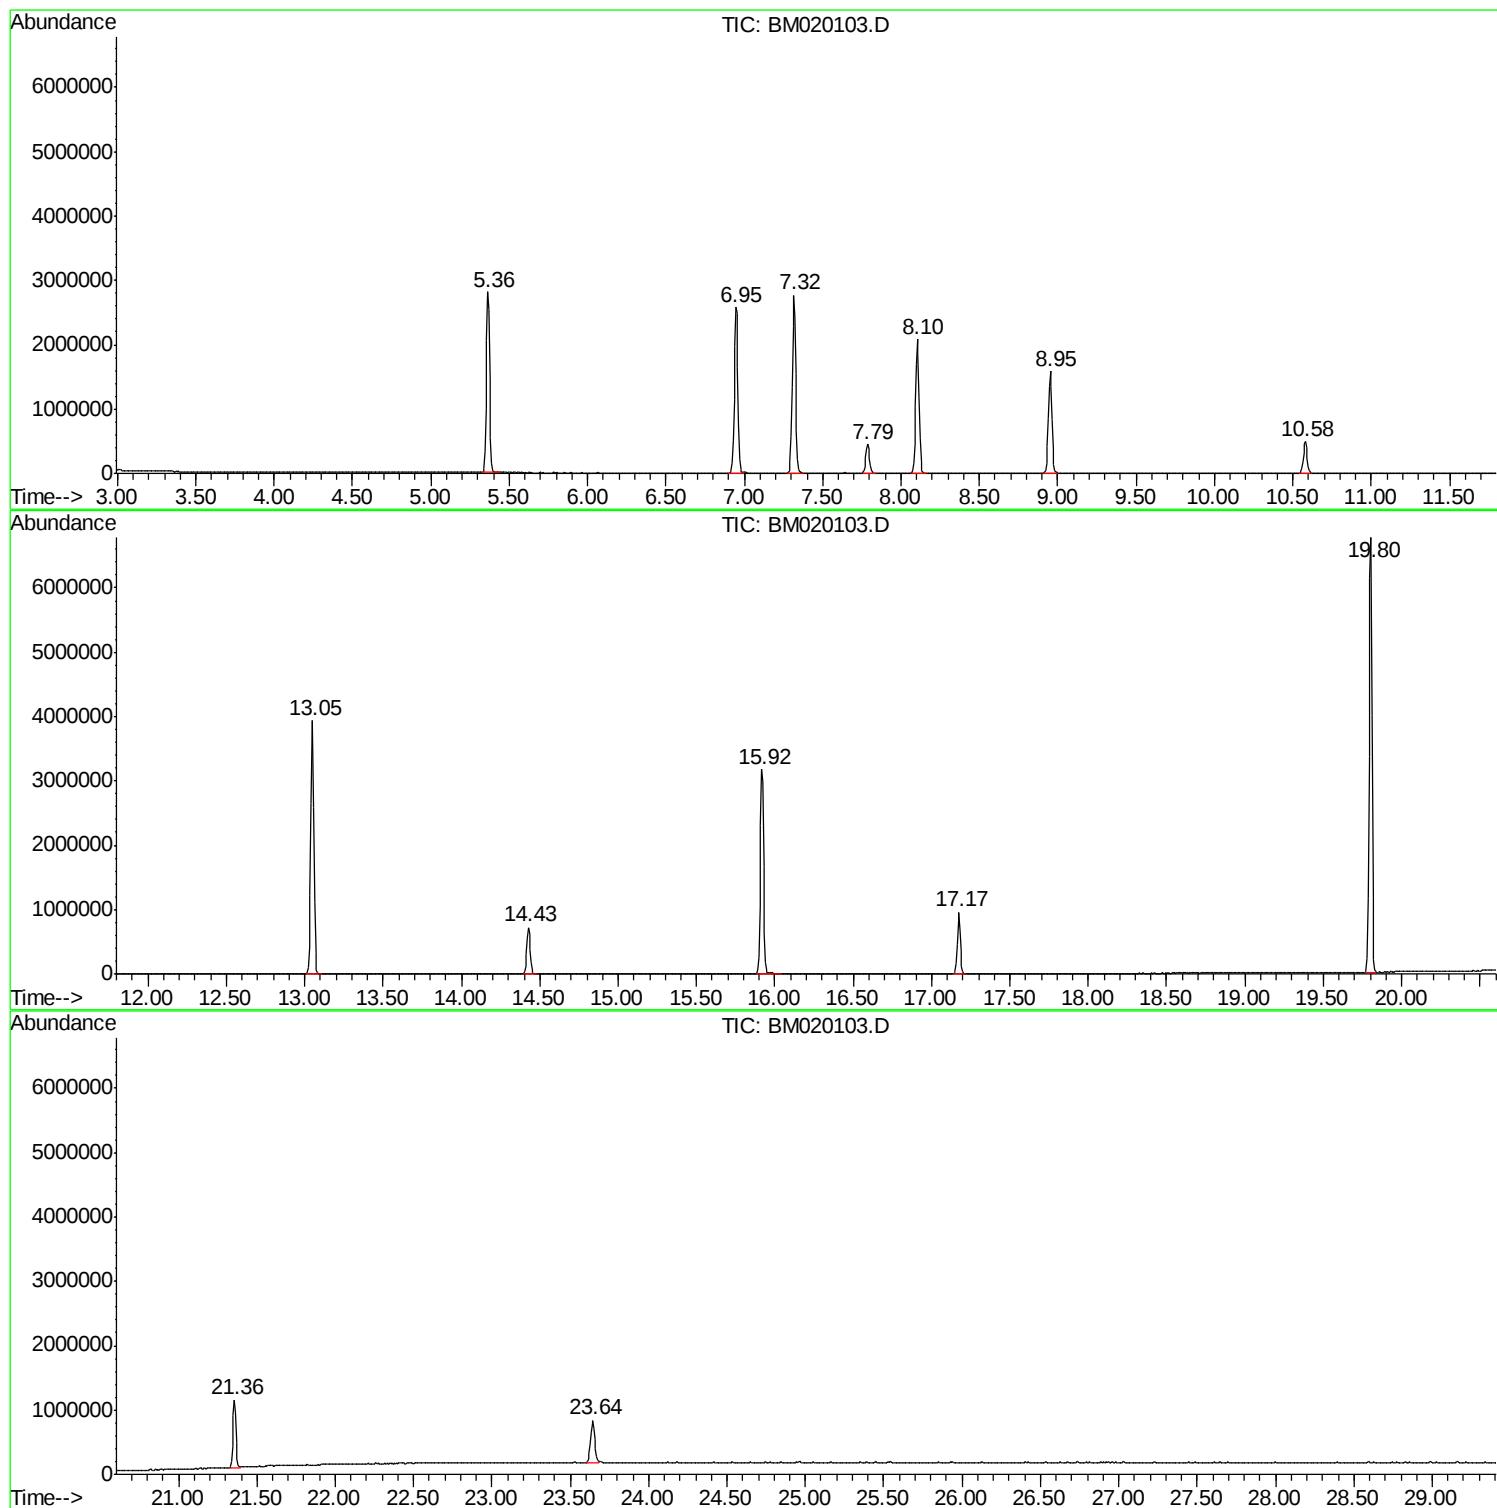

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050219\
Data File : BM020103.D
Acq On : 02 May 2019 10:49
Operator : JU/SJ
Sample : PB119314BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119314BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	125.27 ng	4272730	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
2		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	14
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
4		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9

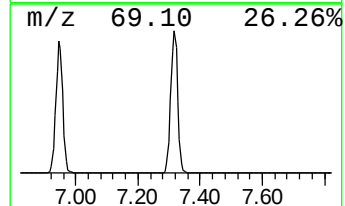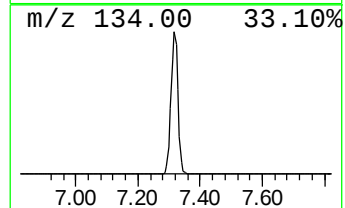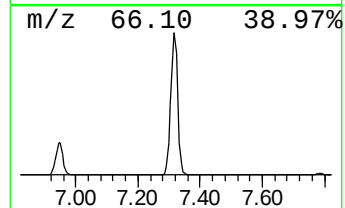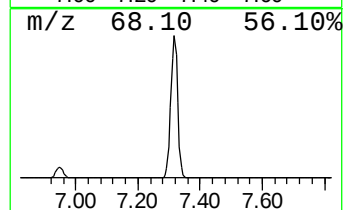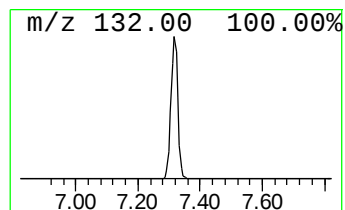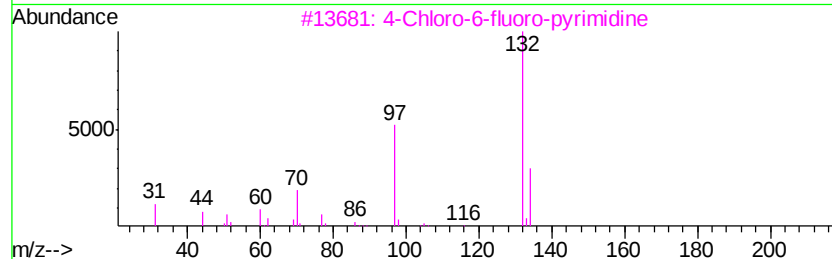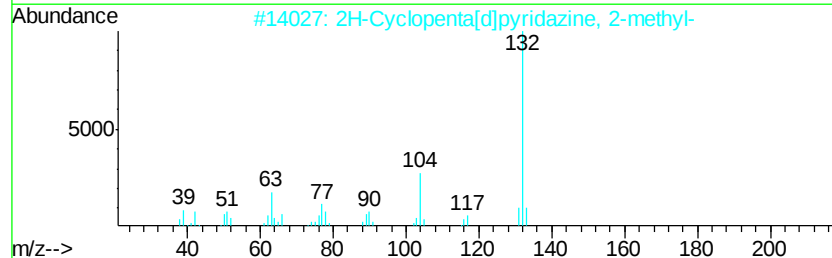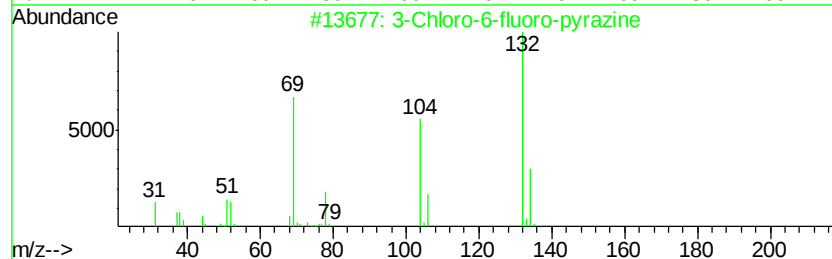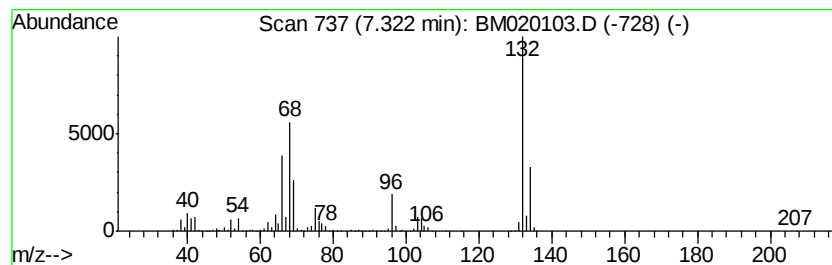

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050219\
Data File : BM020103.D
Acq On : 02 May 2019 10:49
Operator : JU/SJ
Sample : PB119314BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119314BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.32	7.32	125.3	ng	4272730	1	7.79	682148	20.0