

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
 Data File : BM034881.D
 Acq On : 02 May 2022 20:16
 Operator : CG/JU
 Sample : N2619-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB03-13-14-FT

Quant Time: May 03 05:22:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 01:51:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	201592	20.000	ng	0.00
21) Naphthalene-d8	10.728	136	846128	20.000	ng	0.00
39) Acenaphthene-d10	14.557	164	572651	20.000	ng	0.00
64) Phenanthrene-d10	17.298	188	1269427	20.000	ng	0.00
76) Chrysene-d12	21.474	240	1392527	20.000	ng	0.00
86) Perylene-d12	23.868	264	1288789	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.499	112	1159948	101.512	ng	0.00
7) Phenol-d6	7.093	99	1619622	109.796	ng	0.00
23) Nitrobenzene-d5	9.087	82	1071846	68.408	ng	0.00
42) 2,4,6-Tribromophenol	16.045	330	589872	94.693	ng	0.00
45) 2-Fluorobiphenyl	13.186	172	2561633	64.938	ng	0.00
79) Terphenyl-d14	19.921	244	4880841	67.865	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
Data File : BM034881.D
Acq On : 02 May 2022 20:16
Operator : CG/JU
Sample : N2619-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB03-13-14-FT

Quant Time: May 03 05:22:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration




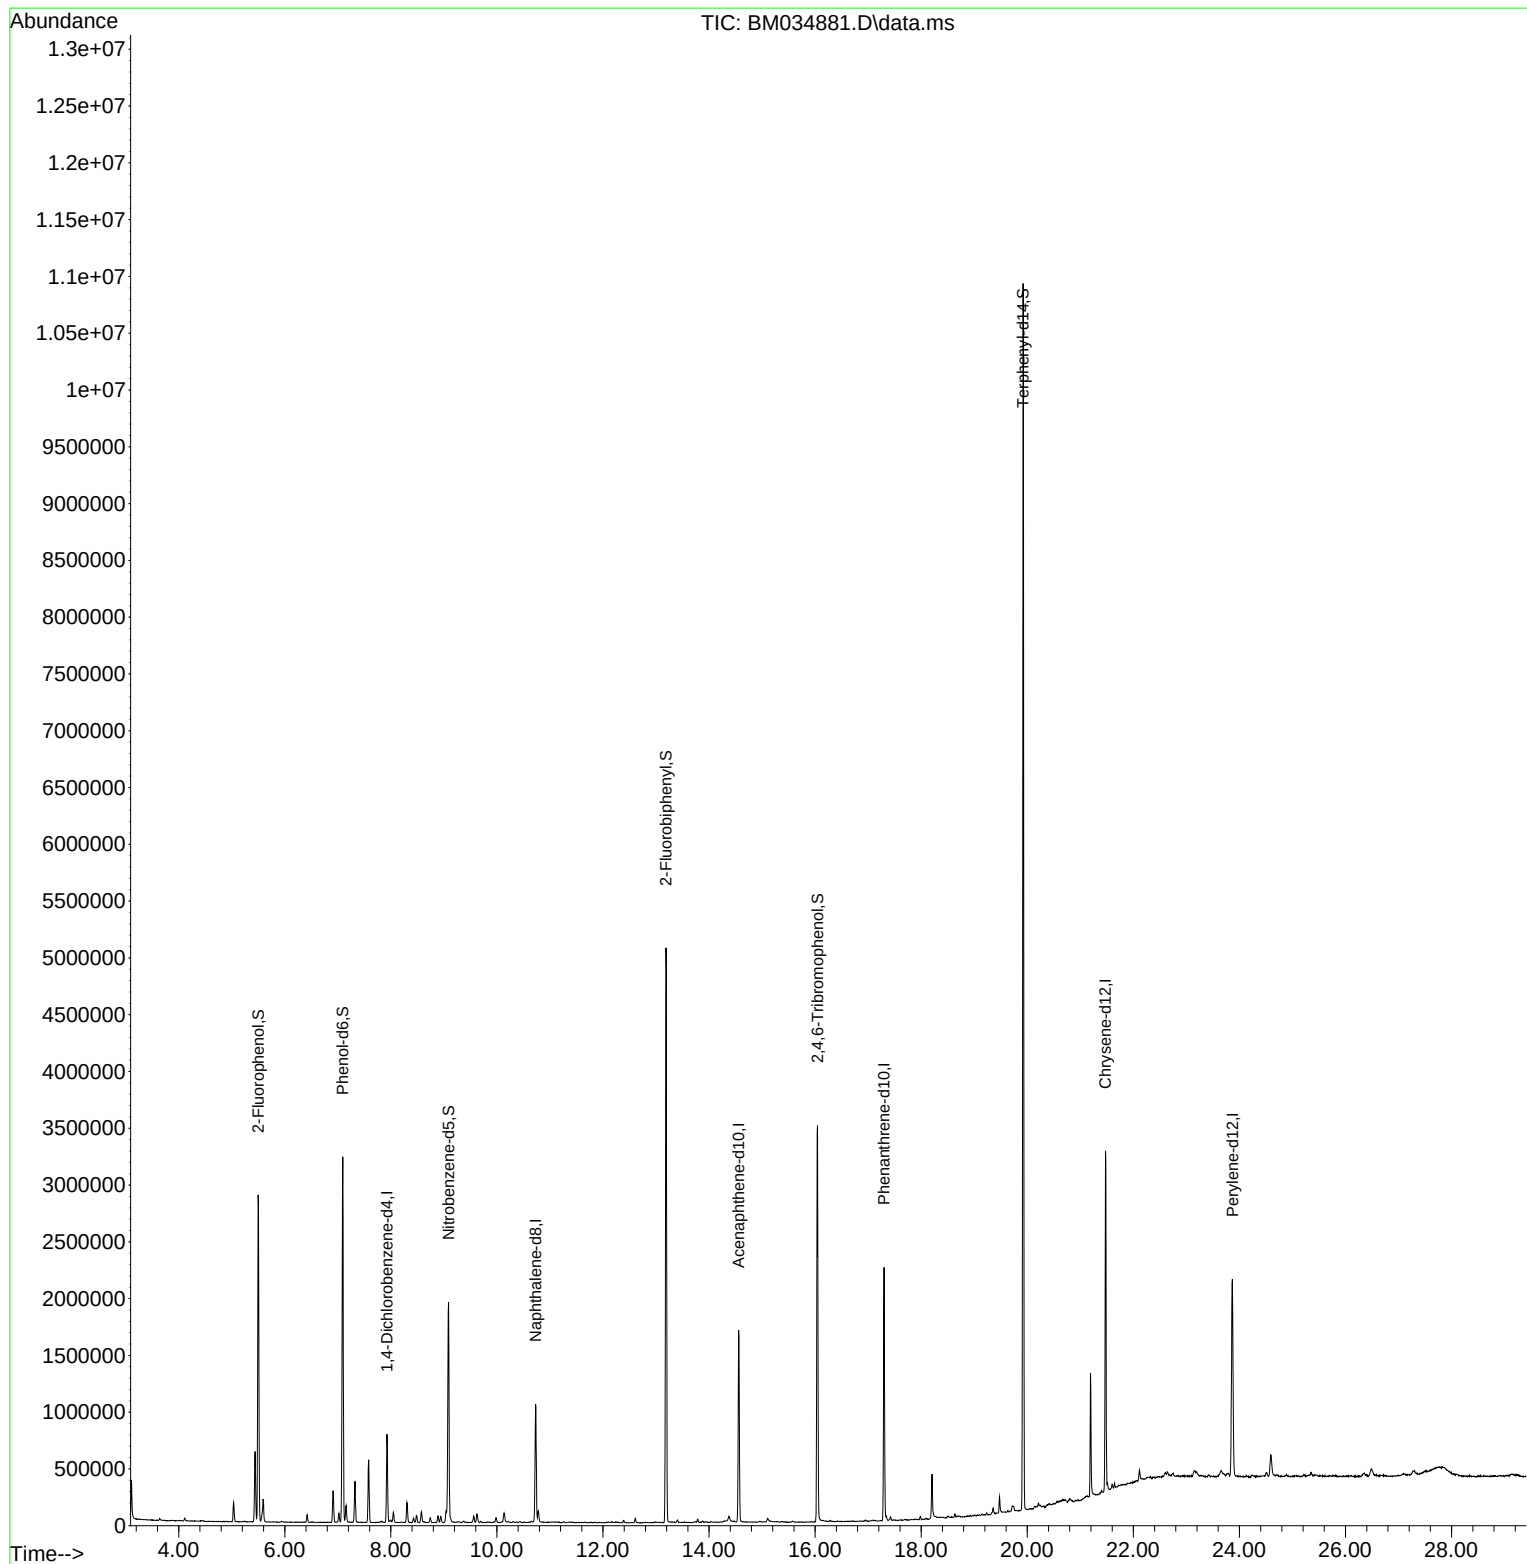




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.928 min Scan# 81
 Delta R.T. -0.006 min
 Lab File: BM034881.D
 Acq: 02 May 2022 20:16




Instrument :
 BNA_M
 ClientSampleId :
 SB03-13-14-FT


Tgt Ion:152 Resp: 201592
 Ion Ratio Lower Upper
 152 100
 150 158.2 124.9 187.3
 115 59.4 47.9 71.9

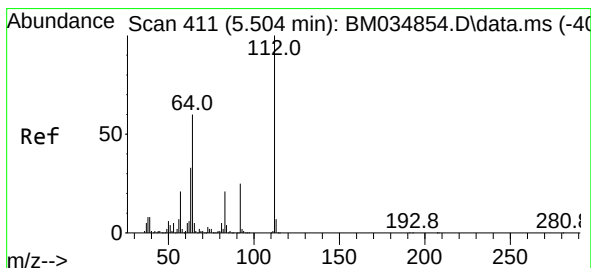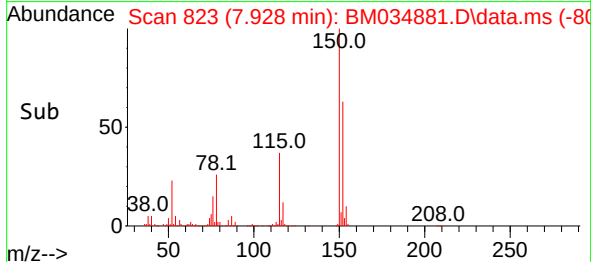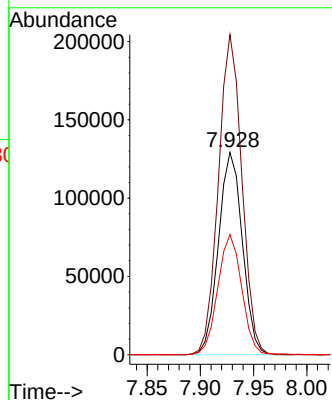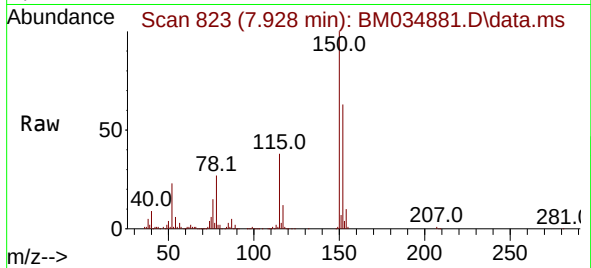

#5
 2-Fluorophenol
 Concen: 101.512 ng
 RT: 5.499 min Scan# 410
 Delta R.T. -0.005 min
 Lab File: BM034881.D
 Acq: 02 May 2022 20:16

Tgt Ion:112 Resp: 1159948
 Ion Ratio Lower Upper
 112 100
 64 61.2 47.8 71.6
 63 33.7 26.6 40.0


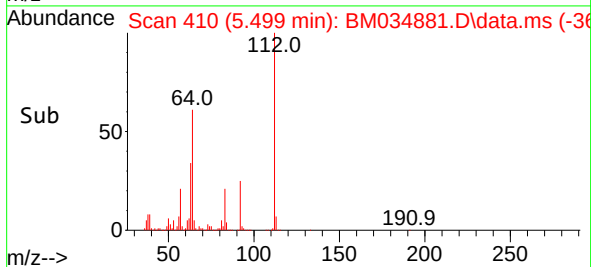
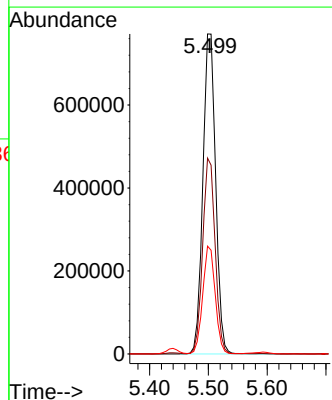
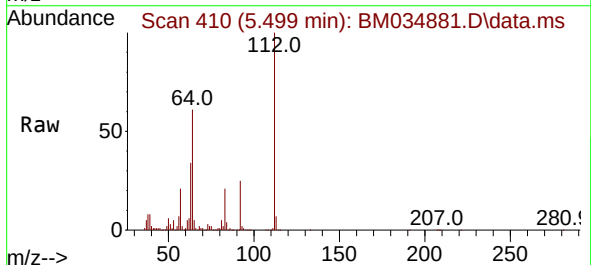




#7
Phenol-d6
Concen: 109.796 ng
RT: 7.093 min Scan# 61
Delta R.T. 0.001 min
Lab File: BM034881.D
Acq: 02 May 2022 20:16




Instrument :
BNA_M
ClientSampleId :
SB03-13-14-FT


Tgt Ion: 99 Resp: 1619622
Ion Ratio Lower Upper
99 100
42 22.5 18.8 28.2
71 36.9 30.2 45.2

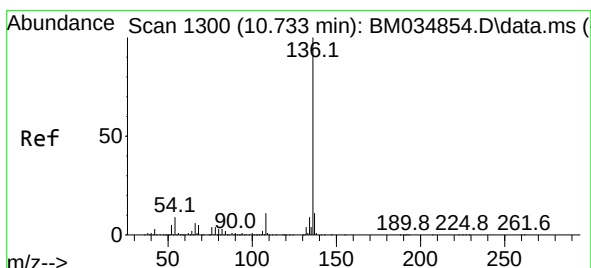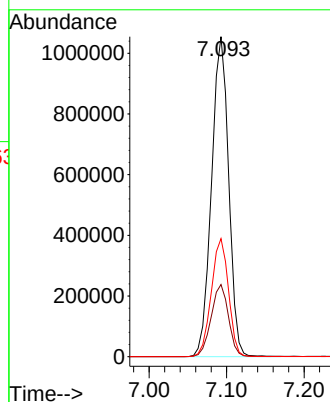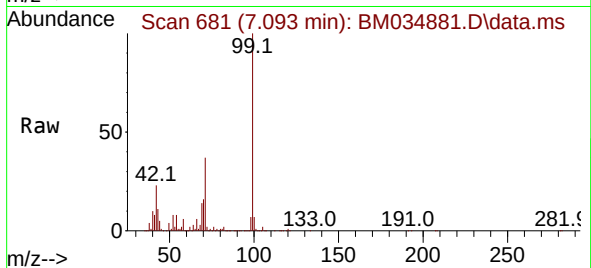

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.728 min Scan# 1299
Delta R.T. -0.005 min
Lab File: BM034881.D
Acq: 02 May 2022 20:16

Tgt Ion:136 Resp: 846128
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 8.2 7.0 10.4
68 5.8 4.3 6.5


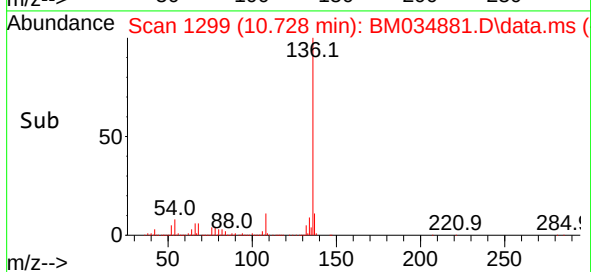
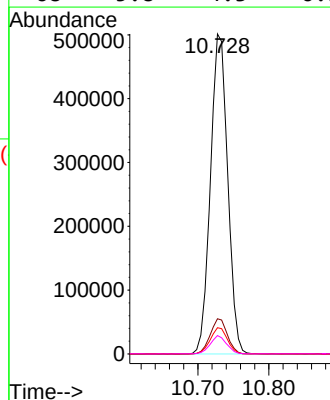





#23
Nitrobenzene-d5
Concen: 68.408 ng
RT: 9.087 min Scan# 1020
Delta R.T. -0.005 min
Lab File: BM034881.D
Acq: 02 May 2022 20:16




Instrument :
BNA_M
ClientSampleId :
SB03-13-14-FT


Tgt Ion: 82 Resp: 1071846
Ion Ratio Lower Upper
82 100
128 42.8 33.7 50.5
54 53.9 43.2 64.8

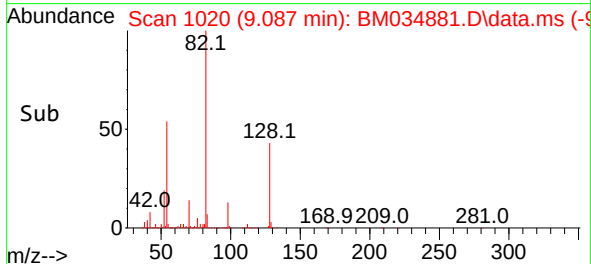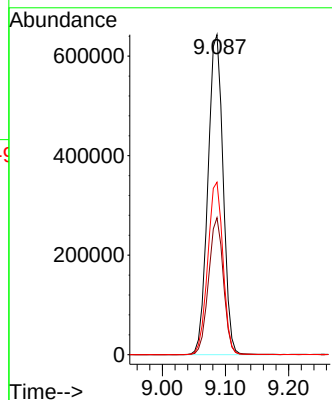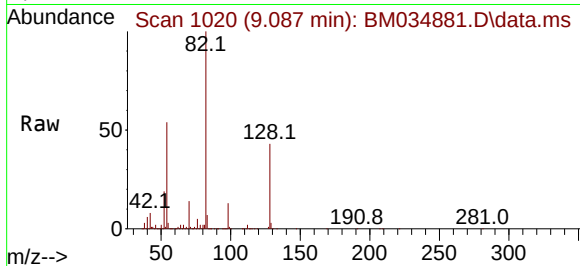

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.557 min Scan# 1950
Delta R.T. -0.005 min
Lab File: BM034881.D
Acq: 02 May 2022 20:16

Tgt Ion: 164 Resp: 572651
Ion Ratio Lower Upper
164 100
162 103.3 83.0 124.6
160 45.7 37.0 55.4


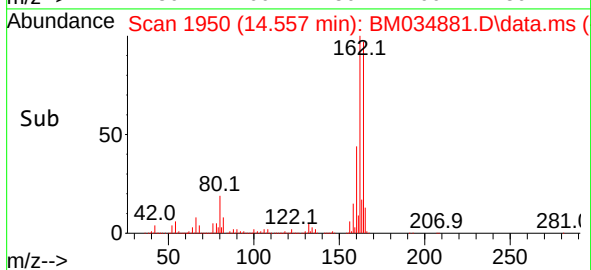
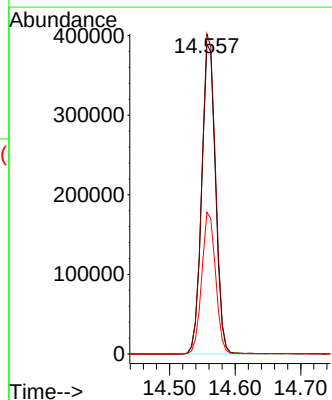
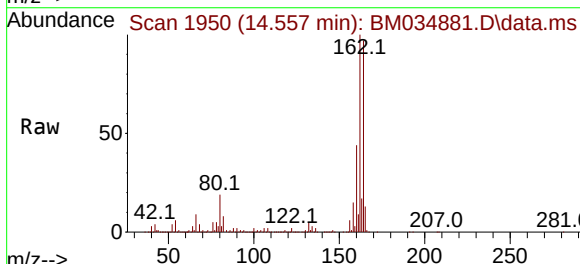




#42
2,4,6-Tribromophenol
Concen: 94.693 ng
RT: 16.045 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM034881.D
Acq: 02 May 2022 20:16




Instrument :
BNA_M
ClientSampleId :
SB03-13-14-FT


Tgt Ion:330 Resp: 589872
Ion Ratio Lower Upper
330 100
332 96.1 77.0 115.4
141 42.2 35.3 52.9

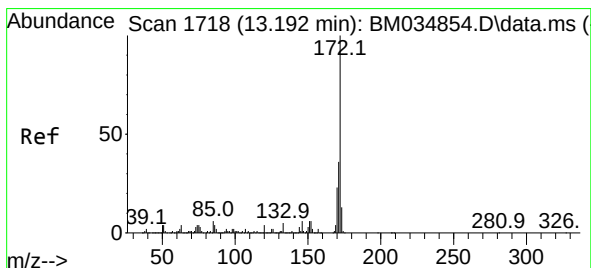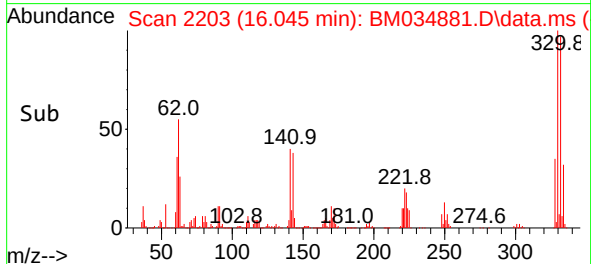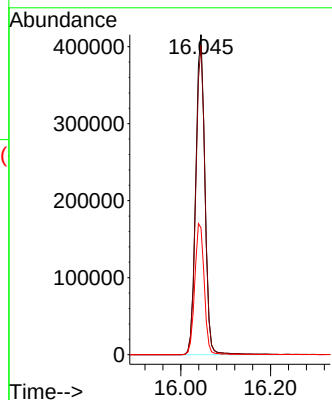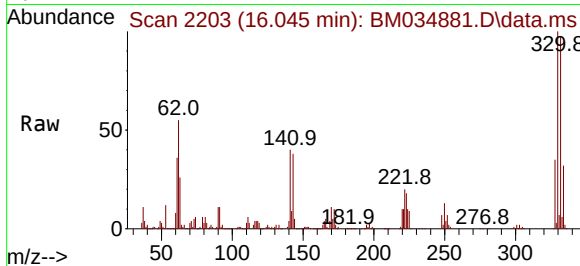

#45
2-Fluorobiphenyl
Concen: 64.938 ng
RT: 13.186 min Scan# 1717
Delta R.T. -0.006 min
Lab File: BM034881.D
Acq: 02 May 2022 20:16

Tgt Ion:172 Resp: 2561633
Ion Ratio Lower Upper
172 100
171 35.7 28.5 42.7
170 23.7 18.7 28.1

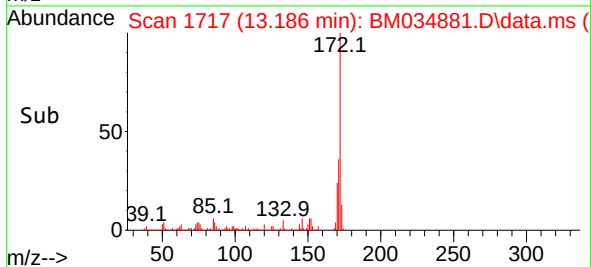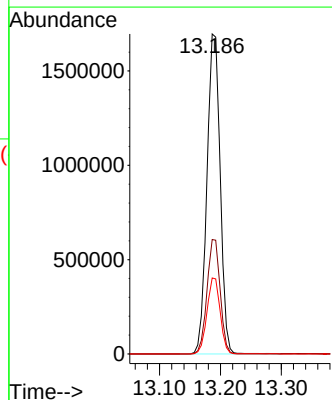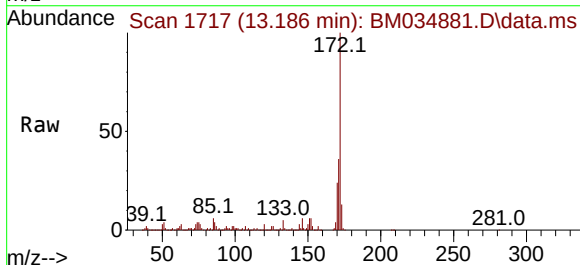

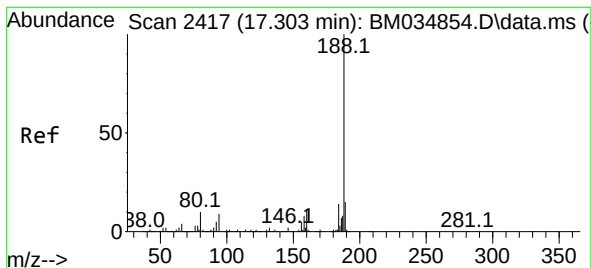

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.298 min Scan# 2416

Delta R.T. -0.006 min

Lab File: BM034881.D

Acq: 02 May 2022 20:16

Instrument :

BNA_M

ClientSampleId :

SB03-13-14-FT





Tgt Ion:188 Resp: 1269427

Ion Ratio Lower Upper

188 100

94 8.7 7.0 10.4

80 9.7 7.6 11.4

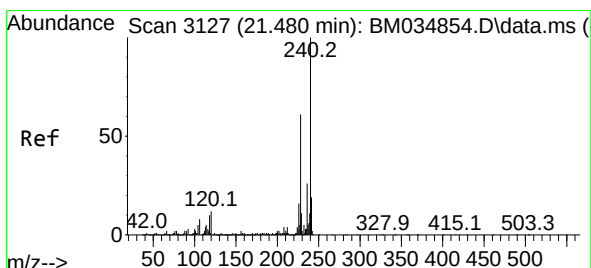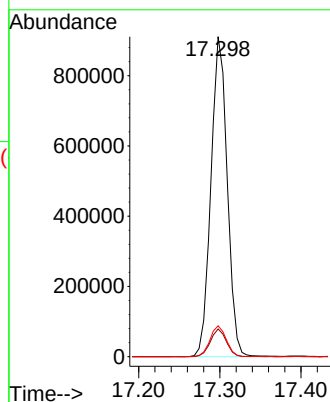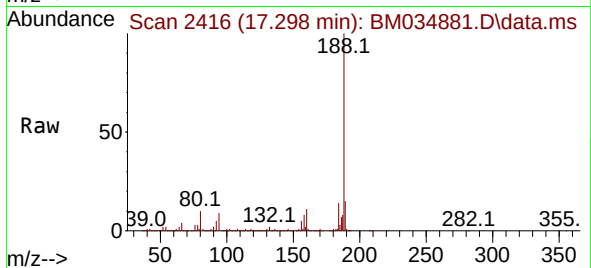

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.474 min Scan# 3126

Delta R.T. -0.006 min

Lab File: BM034881.D

Acq: 02 May 2022 20:16




Tgt Ion:240 Resp: 1392527


Ion Ratio Lower Upper

240 100

120 11.4 9.4 14.0

236 25.9 20.6 30.8


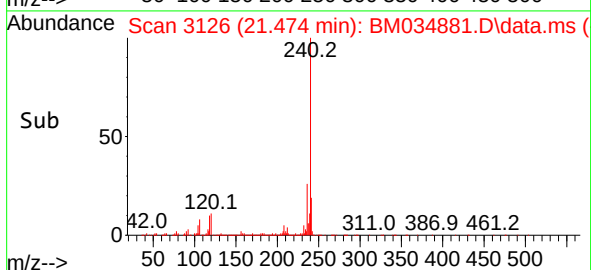
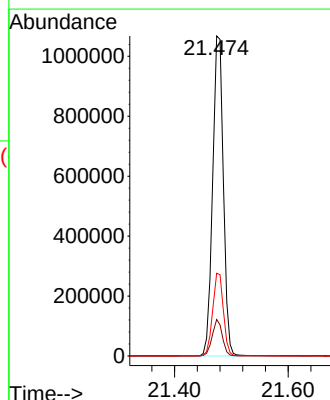





#79
 Terphenyl-d14
 Concen: 67.865 ng
 RT: 19.921 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM034881.D
 Acq: 02 May 2022 20:16

Instrument :
 BNA_M
 ClientSampleId :
 SB03-13-14-FT

Tgt Ion:244 Resp: 4880841
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.2 9.4
 122 10.6 8.3 12.5

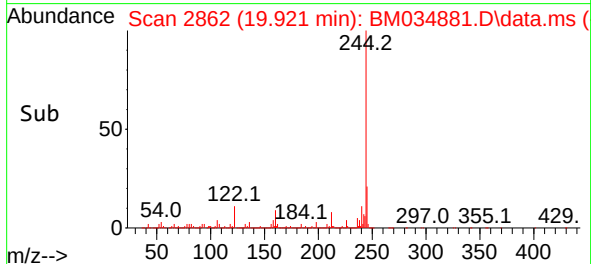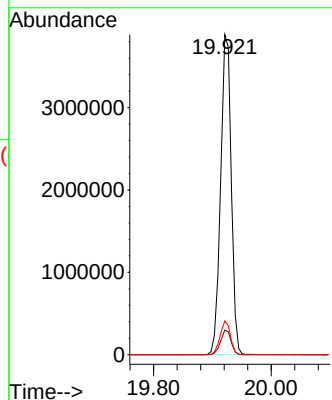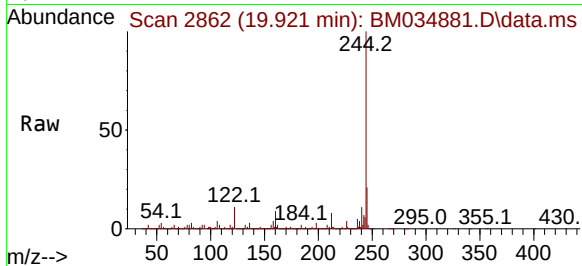

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.868 min Scan# 3533
 Delta R.T. -0.006 min
 Lab File: BM034881.D
 Acq: 02 May 2022 20:16

Tgt Ion:264 Resp: 1288789
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.9 28.3
 265 22.1 17.5 26.3

