

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
 Data File : BM034883.D
 Acq On : 02 May 2022 21:28
 Operator : CG/JU
 Sample : N2619-14
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB06-12-14-FT

Quant Time: May 03 05:22:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 01:51:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	204309	20.000	ng	0.00
21) Naphthalene-d8	10.728	136	845692	20.000	ng	0.00
39) Acenaphthene-d10	14.557	164	571840	20.000	ng	0.00
64) Phenanthrene-d10	17.298	188	1294650	20.000	ng	0.00
76) Chrysene-d12	21.474	240	1384958	20.000	ng	0.00
86) Perylene-d12	23.868	264	1270924	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.505	112	1877745	162.144	ng	0.00
7) Phenol-d6	7.093	99	2465923	164.945	ng	0.00
23) Nitrobenzene-d5	9.087	82	1601833	102.285	ng	0.00
42) 2,4,6-Tribromophenol	16.045	330	1131085	181.833	ng	0.00
45) 2-Fluorobiphenyl	13.192	172	3778725	95.927	ng	0.00
79) Terphenyl-d14	19.927	244	6735935	94.170	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
Data File : BM034883.D
Acq On : 02 May 2022 21:28
Operator : CG/JU
Sample : N2619-14
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB06-12-14-FT

Quant Time: May 03 05:22:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration




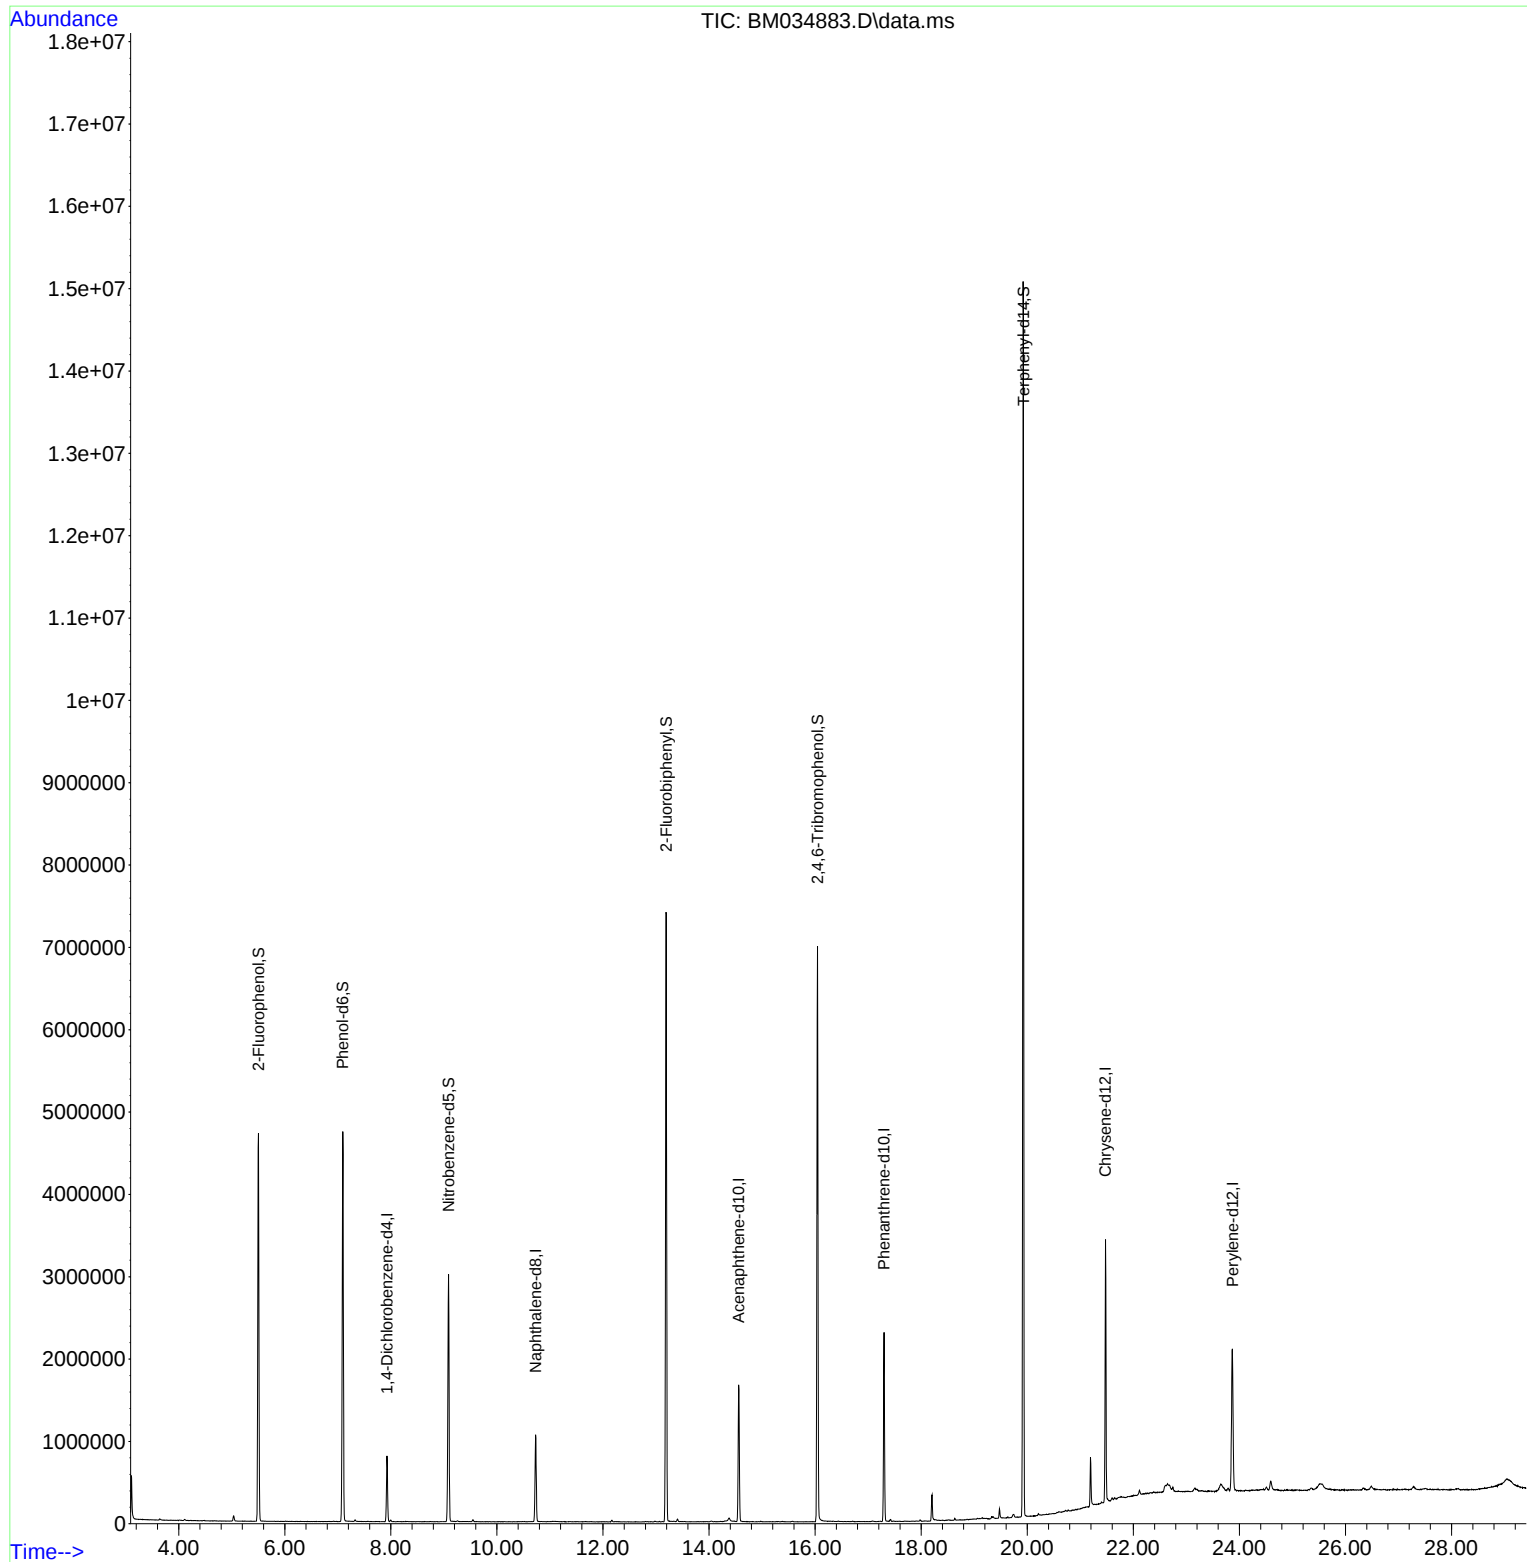




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.928 min Scan# 81
Delta R.T. -0.006 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28




Instrument :
BNA_M
ClientSampleId :
SB06-12-14-FT

Tgt Ion:152 Resp: 204309
Ion Ratio Lower Upper
152 100
150 159.1 124.9 187.3
115 60.8 47.9 71.9

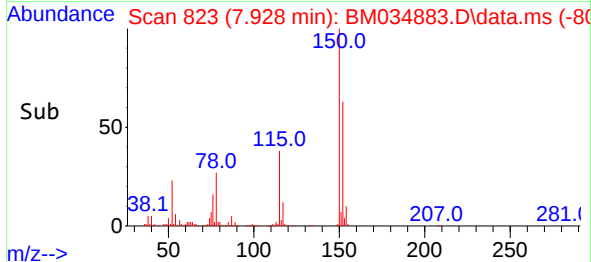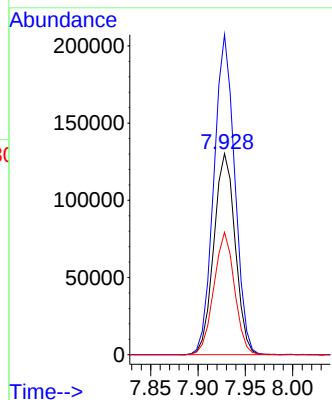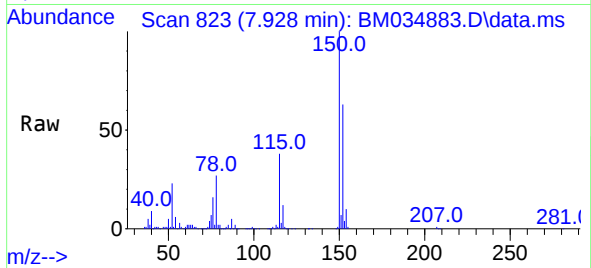

#5
2-Fluorophenol
Concen: 162.144 ng
RT: 5.505 min Scan# 411
Delta R.T. 0.001 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28

Tgt Ion:112 Resp: 1877745
Ion Ratio Lower Upper
112 100
64 59.4 47.8 71.6
63 33.4 26.6 40.0

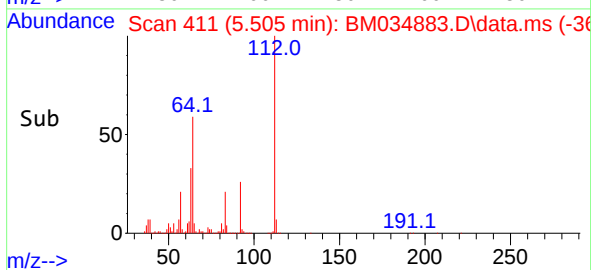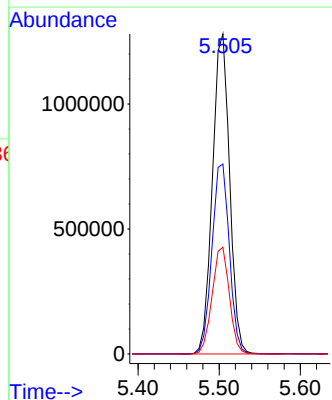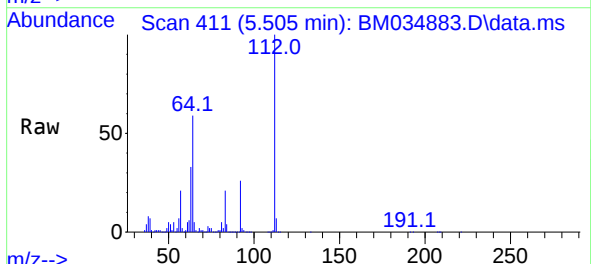







#7
Phenol-d6
Concen: 164.945 ng
RT: 7.093 min Scan# 61
Delta R.T. 0.001 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28

Instrument :
BNA_M
ClientSampleId :
SB06-12-14-FT

Tgt Ion: 99 Resp: 2465923




Ion	Ratio	Lower	Upper
99	100		
42	22.9	18.8	28.2
71	38.1	30.2	45.2

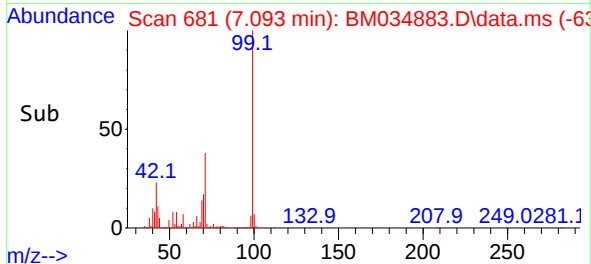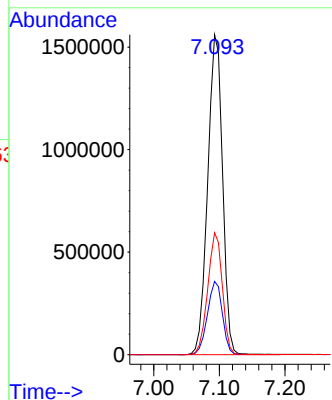


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.728 min Scan# 1299
Delta R.T. -0.005 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28

Tgt Ion: 136 Resp: 845692

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	8.3	7.0	10.4
68	5.6	4.3	6.5


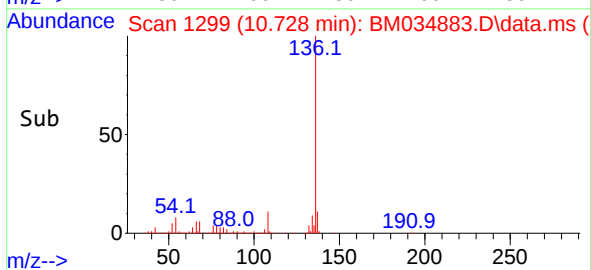
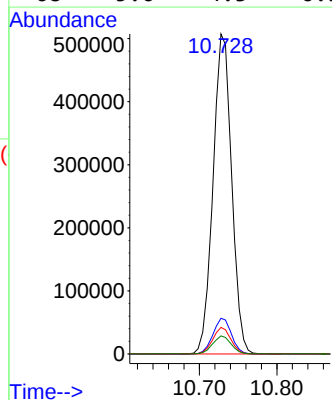
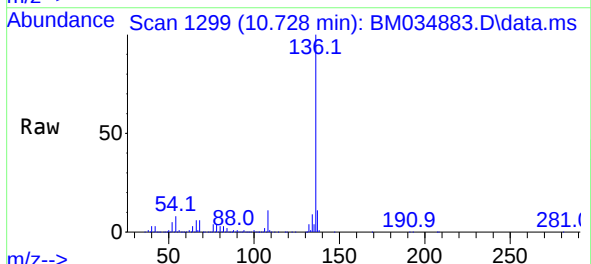




#23
Nitrobenzene-d5
Concen: 102.285 ng
RT: 9.087 min Scan# 1020
Delta R.T. -0.005 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28




Instrument :
BNA_M
ClientSampleId :
SB06-12-14-FT


Tgt Ion: 82 Resp: 1601833
Ion Ratio Lower Upper
82 100
128 42.7 33.7 50.5
54 54.2 43.2 64.8

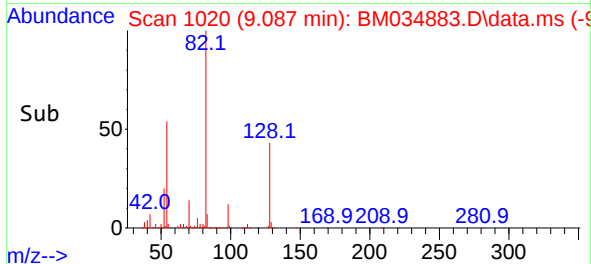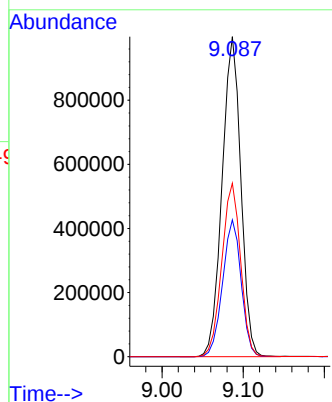

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.557 min Scan# 1950
Delta R.T. -0.005 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28

Tgt Ion:164 Resp: 571840
Ion Ratio Lower Upper
164 100
162 104.4 83.0 124.6
160 45.7 37.0 55.4


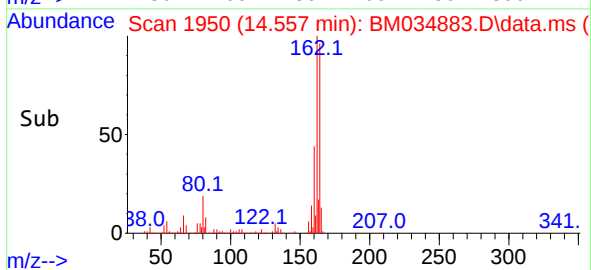
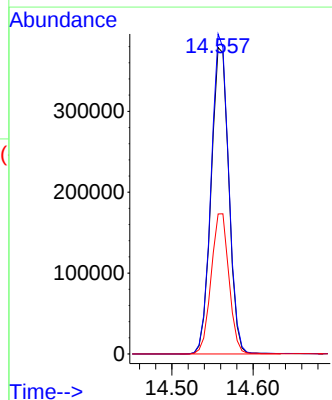
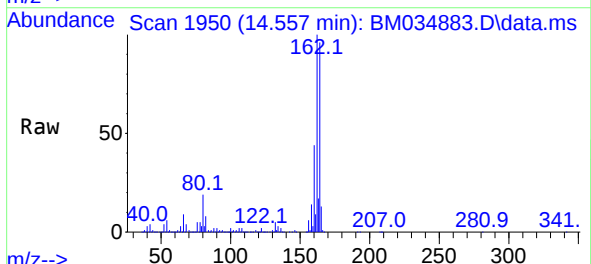


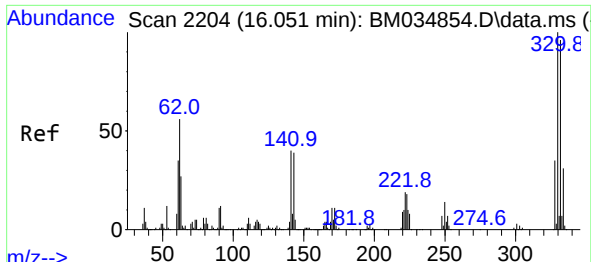

#42
2,4,6-Tribromophenol
Concen: 181.833 ng
RT: 16.045 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28




Instrument :
BNA_M
ClientSampleId :
SB06-12-14-FT


Tgt Ion:330 Resp: 1131085
Ion Ratio Lower Upper
330 100
332 96.6 77.0 115.4
141 41.1 35.3 52.9

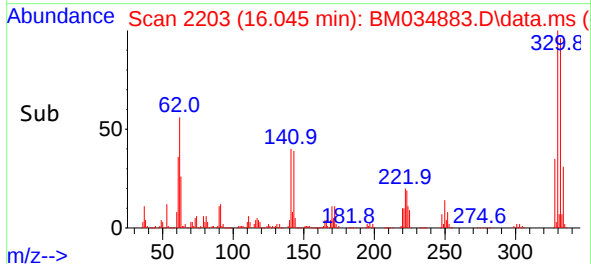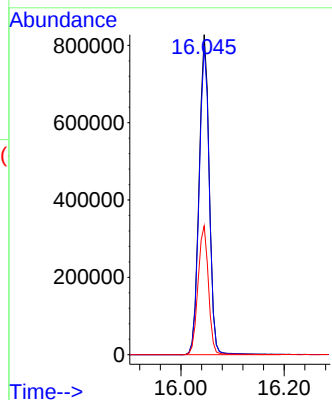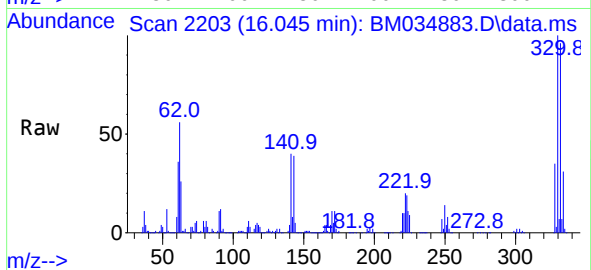

#45
2-Fluorobiphenyl
Concen: 95.927 ng
RT: 13.192 min Scan# 1718
Delta R.T. 0.000 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28

Tgt Ion:172 Resp: 3778725
Ion Ratio Lower Upper
172 100
171 35.5 28.5 42.7
170 23.7 18.7 28.1


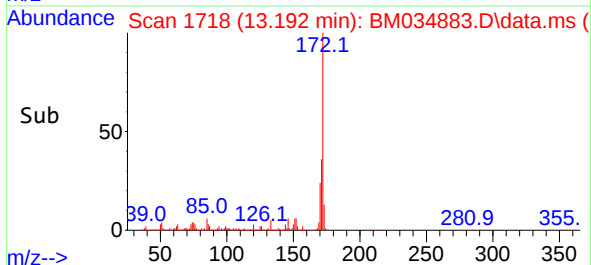
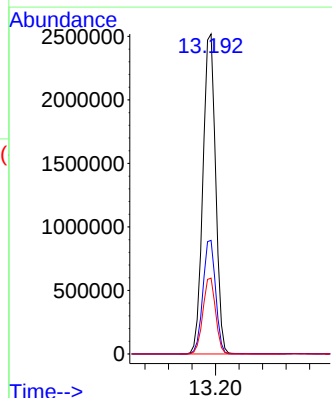
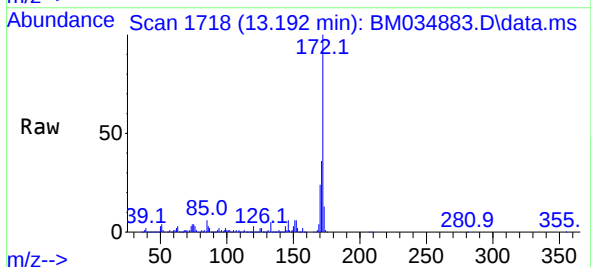




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.298 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28




Instrument :
BNA_M
ClientSampleId :
SB06-12-14-FT


Tgt Ion:188 Resp: 1294650
Ion Ratio Lower Upper
188 100
94 8.4 7.0 10.4
80 9.8 7.6 11.4

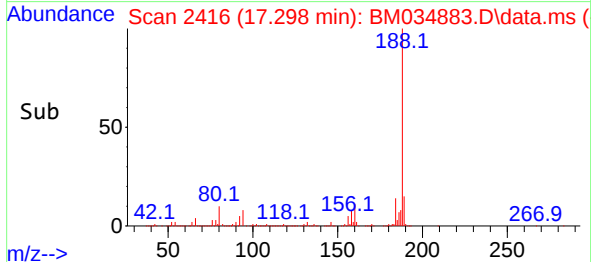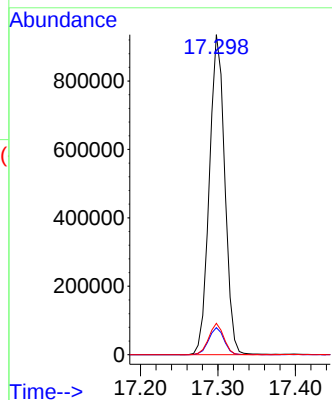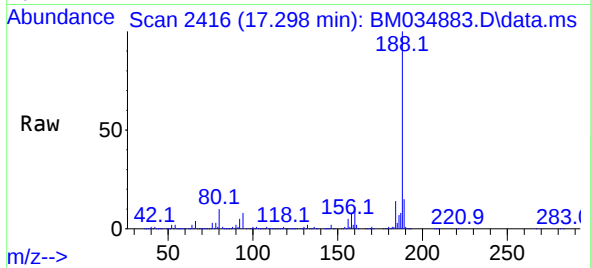

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.474 min Scan# 3126
Delta R.T. -0.006 min
Lab File: BM034883.D
Acq: 02 May 2022 21:28

Tgt Ion:240 Resp: 1384958
Ion Ratio Lower Upper
240 100
120 11.0 9.4 14.0
236 26.1 20.6 30.8


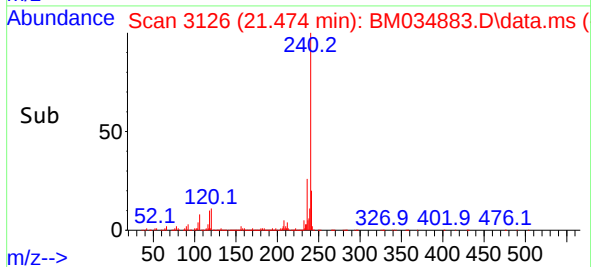
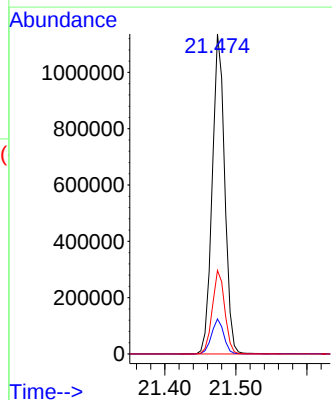
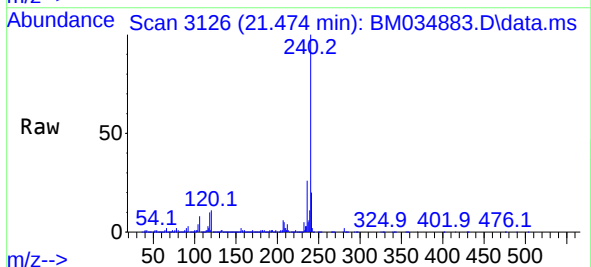




#79
 Terphenyl-d14
 Concen: 94.170 ng
 RT: 19.927 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM034883.D
 Acq: 02 May 2022 21:28

Instrument :
 BNA_M
 ClientSampleId :
 SB06-12-14-FT

Tgt Ion:244 Resp: 6735935
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.4
 122 9.6 8.3 12.5

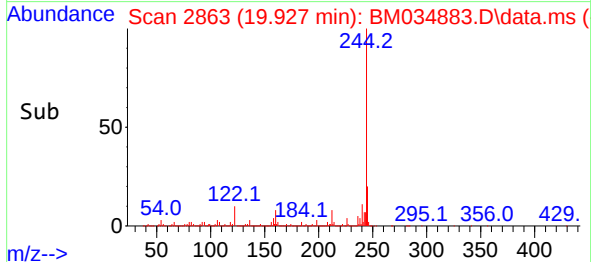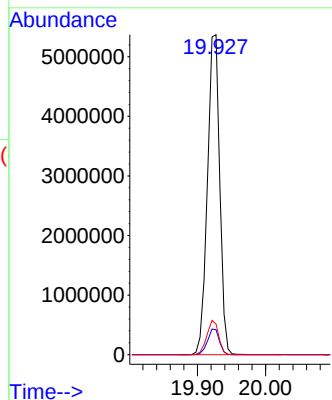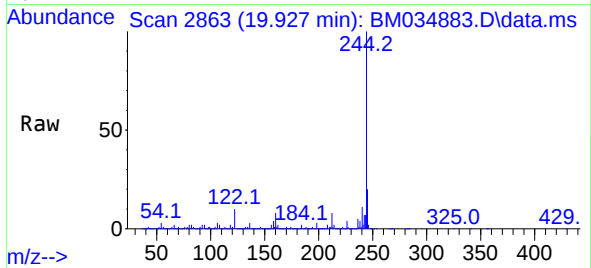

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.868 min Scan# 3533
 Delta R.T. -0.006 min
 Lab File: BM034883.D
 Acq: 02 May 2022 21:28

Tgt Ion:264 Resp: 1270924
 Ion Ratio Lower Upper
 264 100
 260 24.0 18.9 28.3
 265 21.8 17.5 26.3

