

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
 Data File : BM034870.D
 Acq On : 02 May 2022 11:40
 Operator : CG/JU
 Sample : PB144493BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB144493BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	404	411	421	rBV	5796493	8214777	40.95%	9.923%
2	7.098	673	682	695	rBV	5407462	8755338	43.65%	10.576%
3	7.928	816	823	832	rVB	991718	1543331	7.69%	1.864%
4	9.086	1012	1020	1033	rBV	3396175	5623487	28.03%	6.793%
5	10.733	1291	1300	1312	rVB	1267575	2154024	10.74%	2.602%
6	13.192	1710	1718	1734	rBV	9296969	13251778	66.06%	16.007%
7	14.563	1943	1951	1964	rBV	1940474	2924364	14.58%	3.532%
8	16.045	2196	2203	2223	rBV	7211054	10138412	50.54%	12.246%
9	17.298	2410	2416	2424	rBV	2386243	3505712	17.48%	4.235%
10	19.927	2857	2863	2868	rBV	16599969	20059996	100.00%	24.231%
11	21.480	3121	3127	3133	rBV	2785035	3556233	17.73%	4.296%
12	23.868	3526	3533	3545	rVB2	1558905	3058865	15.25%	3.695%




Sum of corrected areas: 82786317

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
Data File : BM034870.D
Acq On : 02 May 2022 11:40
Operator : CG/JU
Sample : PB144493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144493BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

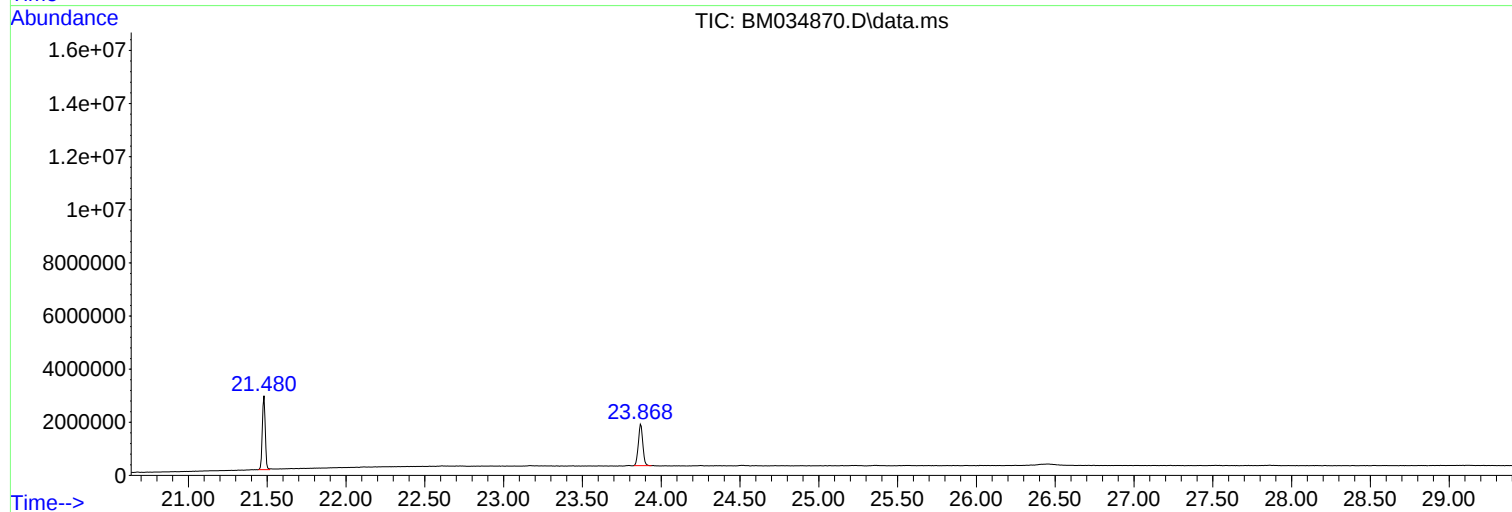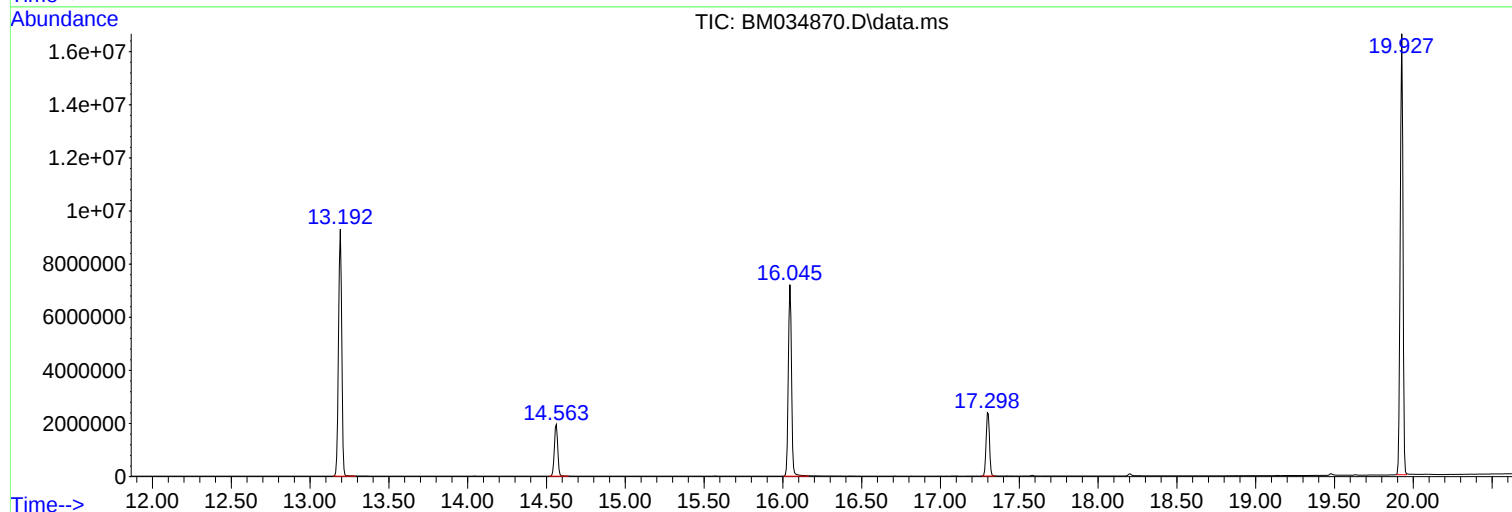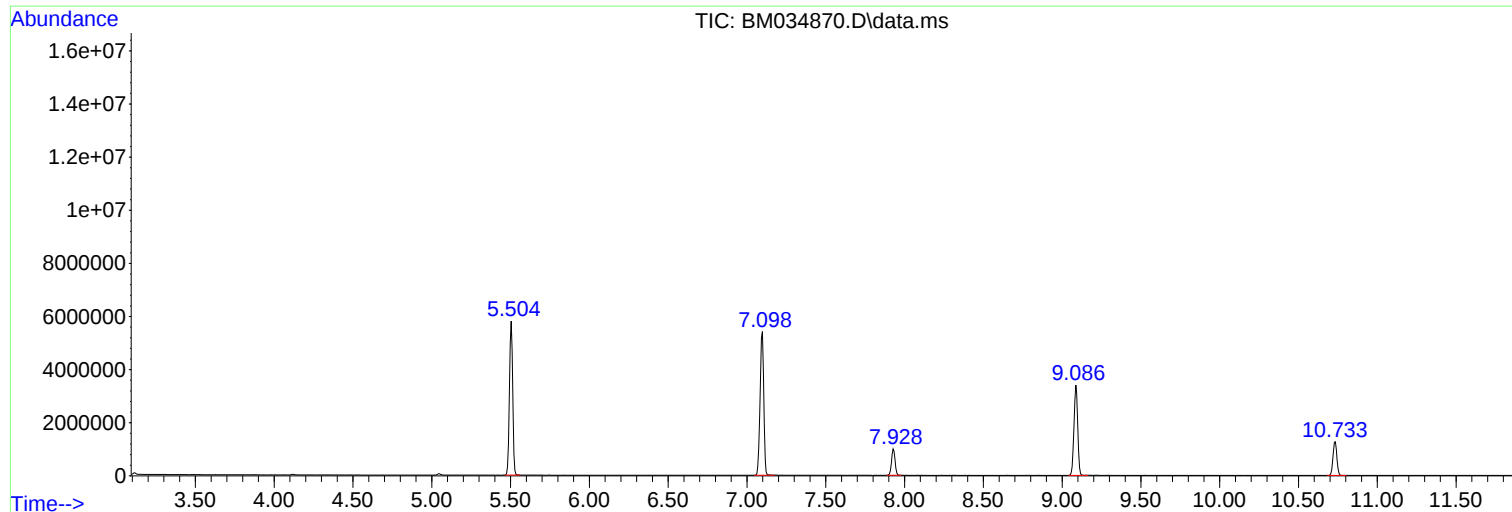

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
Data File : BM034870.D
Acq On : 02 May 2022 11:40
Operator : CG/JU
Sample : PB144493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144493BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
Data File : BM034870.D
Acq On : 02 May 2022 11:40
Operator : CG/JU
Sample : PB144493BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144493BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------