
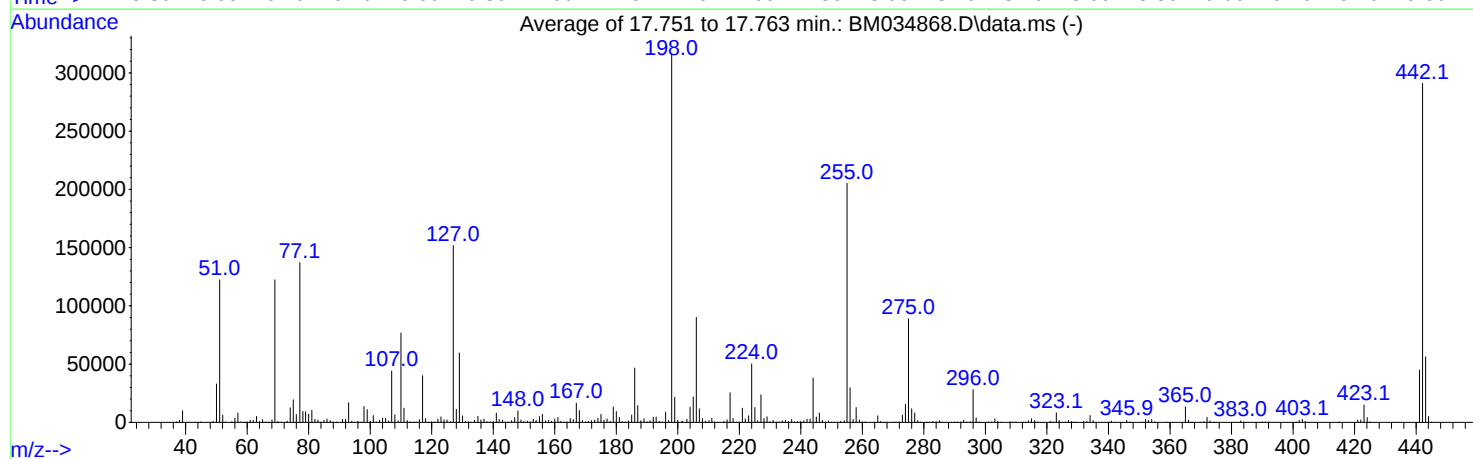


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
 Data File : BM034868.D
 Acq On : 02 May 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 01:51:59 2022

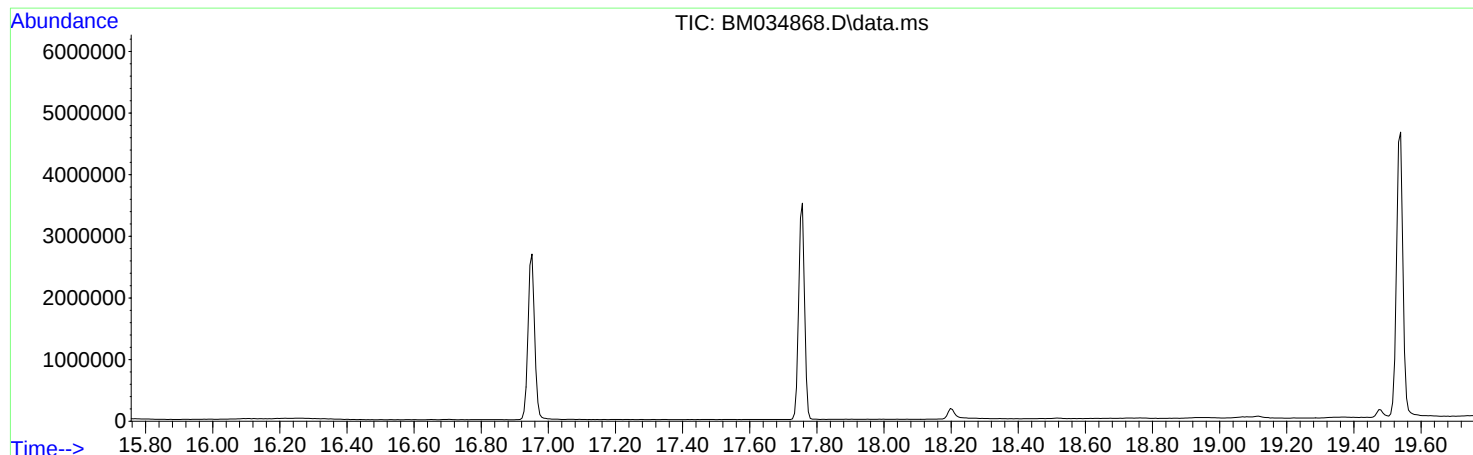




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	122281	PASS
68	69	0.00	2	1.9	2264	PASS
69	198	0.00	100	38.7	122346	PASS
70	69	0.00	2	0.6	757	PASS
127	198	10	80	48.1	151779	PASS
197	198	0.00	2	0.5	1611	PASS
198	198	100	100	100.0	315776	PASS
199	198	5	9	6.8	21585	PASS
275	198	10	60	28.1	88853	PASS
365	198	1	100	4.2	13248	PASS
441	198	0.01	100	14.2	44899	PASS
442	442	50	100	100.0	290987	PASS
443	442	15	24	19.3	56157	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
 Data File : BM034868.D
 Acq On : 02 May 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 03 06:33:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 01:51:59 2022
 Response via : Initial Calibration

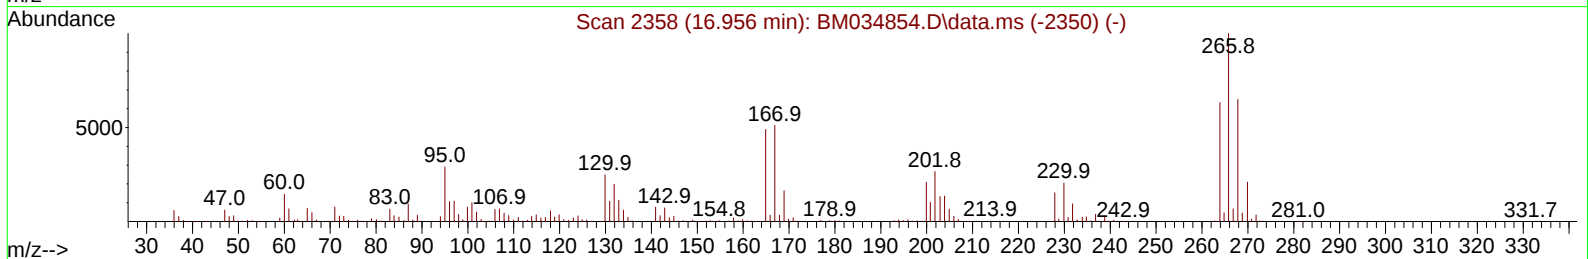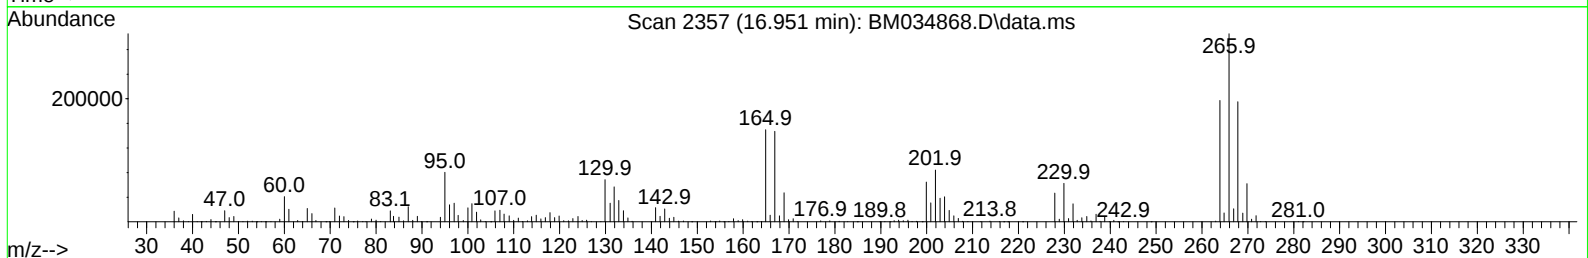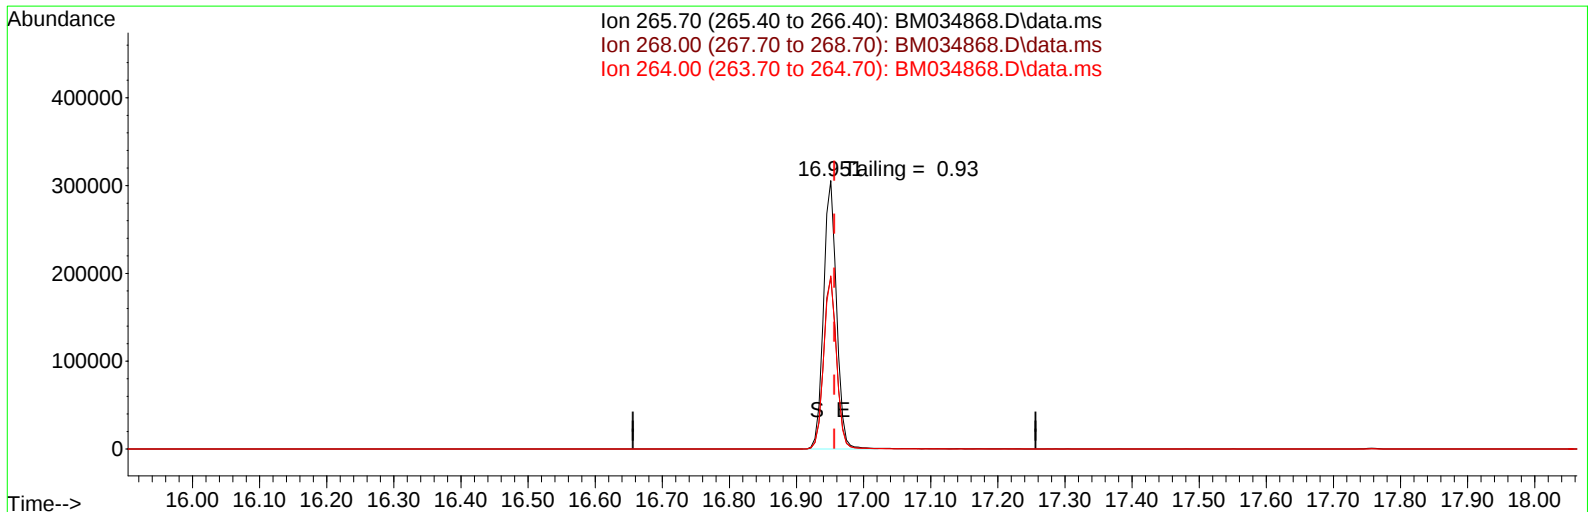

TIC: BM034868.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.005) 0.00 ng




response 411343

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.84
264.00	63.30	64.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050222\
Data File : BM034868.D
Acq On : 02 May 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 03 06:33:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

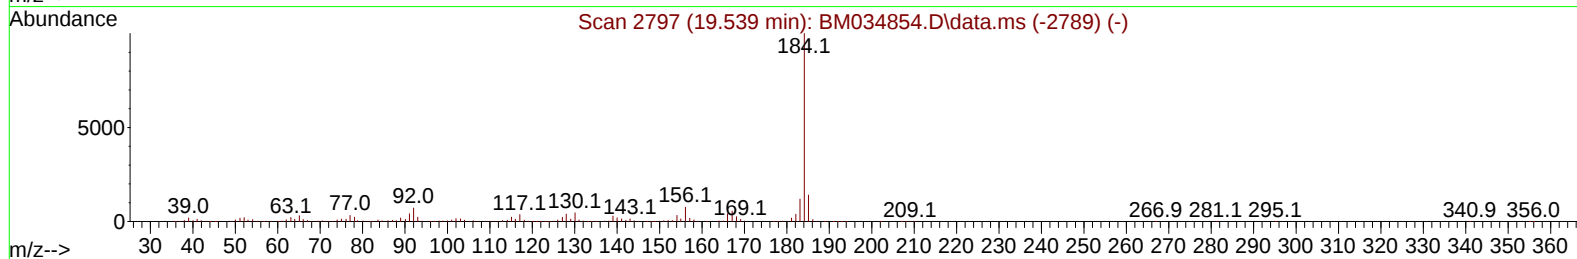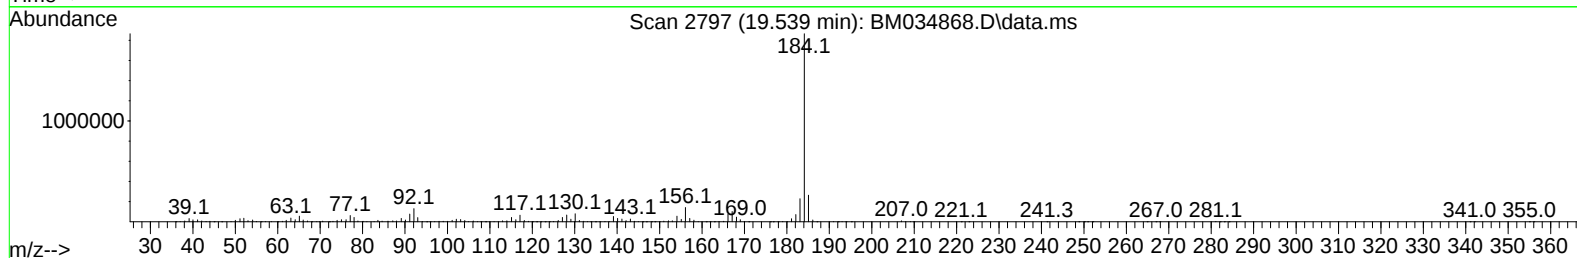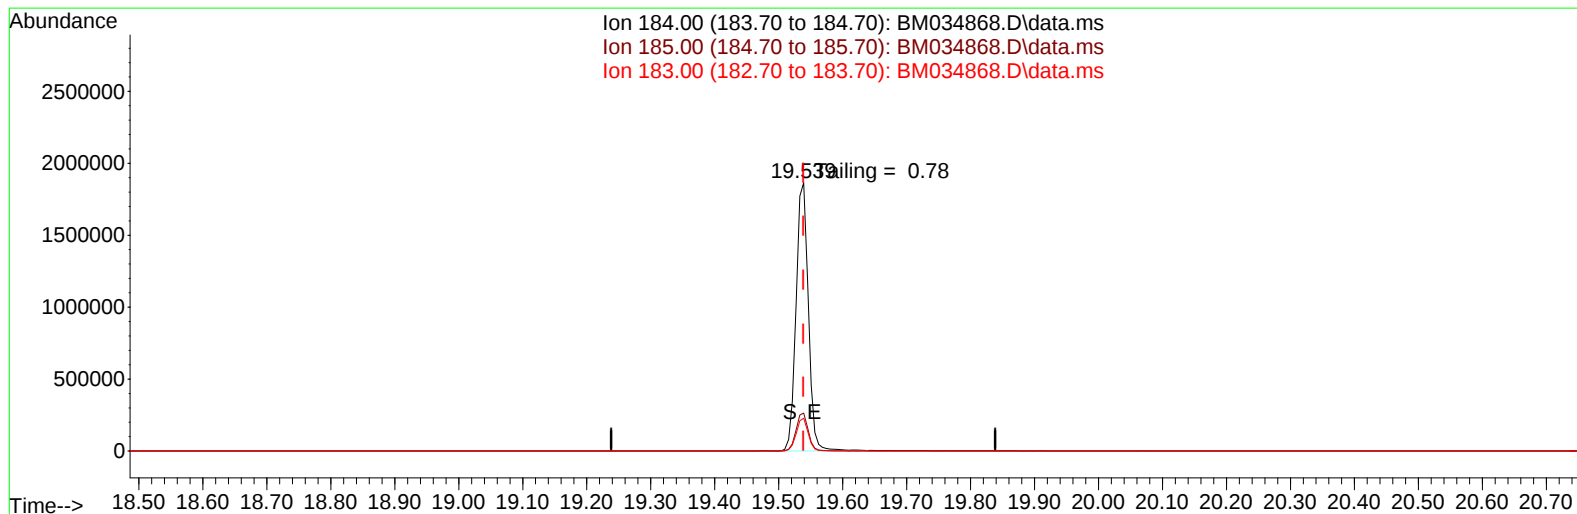

TIC: BM034868.D\data.ms

(77) Benzidine

19.539min (+ 0.000) 155694.46 ng

response 2511360

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.17
183.00	11.90	12.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/2/2022	BNA_M	<u>BM034868.D</u>
Compound Name	Response	Retention Time
DDT	1294187	20.78
DDD	14951	20.339
DDE	1131	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16082	1310269	1.23

Instrument :
BNA_M
ClientSampleId :
DFTPP