
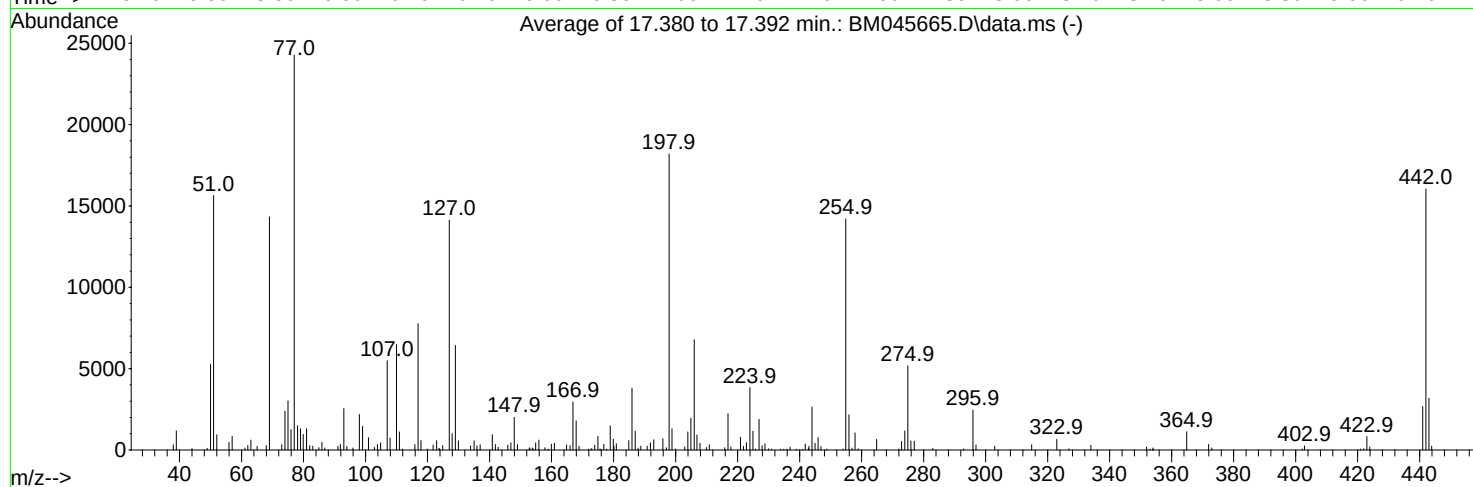


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050224\
Data File : BM045665.D
Acq On : 02 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

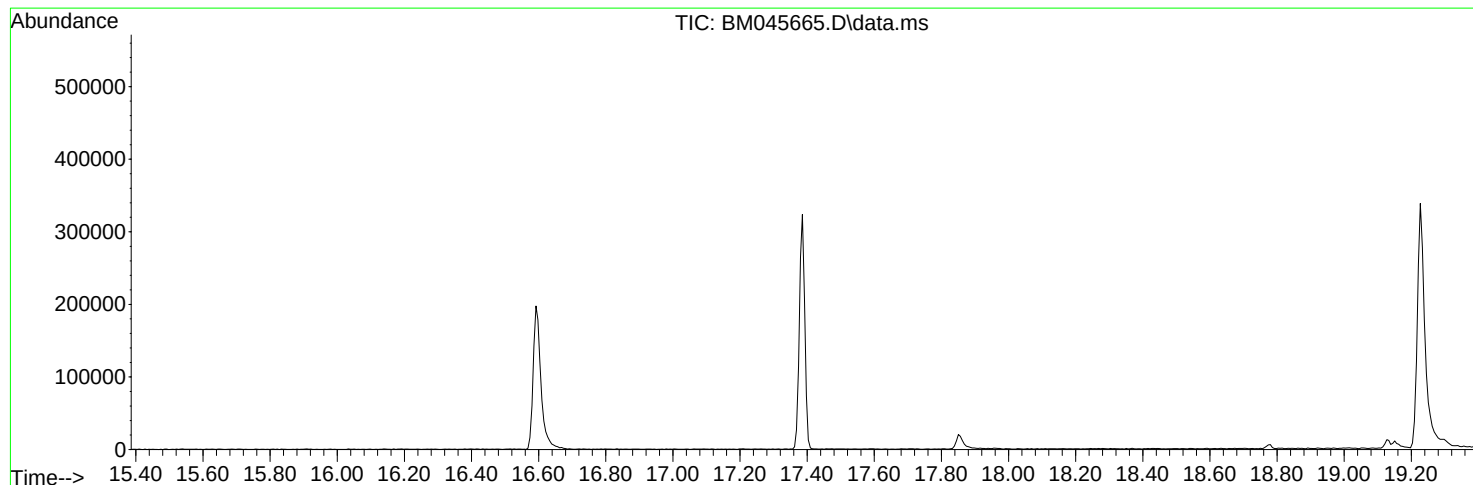




AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2424

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	271	PASS
69	69	100	100	100.0	14327	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.8	141	PASS
198	198	100	100	100.0	18191	PASS
199	198	5	9	7.2	1304	PASS
365	198	1	100	6.2	1120	PASS
441	443	0.01	150	84.1	2676	PASS
442	442	100	100	100.0	16047	PASS
443	442	15	24	19.8	3182	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050224\
Data File : BM045665.D
Acq On : 02 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 02 12:47:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 06:17:41 2024
Response via : Initial Calibration

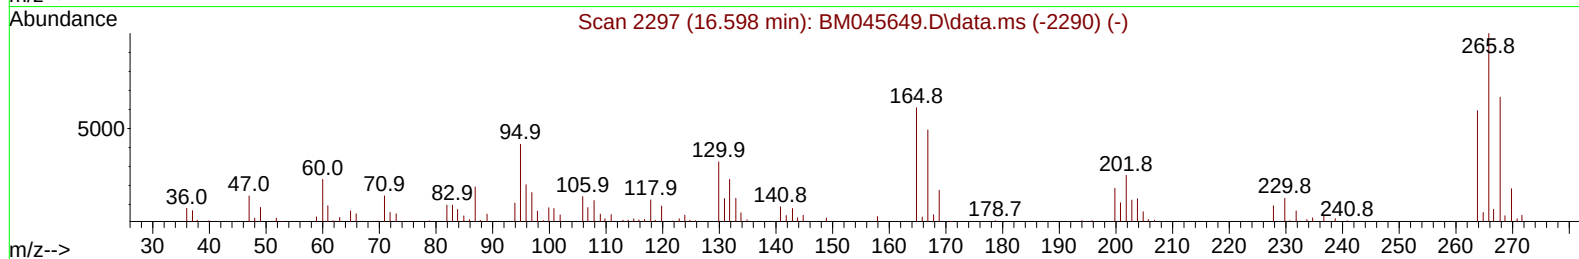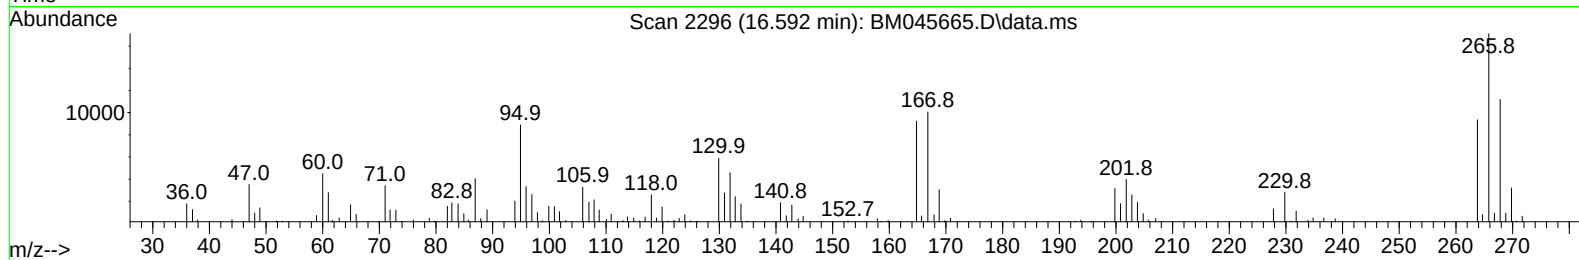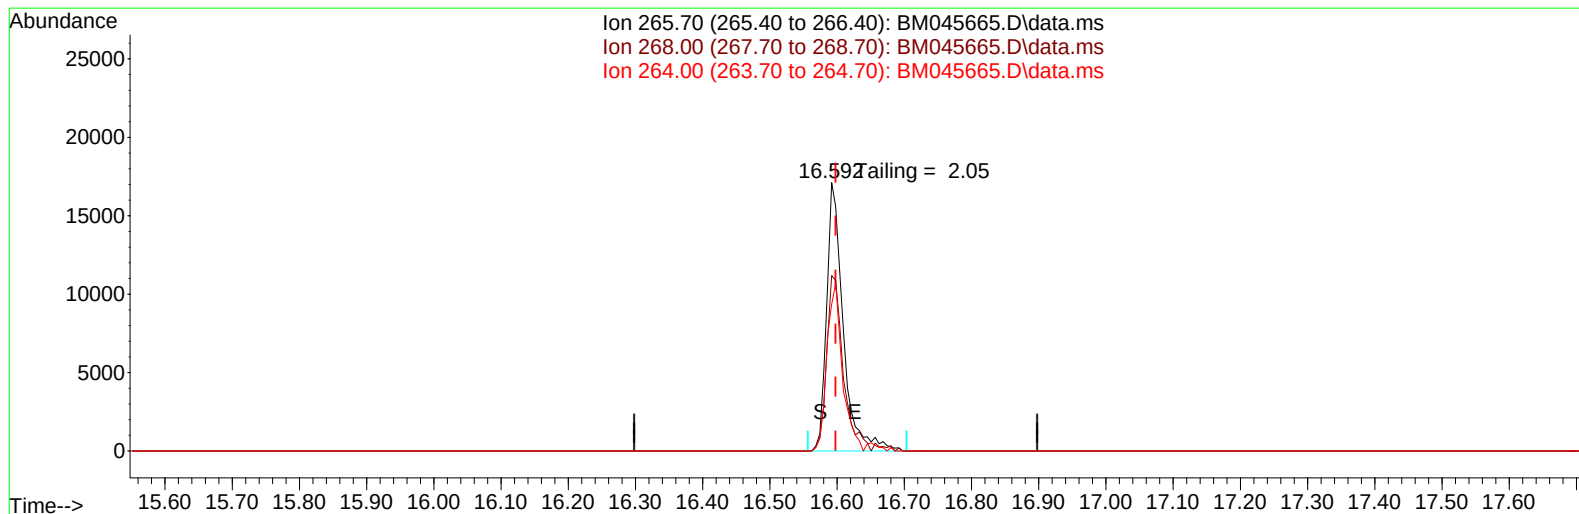

TIC: BM045665.D\data.ms

(70) Pentachlorophenol (C)

16.592min (-0.006) 0.00 ng




response 29516

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.70	65.32
264.00	59.40	59.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050224\
Data File : BM045665.D
Acq On : 02 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 02 12:47:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 06:17:41 2024
Response via : Initial Calibration

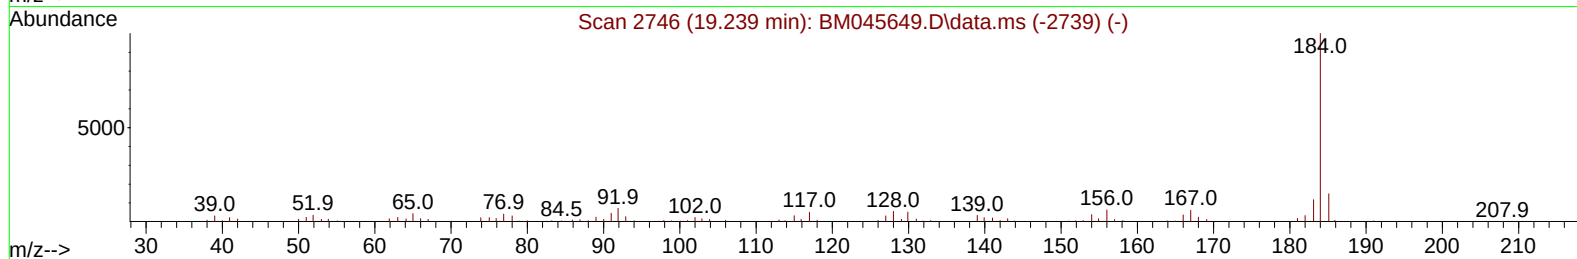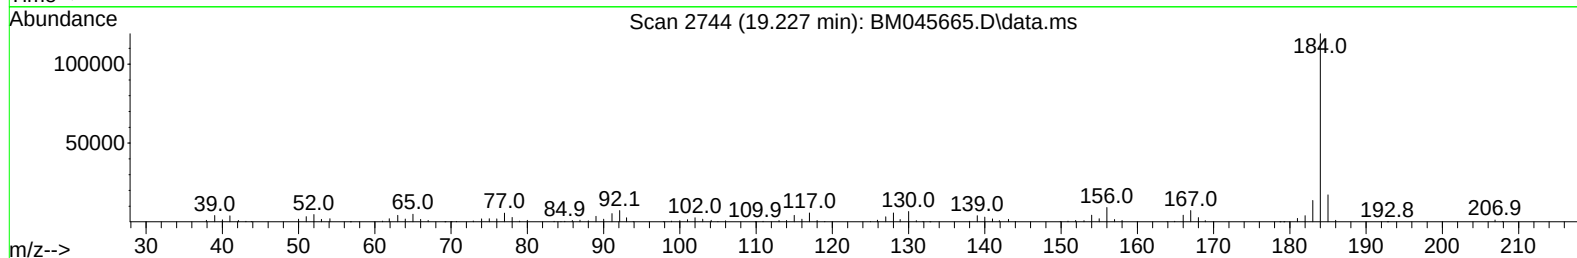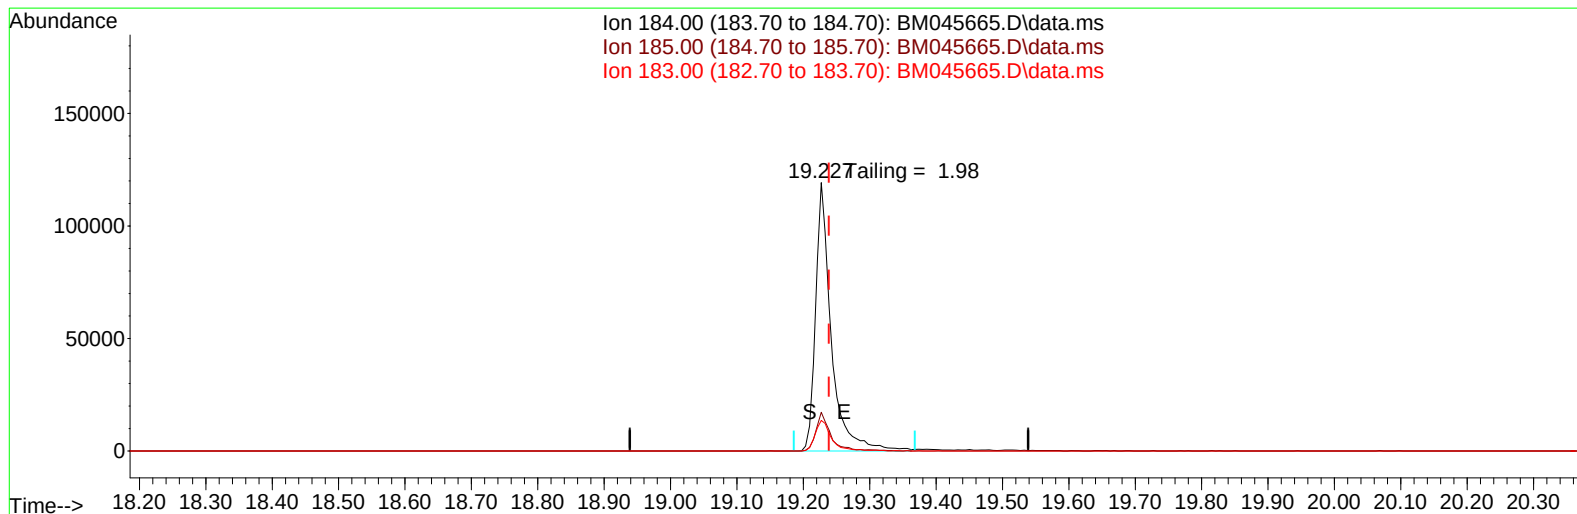

TIC: BM045665.D\data.ms

(77) Benzidine

19.227min (-0.012) 0.00 ng

response 196729

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.42
183.00	11.70	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/1/2024	BNA_M	<u>BM045665.D</u>
Compound Name	Response	Retention Time
DDT	89123	20.45
DDD	1498	20.021
DDE	57	19.498
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1555	90678	1.71

Instrument :
BNA_M
ClientSampleId :
DFTPP