

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
 Data File : BM050092.D
 Acq On : 02 May 2025 19:15
 Operator : RC/JU
 Sample : Q1923-01 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MH-MM

Quant Time: May 02 23:58:42 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	419640	20.000	ng	-0.02
21) Naphthalene-d8	10.539	136	1602264	20.000	ng	-0.02
39) Acenaphthene-d10	14.392	164	1141987	20.000	ng	-0.02
64) Phenanthrene-d10	17.145	188	2403893	20.000	ng	-0.01
76) Chrysene-d12	21.386	240	1726548	20.000	ng	-0.01
86) Perylene-d12	24.380	264	1526163	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	988861	41.263	ng	-0.02
7) Phenol-d6	6.934	99	1530093	50.799	ng	-0.02
23) Nitrobenzene-d5	8.904	82	787067	24.206	ng	-0.02
42) 2,4,6-Tribromophenol	15.892	330	963515	57.061	ng	-0.01
45) 2-Fluorobiphenyl	13.010	172	2535834	26.269	ng	-0.02
79) Terphenyl-d14	19.768	244	4538501	38.897	ng	-0.01
Target Compounds						
56) 4-Nitrophenol	14.692	139	296	4.555	ng	Qvalue # 73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050092.D
Acq On : 02 May 2025 19:15
Operator : RC/JU
Sample : Q1923-01 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MH-MM


Quant Time: May 02 23:58:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

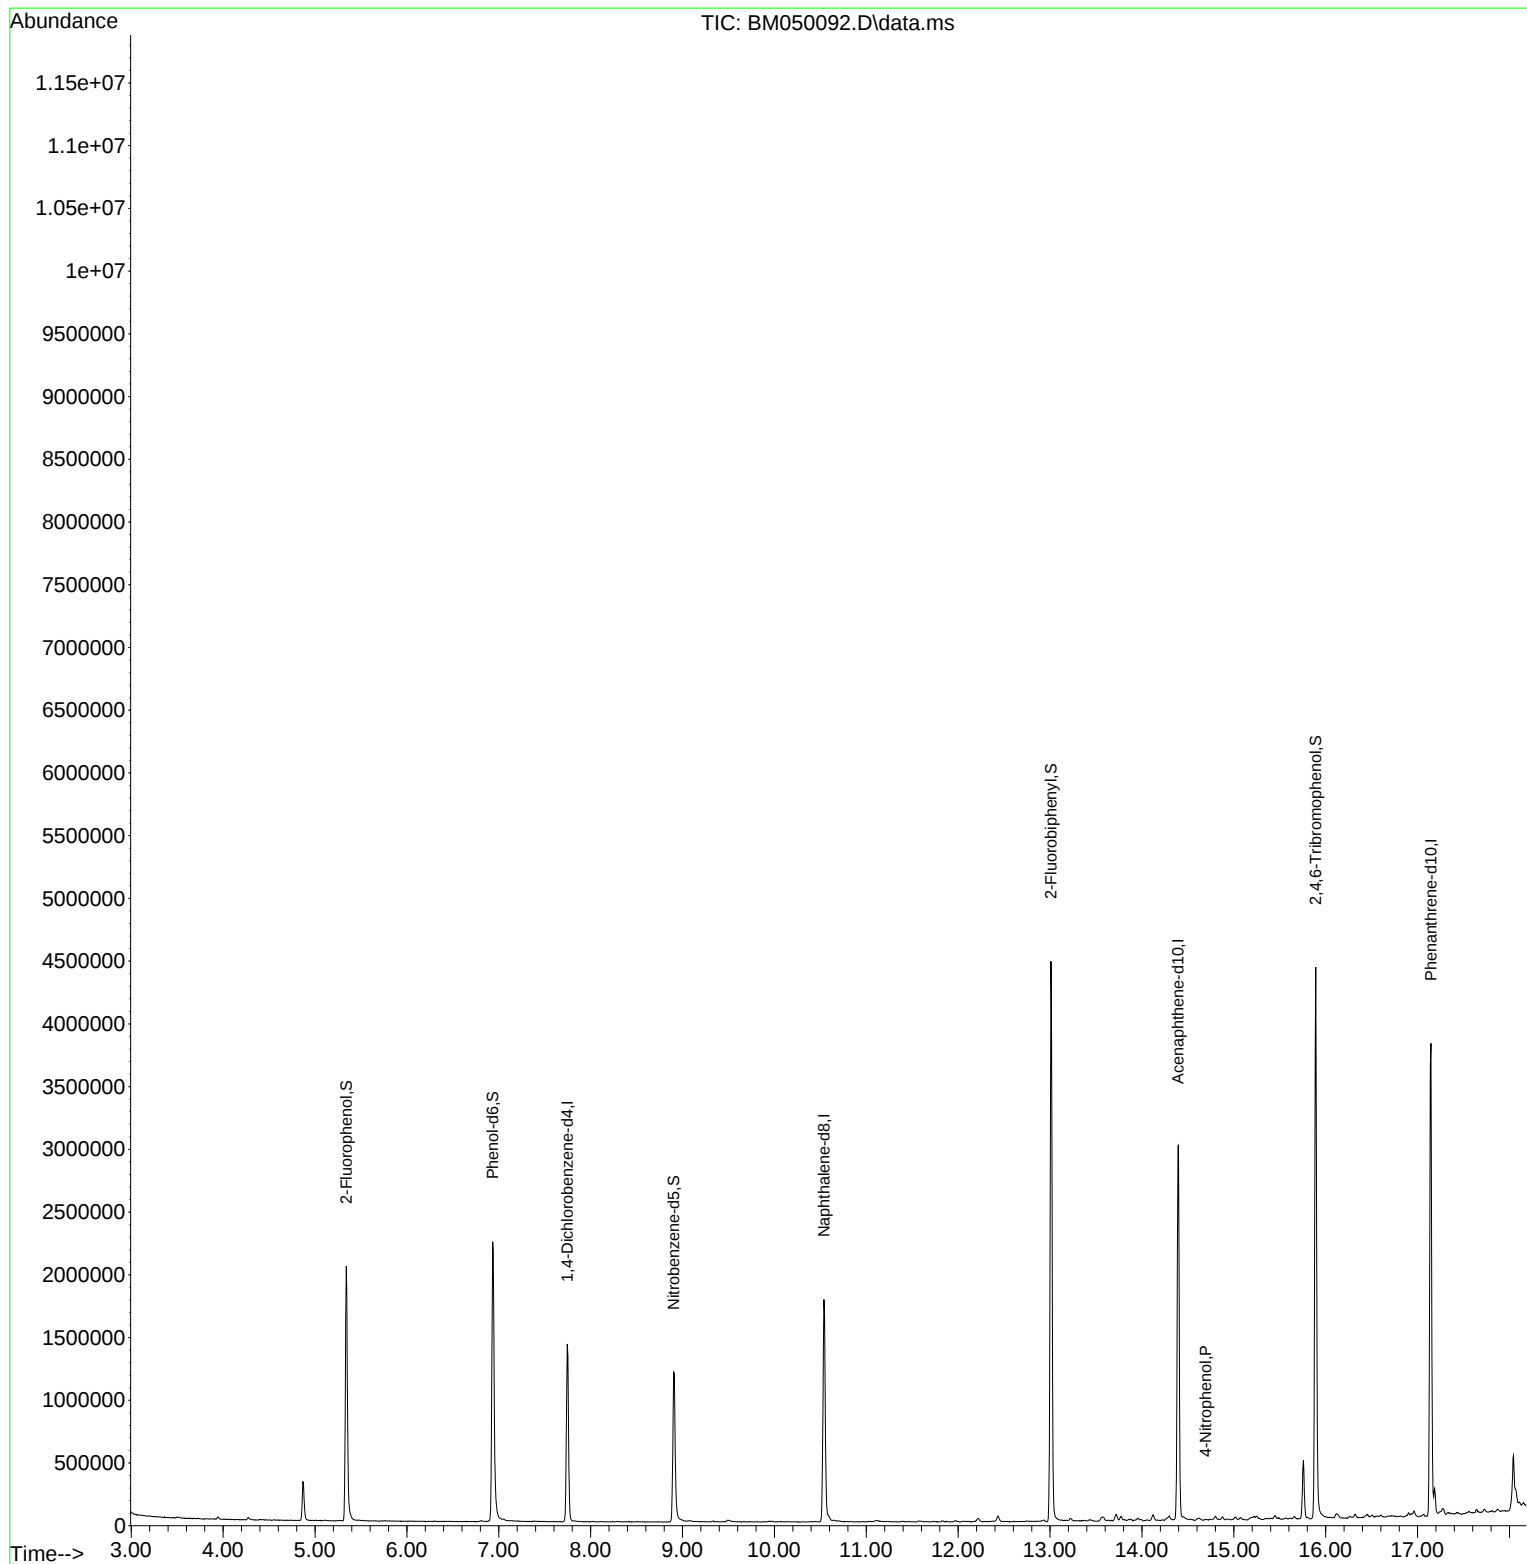

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050092.D
Acq On : 02 May 2025 19:15
Operator : RC/JU
Sample : Q1923-01 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MH-MM

Quant Time: May 02 23:58:42 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration




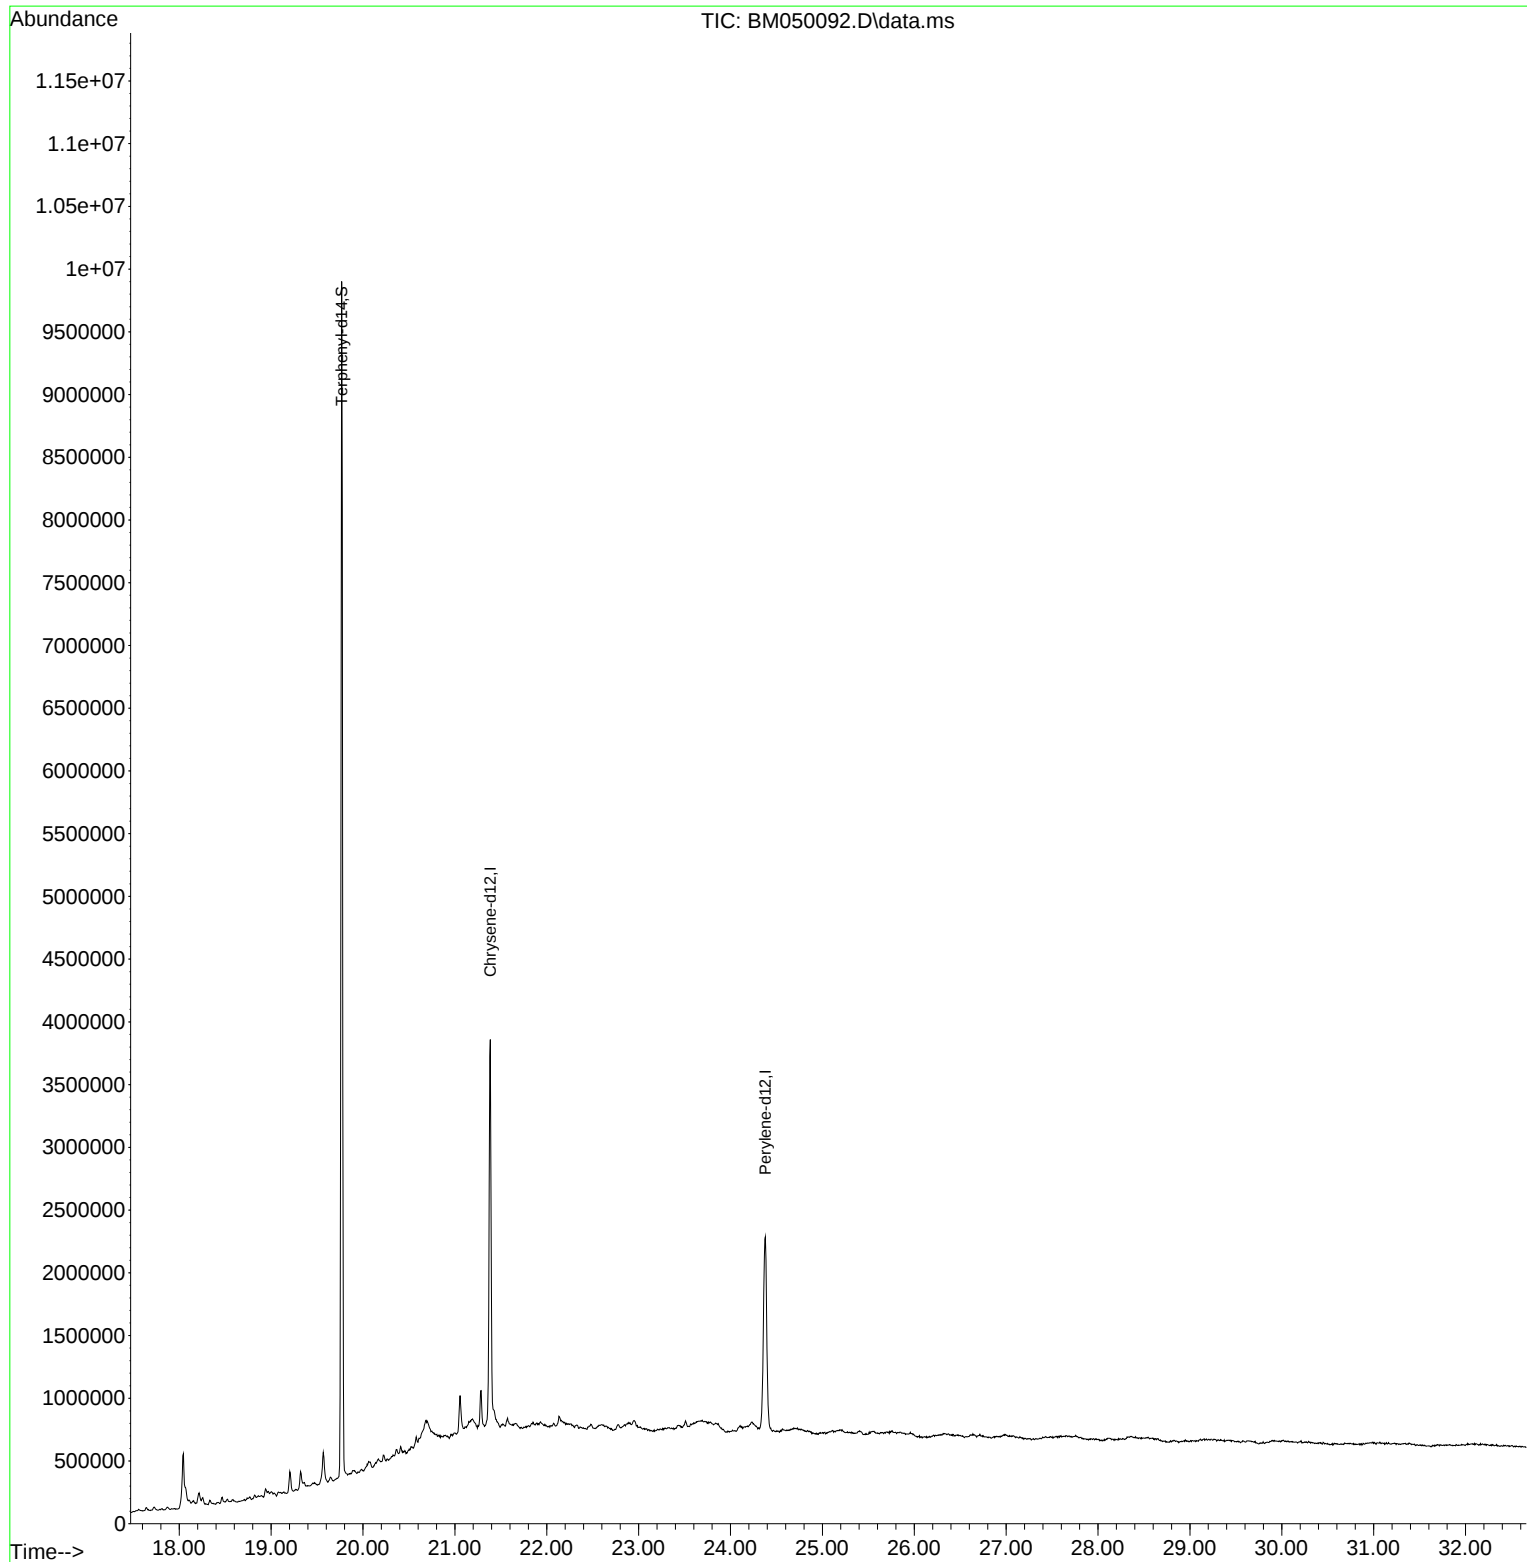




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.745 min Scan# 80
Delta R.T. -0.024 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15




Instrument :
BNA_M
ClientSampleId :
MH-MM


Tgt Ion:152 Resp: 419640
Ion Ratio Lower Upper
152 100
150 155.9 124.1 186.1
115 52.5 41.2 61.8

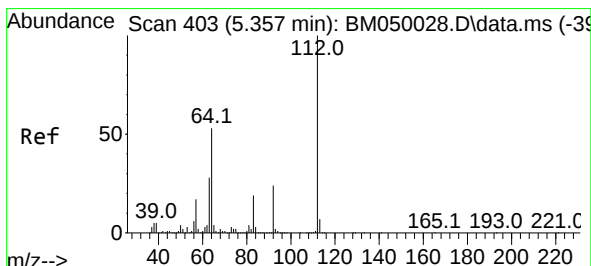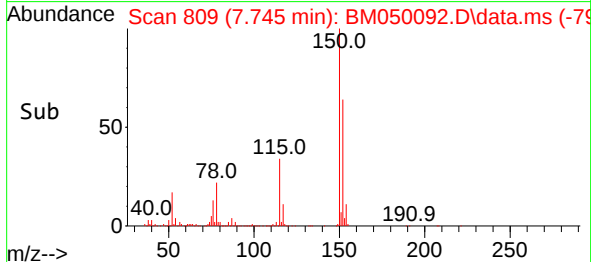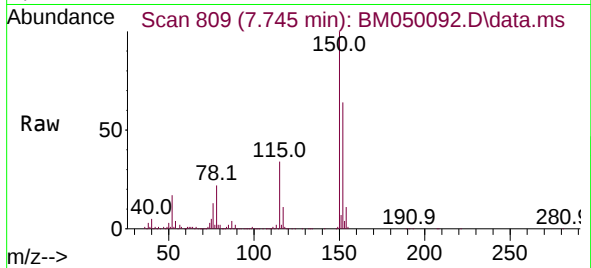

#5
2-Fluorophenol
Concen: 41.263 ng
RT: 5.340 min Scan# 400
Delta R.T. -0.018 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Tgt Ion:112 Resp: 988861
Ion Ratio Lower Upper
112 100
64 52.4 42.6 64.0
63 27.8 22.2 33.4


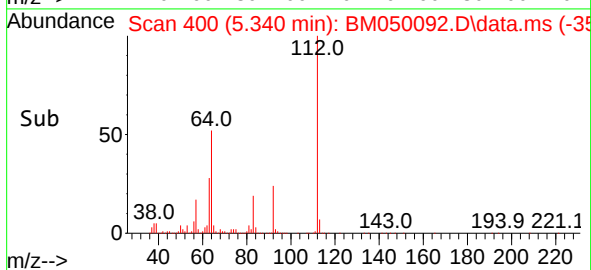

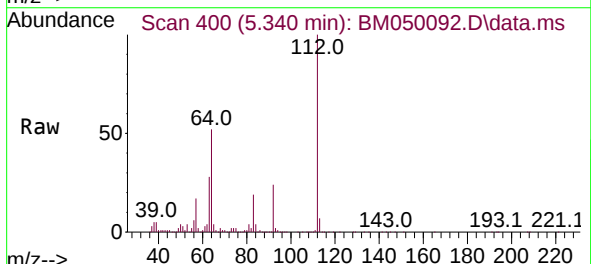


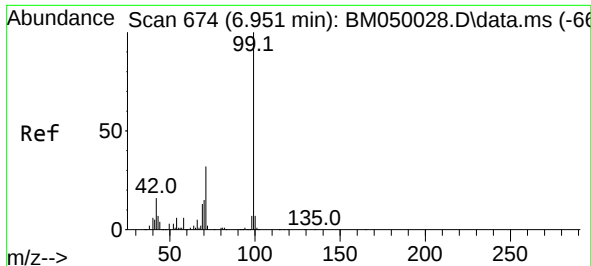

#7
Phenol-d6
Concen: 50.799 ng
RT: 6.934 min Scan# 61
Delta R.T. -0.018 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15




Instrument :
BNA_M
ClientSampleId :
MH-MM


Tgt Ion: 99 Resp: 1530093
Ion Ratio Lower Upper
99 100
42 15.6 13.0 19.4
71 31.5 25.6 38.4

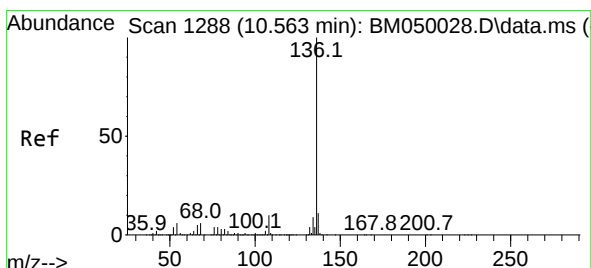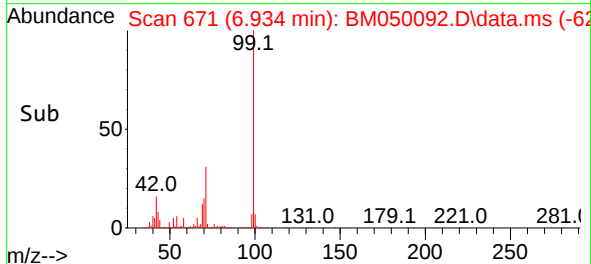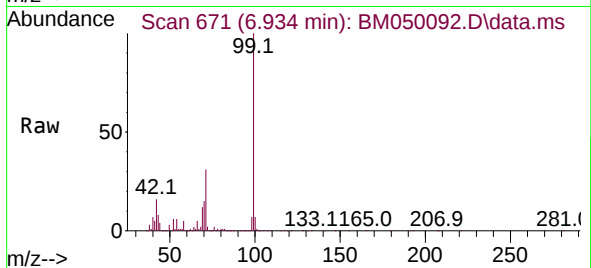

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.539 min Scan# 1284
Delta R.T. -0.024 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Tgt Ion: 136 Resp: 1602264
Ion Ratio Lower Upper
136 100
137 11.3 8.9 13.3
54 6.6 5.1 7.7
68 5.4 4.4 6.6


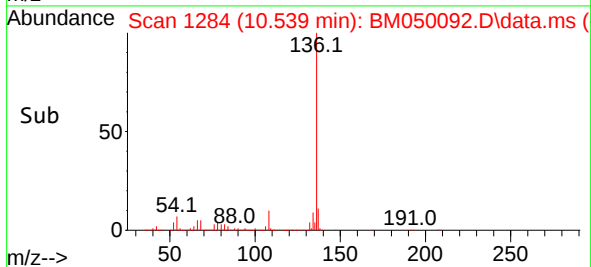

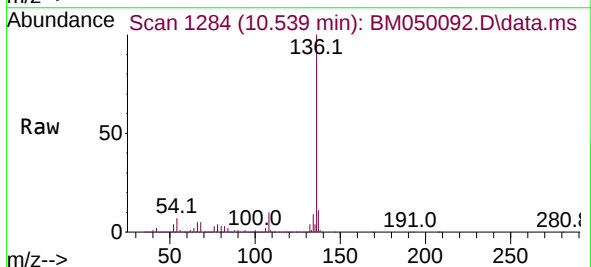


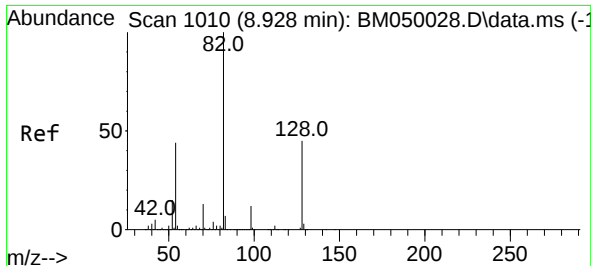

#23
Nitrobenzene-d5
Concen: 24.206 ng
RT: 8.904 min Scan# 1006
Delta R.T. -0.024 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15




Instrument :
BNA_M
ClientSampleId :
MH-MM


Tgt Ion: 82 Resp: 787067
Ion Ratio Lower Upper
82 100
128 45.1 35.7 53.5
54 44.5 35.4 53.2

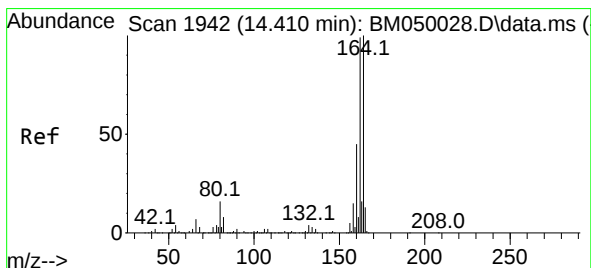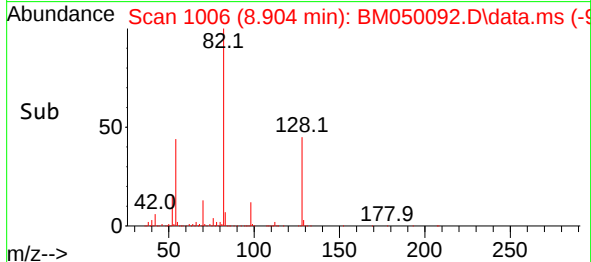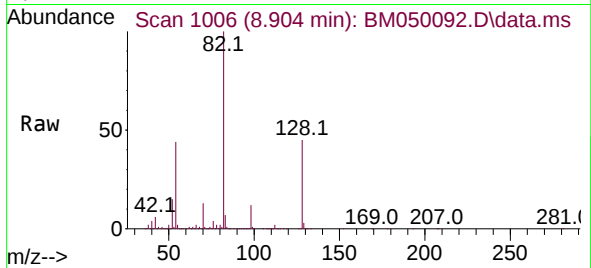

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.392 min Scan# 1939
Delta R.T. -0.018 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Tgt Ion:164 Resp: 1141987
Ion Ratio Lower Upper
164 100
162 98.1 79.4 119.0
160 44.3 36.2 54.4


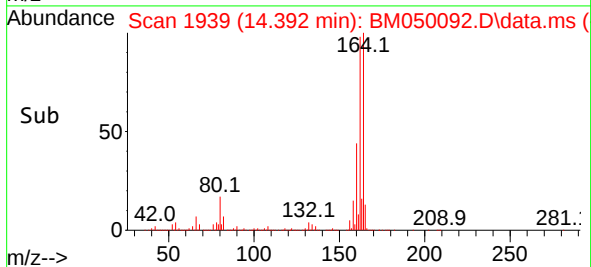

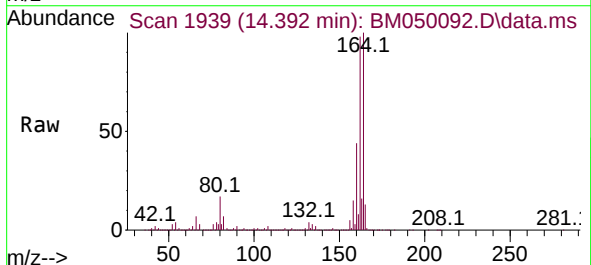


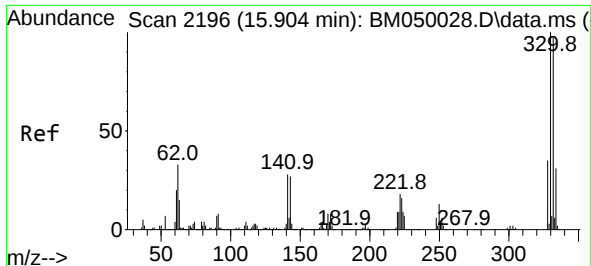

#42
2,4,6-Tribromophenol
Concen: 57.061 ng
RT: 15.892 min Scan# 2194
Delta R.T. -0.012 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15




Instrument :
BNA_M
ClientSampleId :
MH-MM


Tgt Ion:330 Resp: 963515
Ion Ratio Lower Upper
330 100
332 96.9 77.3 115.9
141 26.2 22.5 33.7

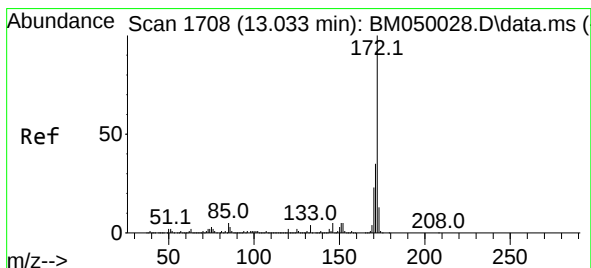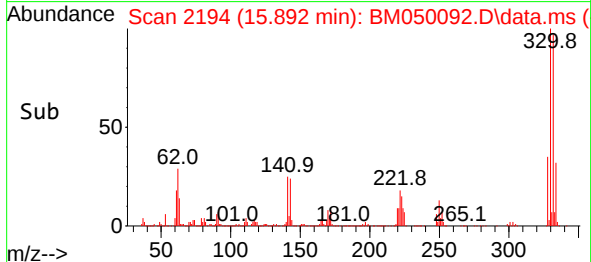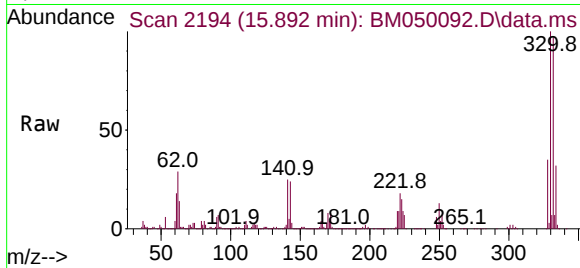

#45
2-Fluorobiphenyl
Concen: 26.269 ng
RT: 13.010 min Scan# 1704
Delta R.T. -0.024 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Tgt Ion:172 Resp: 2535834
Ion Ratio Lower Upper
172 100
171 34.2 27.8 41.6
170 23.2 18.6 28.0


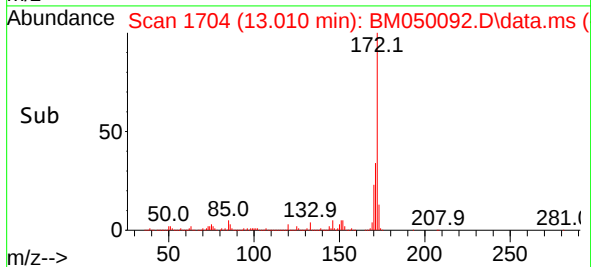

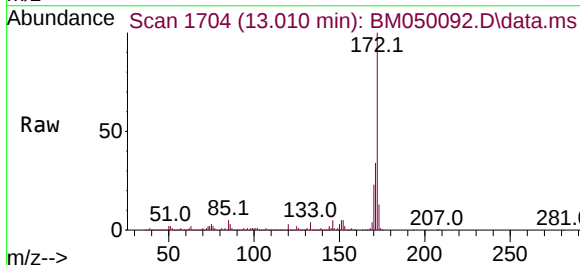


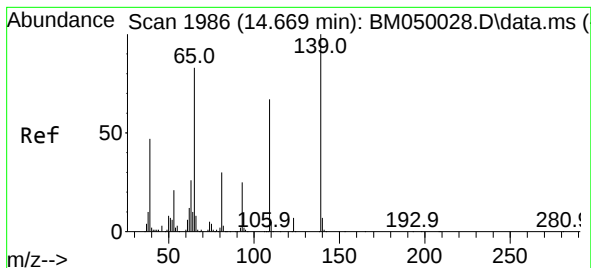

#56
4-Nitrophenol
Concen: 4.555 ng
RT: 14.692 min Scan# 1986
Delta R.T. 0.023 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15




Instrument :
BNA_M
ClientSampleId :
MH-MM


Tgt Ion:139 Resp: 296
Ion Ratio Lower Upper
139 100
109 98.5 47.0 87.0#
65 99.6 64.3 104.3

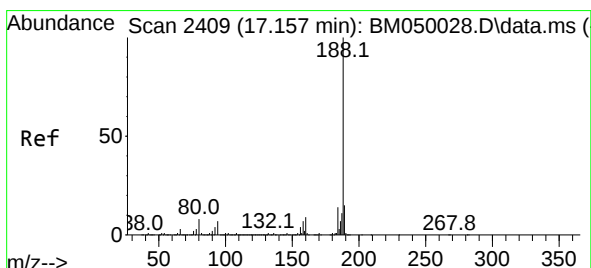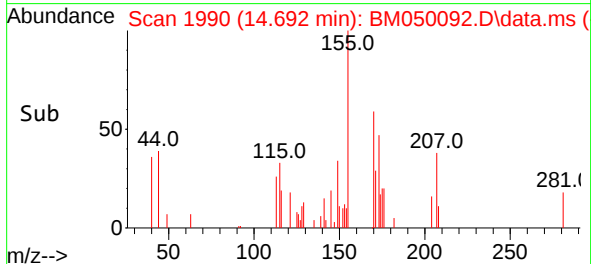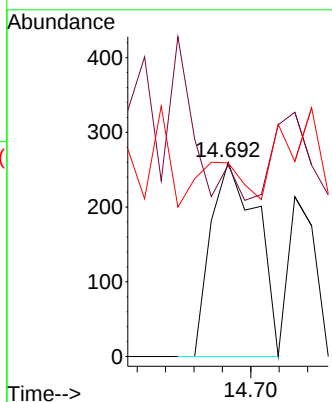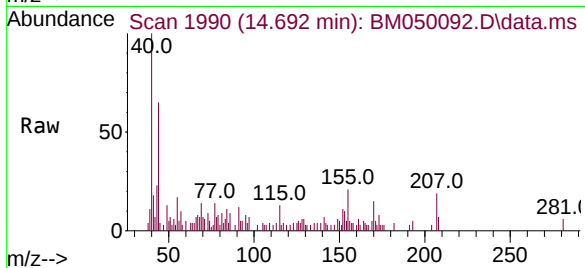

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.145 min Scan# 2407
Delta R.T. -0.012 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Tgt Ion:188 Resp: 2403893
Ion Ratio Lower Upper
188 100
94 6.9 5.7 8.5
80 7.3 6.2 9.4


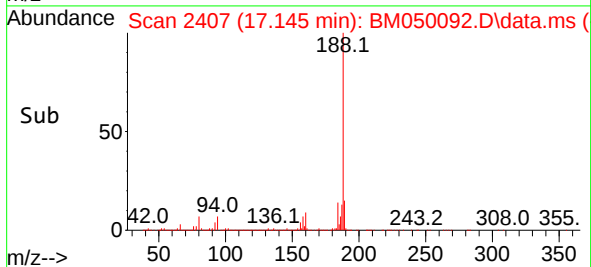
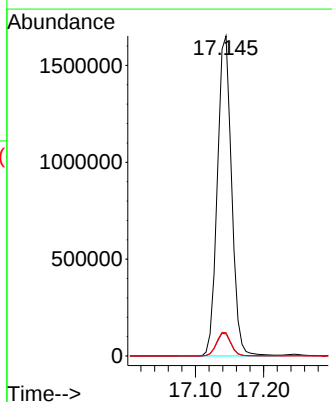
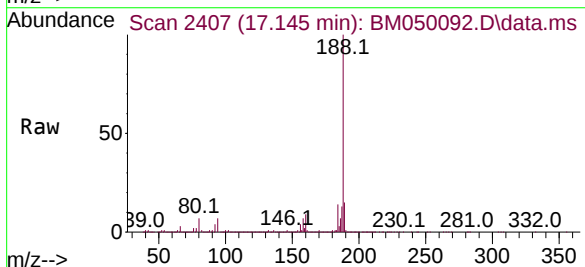


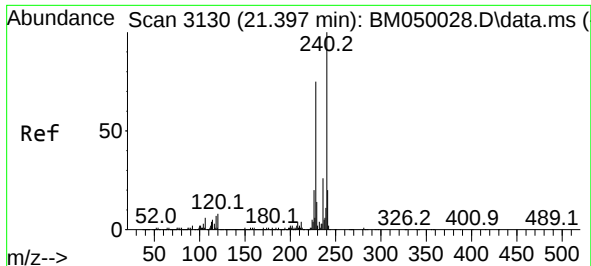

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.386 min Scan# 3130
Delta R.T. -0.011 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15




Instrument :
BNA_M
ClientSampleId :
MH-MM


Tgt Ion:240 Resp: 1726548
Ion Ratio Lower Upper
240 100
120 7.8 6.5 9.7
236 25.9 20.9 31.3

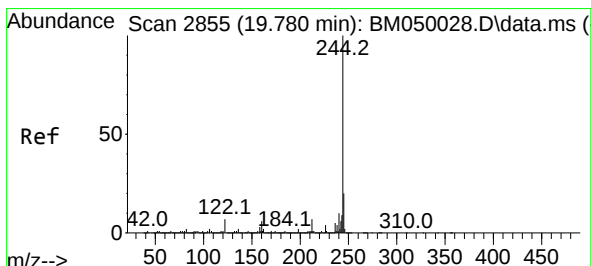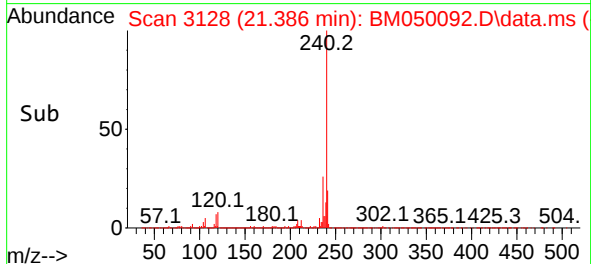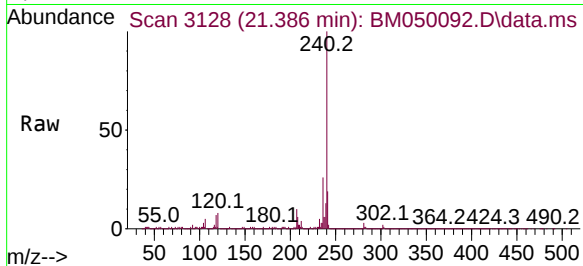

#79
Terphenyl-d14
Concen: 38.897 ng
RT: 19.768 min Scan# 2853
Delta R.T. -0.012 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Tgt Ion:244 Resp: 4538501
Ion Ratio Lower Upper
244 100
212 6.8 5.6 8.4
122 7.0 5.6 8.4

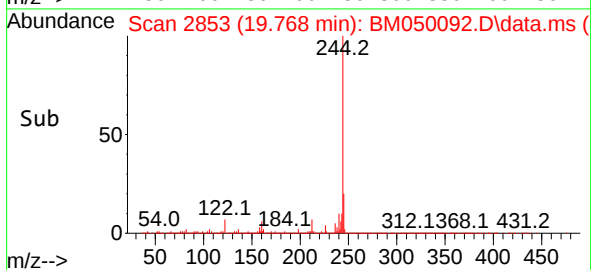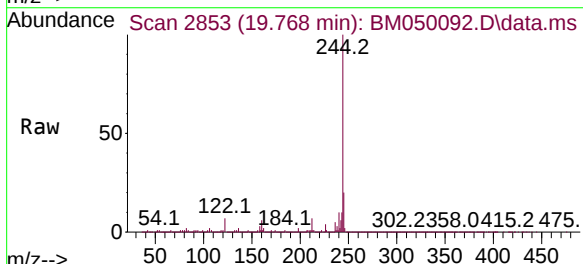

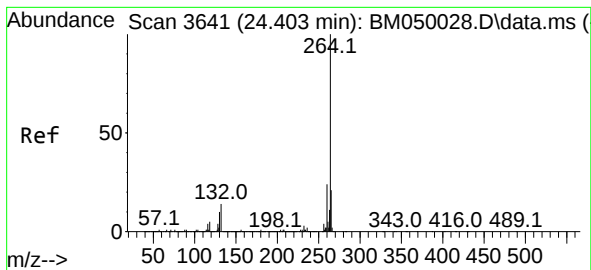

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.380 min Scan# 30
Delta R.T. -0.024 min
Lab File: BM050092.D
Acq: 02 May 2025 19:15

Instrument :
BNA_M
ClientSampleId :
MH-MM

Tgt Ion:264 Resp: 1526163

Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.8	28.2
265	21.5	17.0	25.4

