

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
 Data File : BM050094.D
 Acq On : 02 May 2025 20:34
 Operator : RC/JU
 Sample : Q1933-01 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 OK-01-050125

Quant Time: May 02 23:59:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.751	152	409837	20.000	ng	-0.02
21) Naphthalene-d8	10.539	136	1575589	20.000	ng	-0.02
39) Acenaphthene-d10	14.398	164	1152250	20.000	ng	-0.01
64) Phenanthrene-d10	17.145	188	2420942	20.000	ng	-0.01
76) Chrysene-d12	21.386	240	1706448	20.000	ng	-0.01
86) Perylene-d12	24.380	264	1569666	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.340	112	875477	37.406	ng	-0.02
7) Phenol-d6	6.939	99	1141186	38.794	ng	-0.01
23) Nitrobenzene-d5	8.910	82	669274	20.931	ng	-0.02
42) 2,4,6-Tribromophenol	15.892	330	673844	39.551	ng	-0.01
45) 2-Fluorobiphenyl	13.016	172	1953292	20.054	ng	-0.02
79) Terphenyl-d14	19.768	244	2958133	25.651	ng	-0.01
Target Compounds						
						Qvalue
75) Fluoranthene	19.203	202	383901	2.395	ng	97
78) Pyrene	19.568	202	415560	3.468	ng	99
88) Benzo(b)fluoranthene	23.433	252	223968	2.194	ng	# 84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050094.D
Acq On : 02 May 2025 20:34
Operator : RC/JU
Sample : Q1933-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OK-01-050125

Quant Time: May 02 23:59:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

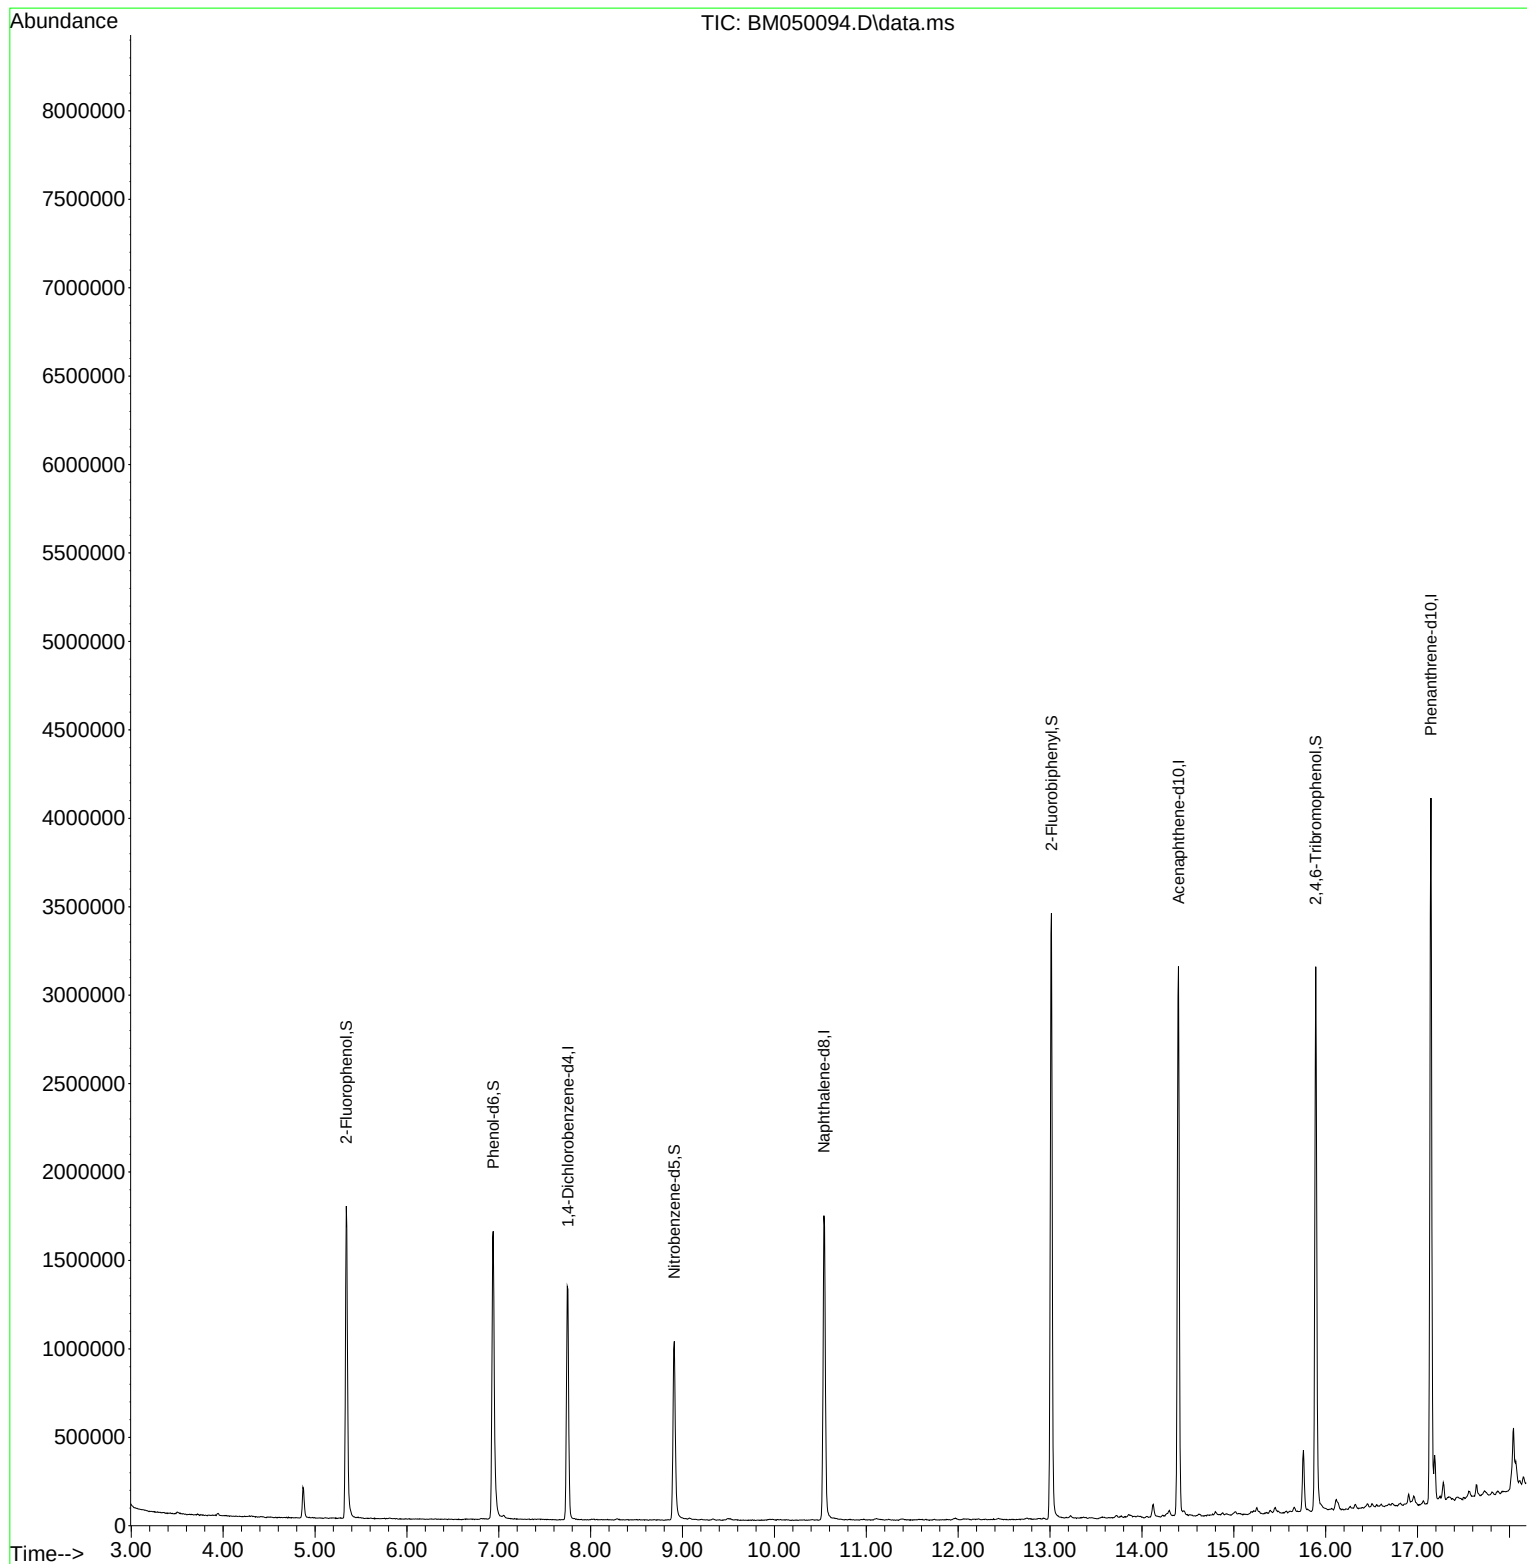

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050094.D
Acq On : 02 May 2025 20:34
Operator : RC/JU
Sample : Q1933-01 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
OK-01-050125

Quant Time: May 02 23:59:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

