
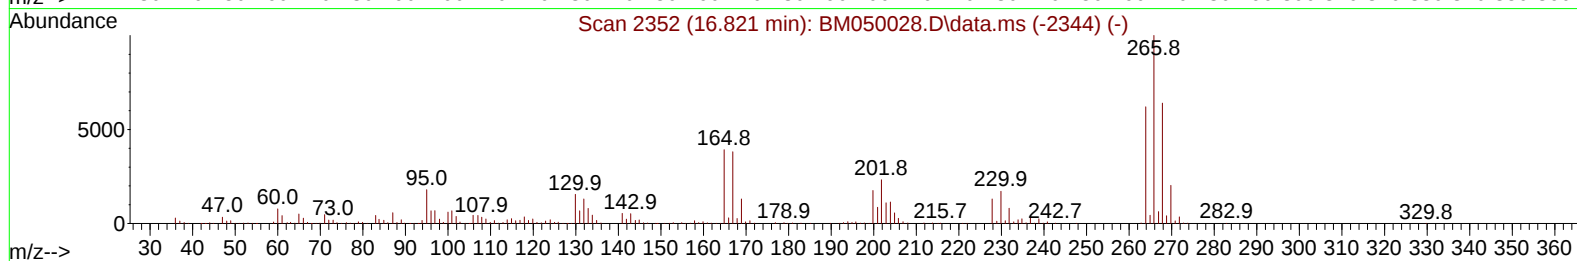
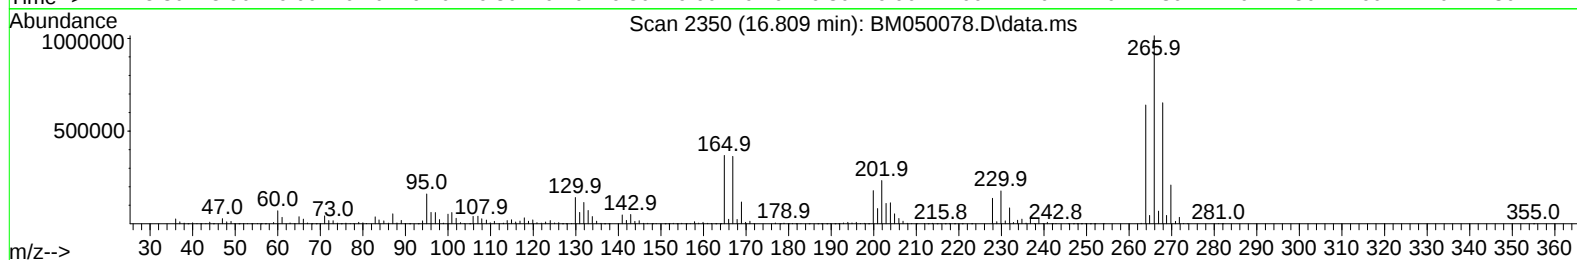


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050078.D
Acq On : 02 May 2025 09:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 11:44:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

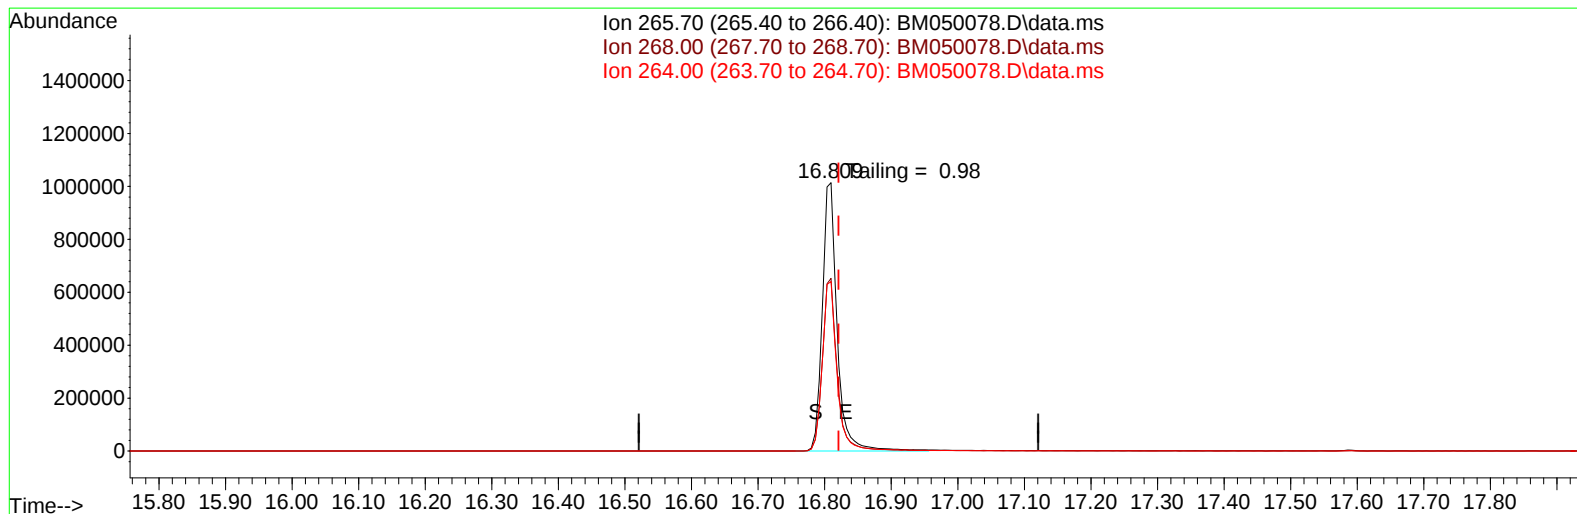

TIC: BM050078.D\data.ms

(70) Pentachlorophenol (C)




16.809min (-0.012) 427399.30 ng

response 1566093

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.32
264.00	62.00	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050225\
Data File : BM050078.D
Acq On : 02 May 2025 09:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 02 11:44:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

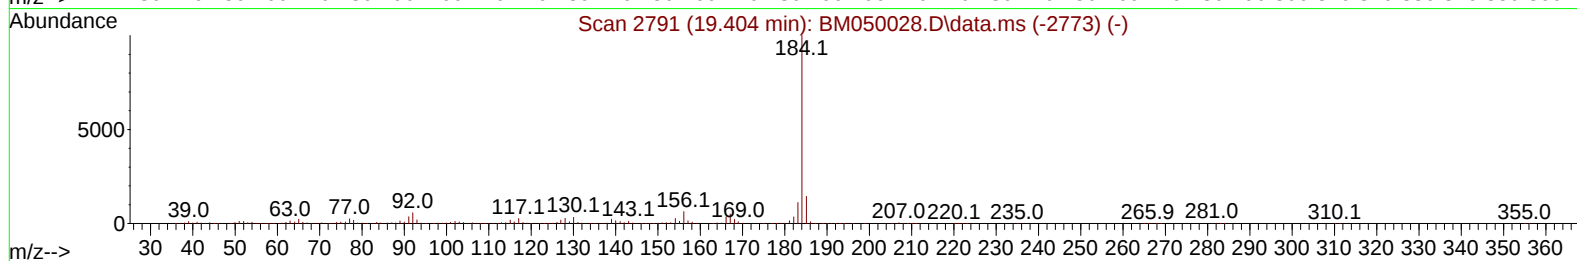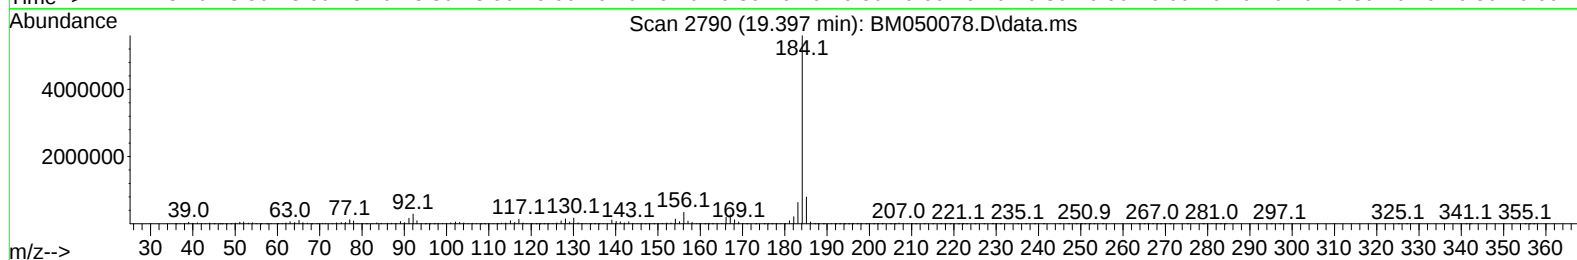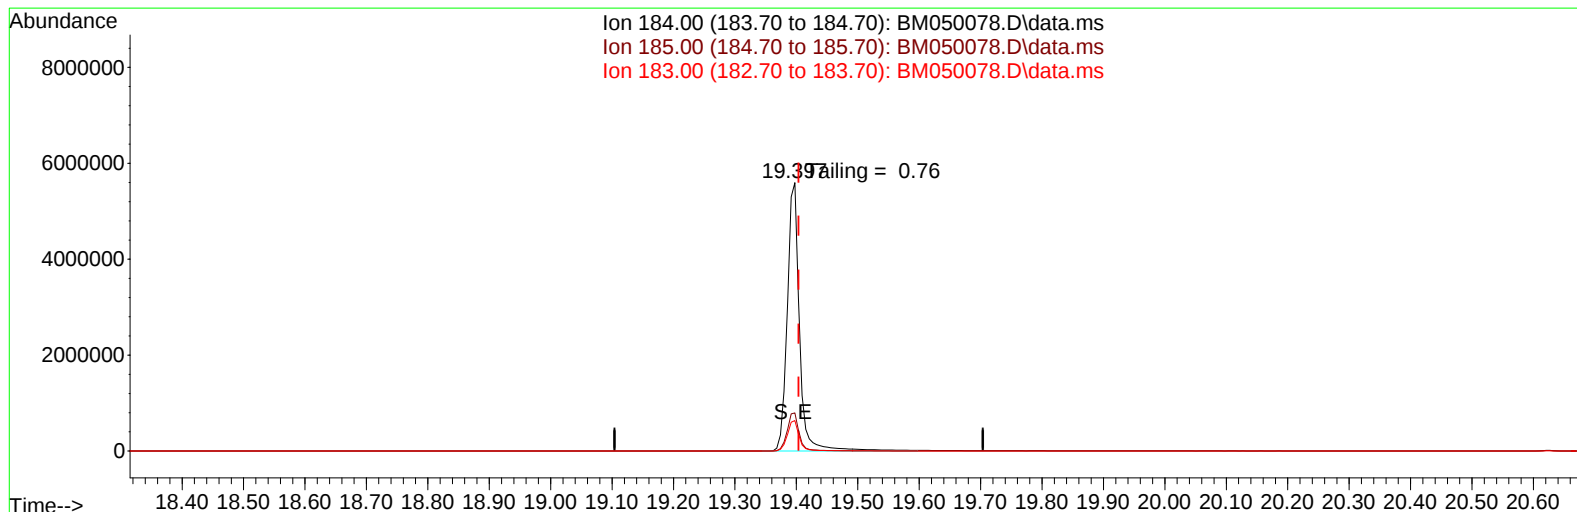

TIC: BM050078.D\data.ms

(77) Benzidine

19.397min (-0.007) 114069.32 ng

response 7848374

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.21
183.00	11.10	11.35
0.00	0.00	0.00