

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050317\
 Data File : BM009873.D
 Acq On : 03 May 2017 14:18
 Operator : SJ/MA
 Sample : I2871-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAB22

Quant Time: May 04 02:03:43 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 04 02:03:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	112003	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	485878	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	308849	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	749862	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	929931	20.00	ng/ul	0.00
83) Perylene-d12	23.70	264	707020	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	7331	3.01	ng/uL	0.00
5) Phenol-d5	6.99	99	167361	13.75	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	140455	16.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	119577	15.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	143042	15.08	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	66426	16.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	70777	17.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	123138	14.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	158341	15.79	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	472805	17.60	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	519684	16.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	60175	11.61	ng/ul	0.00
57) Fluorene-d10	15.45	176	421306	17.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	61281	11.58	ng/ul	0.00
70) Anthracene-d10	17.31	188	675146	17.54	ng/ul	0.00
76) Pyrene-d10	19.60	212	630169	15.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	363318	10.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.91	163	157113	5.91	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050317\
Data File : BM009873.D
Acq On : 03 May 2017 14:18
Operator : SJ/MA
Sample : I2871-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAB22

Quant Time: May 04 02:03:43 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 04 02:03:11 2017
Response via : Initial Calibration

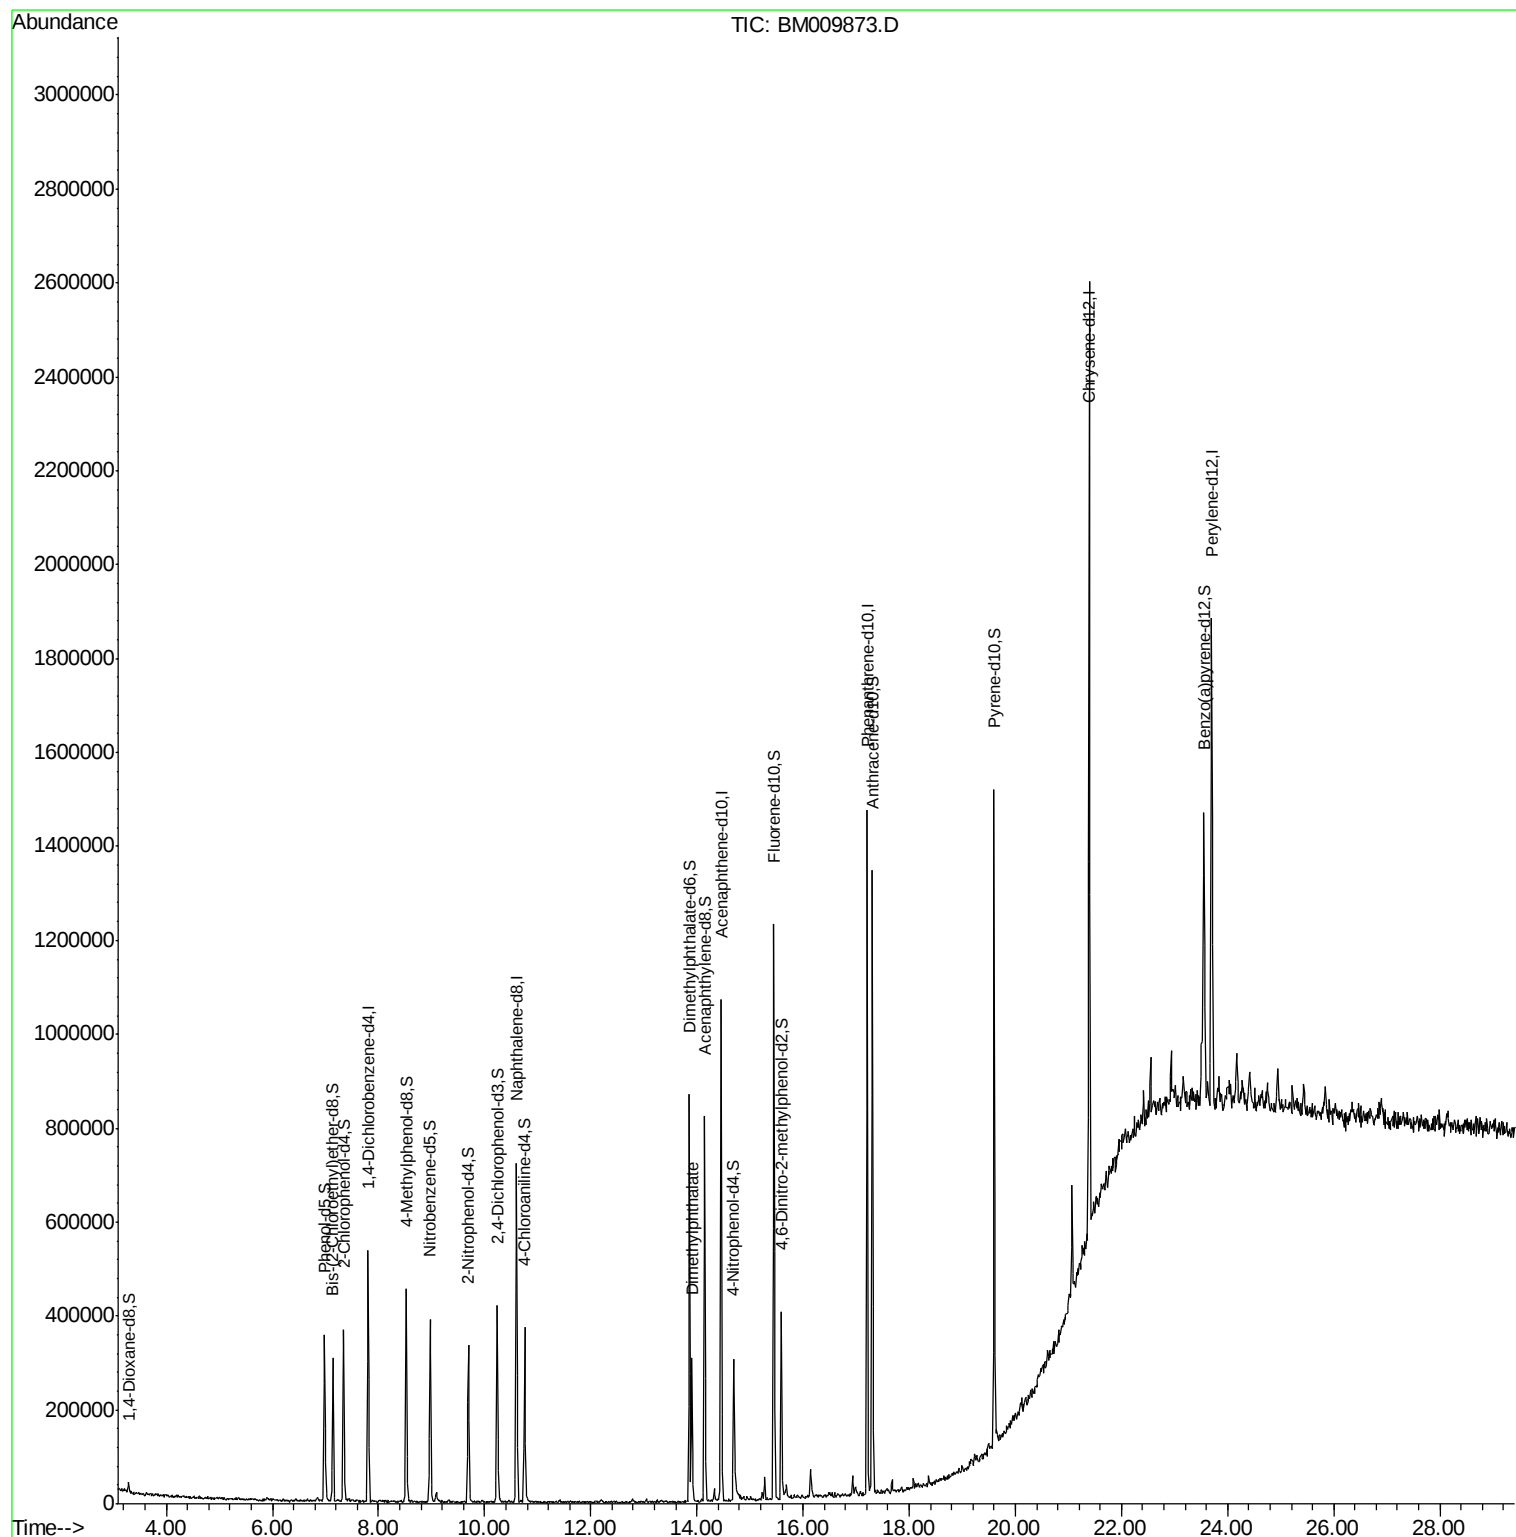

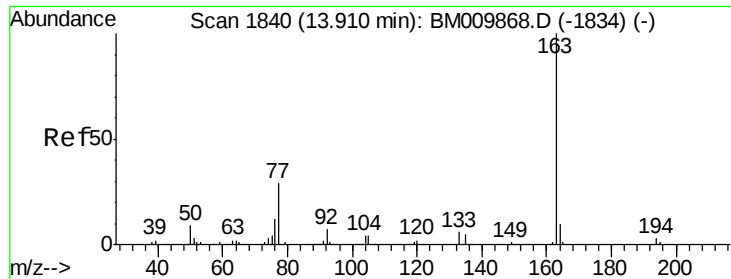

#44

Dimethylphthalate

Concen: 5.91 ng/ul

RT: 13.91 min Scan# 1840

Delta R.T. -0.00 min

Lab File: BM009873.D

Acq: 03 May 2017 14:18

Instrument :

BNA_M

ClientSampleId :

YAB22


Tgt Ion:163 Resp: 157113

Ion Ratio Lower Upper

163 100

194 4.9 3.0 4.6#

164 10.0 8.6 12.8

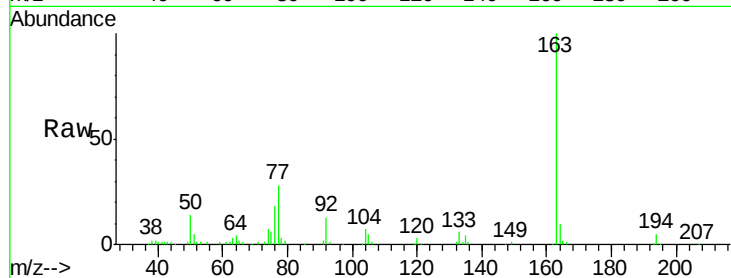

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

