

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050317\
 Data File : BM009875.D
 Acq On : 03 May 2017 15:30
 Operator : SJ/MA
 Sample : I2871-19
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YAB29

Quant Time: May 04 02:03:59 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 04 02:03:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	112240	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	494033	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	306636	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.21	188	772470	20.00	ng/ul	0.00
75) Chrysene-d12	21.39	240	940633	20.00	ng/ul	0.00
83) Perylene-d12	23.70	264	728151	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	8516	3.49	ng/uL	0.00
5) Phenol-d5	6.99	99	208269	17.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	146985	17.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	146860	18.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	167943	17.67	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	70408	17.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	83683	19.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	151069	17.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	183039	17.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	512958	19.23	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	633361	19.69	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	77464	15.05	ng/ul	0.00
57) Fluorene-d10	15.45	176	466306	19.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	60391	11.08	ng/ul	0.00
70) Anthracene-d10	17.31	188	804287	20.28	ng/ul	0.00
76) Pyrene-d10	19.60	212	955877	23.03	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	705114	19.91	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.91	163	105568	4.00 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050317\
Data File : BM009875.D
Acq On : 03 May 2017 15:30
Operator : SJ/MA
Sample : I2871-19
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YAB29

Quant Time: May 04 02:03:59 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 04 02:03:11 2017
Response via : Initial Calibration

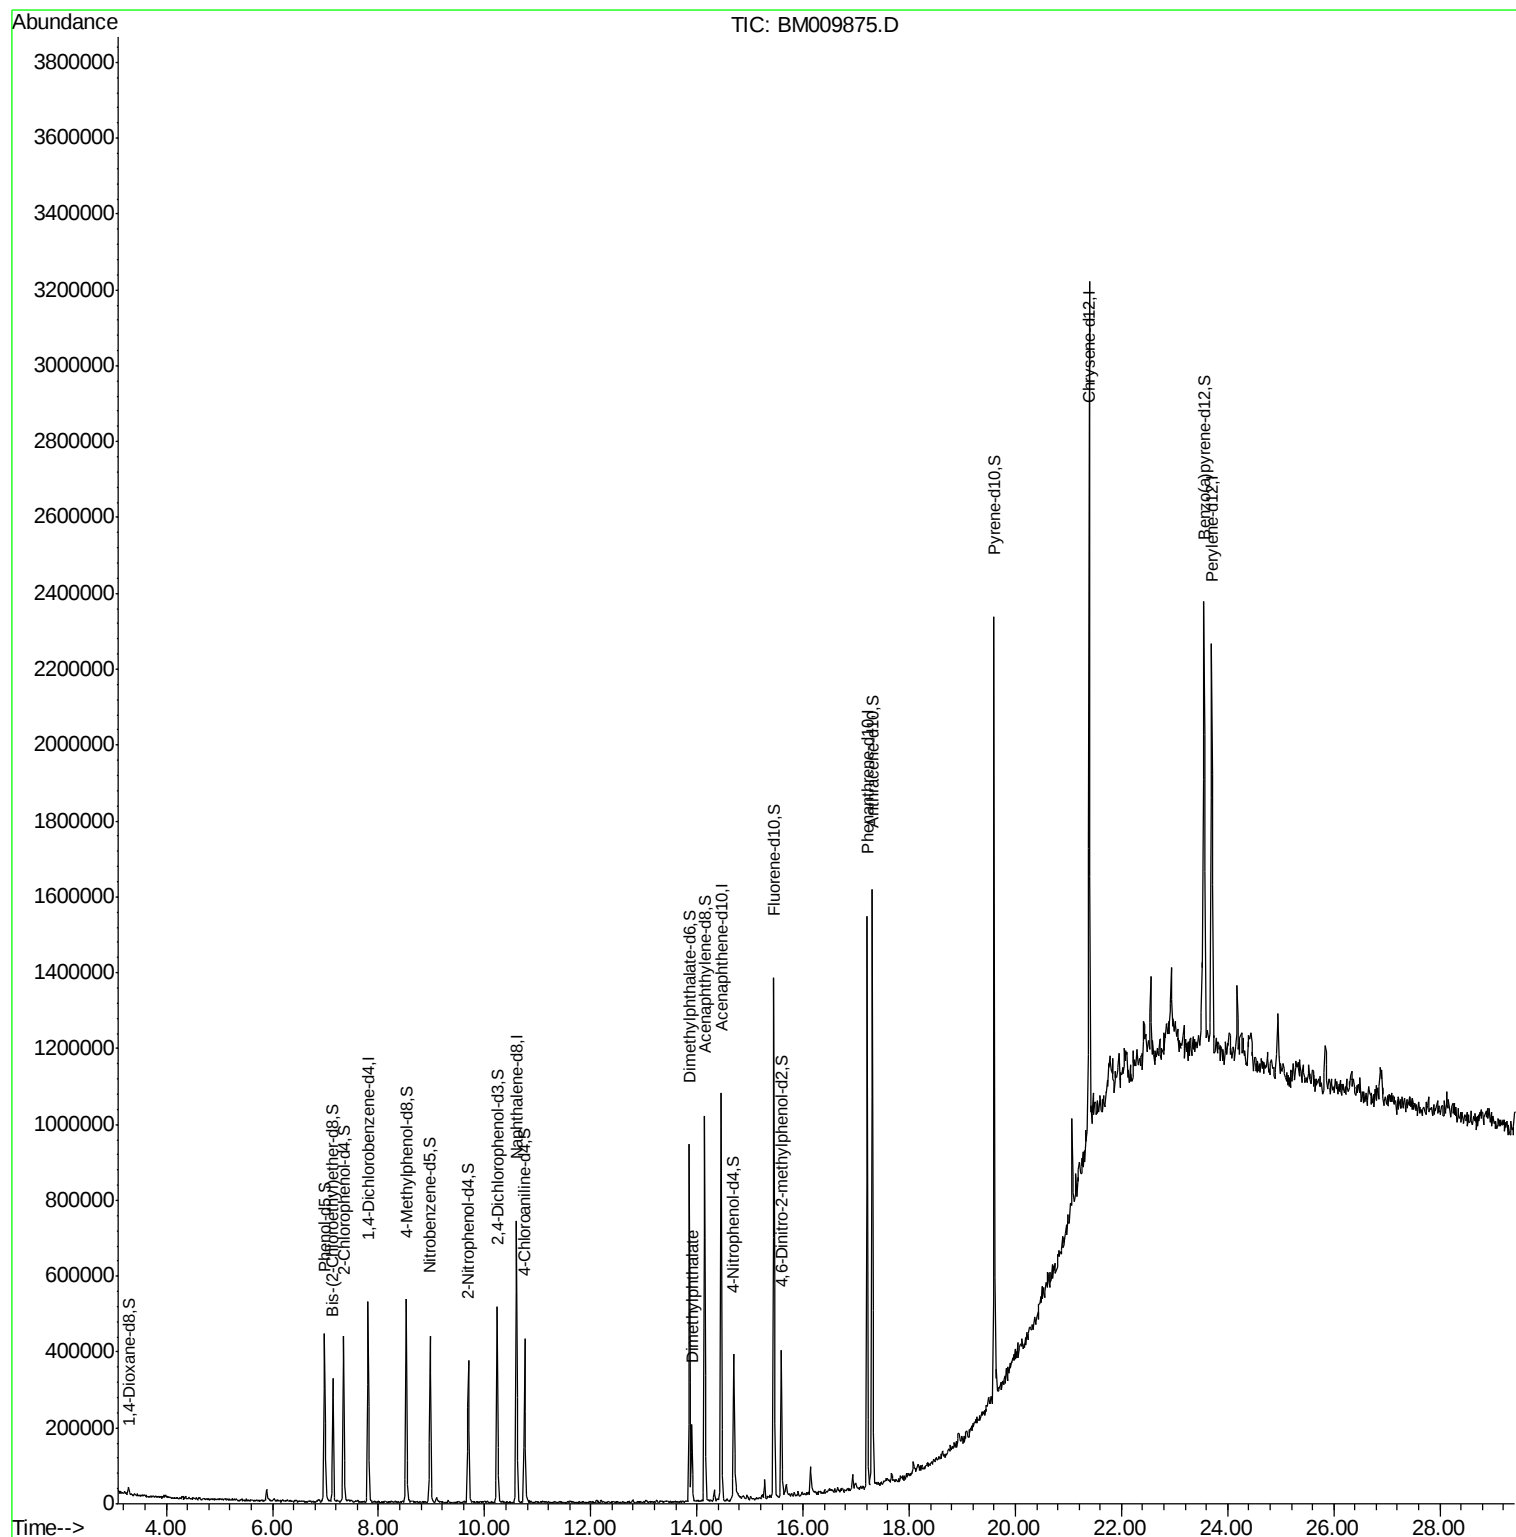

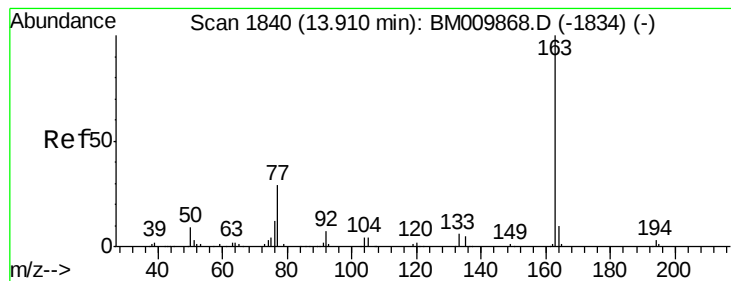

#44

Dimethylphthalate

Concen: 4.00 ng/ul

RT: 13.91 min Scan# 1840

Delta R.T. -0.00 min

Lab File: BM009875.D

Acq: 03 May 2017 15:30

Instrument :

BNA_M

ClientSampleId :

YAB29


Tgt Ion:163 Resp: 105568

Ion Ratio Lower Upper

163 100

194 5.5 3.0 4.6#

164 10.2 8.6 12.8

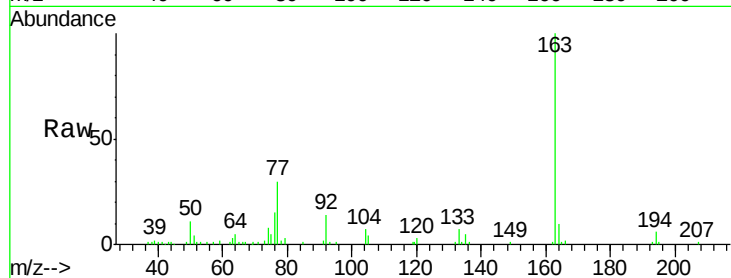

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

