

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050318\
 Data File : BM014945.D
 Acq On : 03 May 2018 16:20
 Operator : SJ/JU
 Sample : J2554-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 04 05:08:14 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 04 05:03:56 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.49	152	332688	20.00	ng/ul	0.00
18) Naphthalene-d8	11.33	136	1431963	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	760297	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.81	188	1625912	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1439531	20.00	ng/ul	0.00
83) Perylene-d12	24.37	264	1284491	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.64	96	55806	7.32	ng/uL	0.00
5) Phenol-d5	7.62	99	1090525	42.40	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.79	67	774750	46.98	ng/ul	0.00
9) 2-Chlorophenol-d4	8.01	132	906948	42.15	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	741060	36.13	ng/ul	0.00
19) Nitrobenzene-d5	9.67	128	431824	41.71	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	458174	44.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	798220	38.11	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	1076616	52.07	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	2511415	42.32	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2921124	39.86	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	418706	38.01	ng/ul	0.00
57) Fluorene-d10	16.07	176	2132762	41.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.17	200	312516	35.52	ng/ul	0.00
70) Anthracene-d10	17.91	188	3208500	42.34	ng/ul	0.00
76) Pyrene-d10	20.15	212	3400532	49.93	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.22	264	2944315	46.66	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	7.65	94	64930	2.566	ng/ul# 86
15) N-Nitroso-di-n-propylamine	9.19	70	19247	1.234	ng/ul# 1
44) Dimethylphthalate	14.53	163	489892	8.539	ng/ul 100
69) Phenanthrene	17.85	178	318166	3.644	ng/ul 99
74) Fluoranthene	19.82	202	509448	5.351	ng/ul# 79
77) Pyrene	20.17	202	423165	5.031	ng/ul# 76
80) Benzo(a)anthracene	21.88	228	203280	2.415	ng/ul 97
82) Chrysene	21.93	228	204274	2.592	ng/ul 99
85) Benzo(b)fluoranthene	23.62	252	247394	3.267	ng/ul# 92
86) Benzo(k)fluoranthene	23.62	252	247394	3.398	ng/ul# 91
88) Benzo(a)pyrene	24.27	252	155556	2.166	ng/ul# 95
89) Indeno(1,2,3-cd)pyrene	26.93	276	108733	1.251	ng/ul# 87
91) Benzo(g,h,i)perylene	27.72	276	100412	1.405	ng/ul# 87




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050318\
Data File : BM014945.D
Acq On : 03 May 2018 16:20
Operator : SJ/JU
Sample : J2554-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 04 05:08:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 04 05:03:56 2018
Response via : Initial Calibration

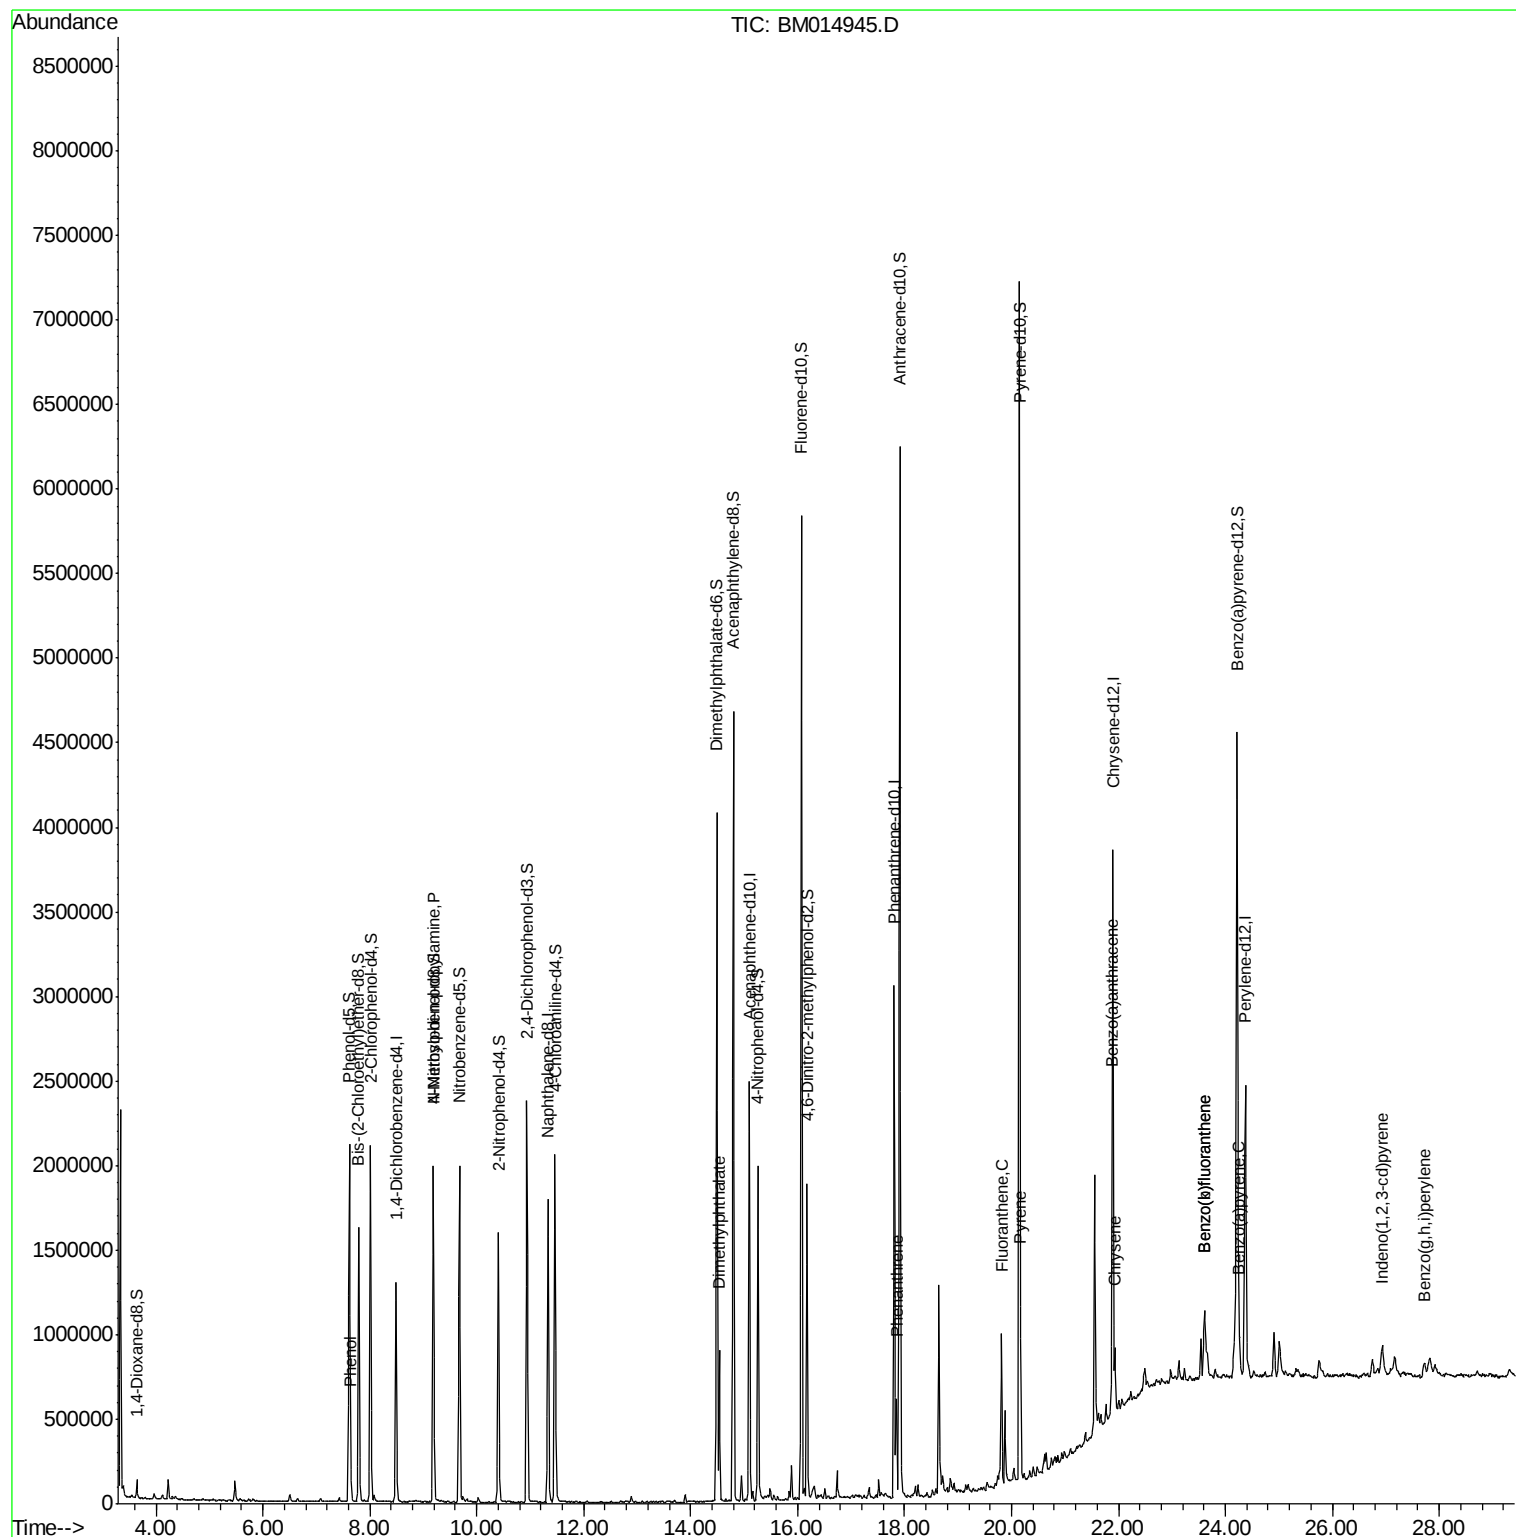

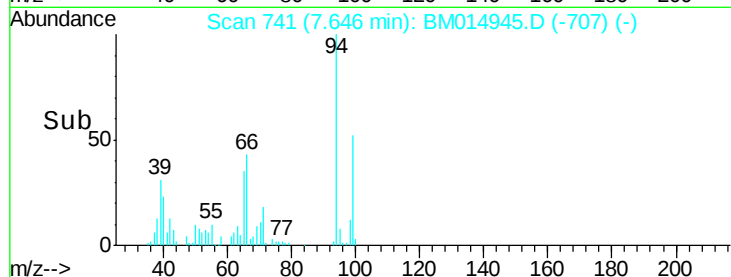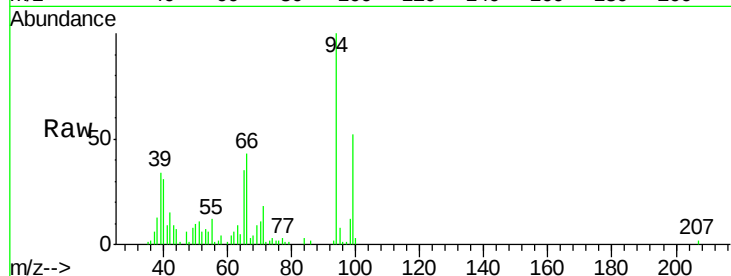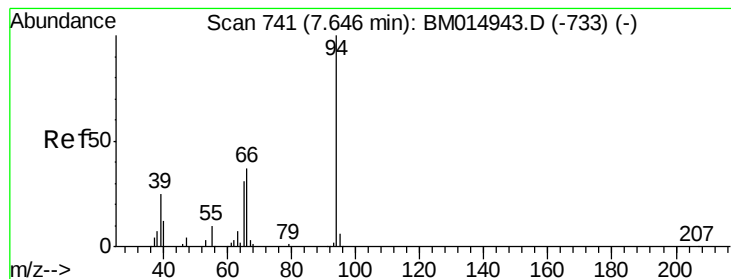

#6

Phenol

Concen: 2.566 ng/ul

RT: 7.65 min Scan# 741

Delta R.T. -0.00 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampleId :





Tot Ion: 94 Resp: 64930

Ion Ratio Lower Upper

94 100

65 34.5 28.2 42.4

66 43.2 47.2 70.8#

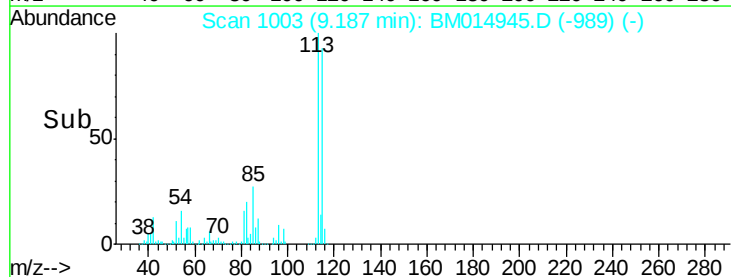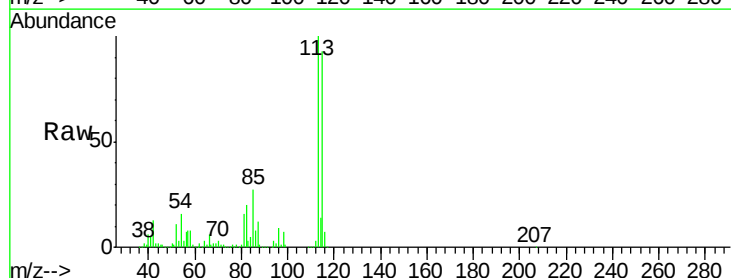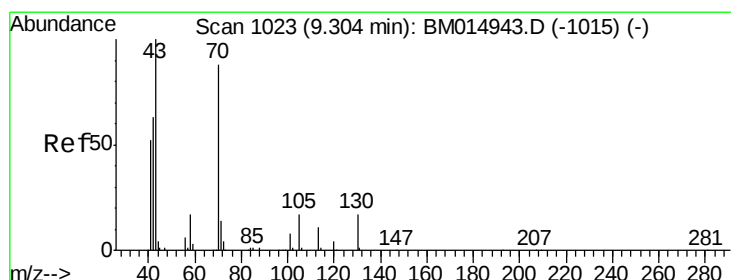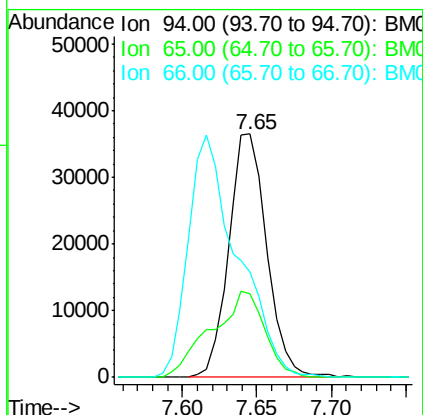

#15

N-Nitroso-di-n-propylamine

Concen: 1.234 ng/ul

RT: 9.19 min Scan# 1003

Delta R.T. -0.12 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Tgt Ion: 70 Resp: 19247


Ion Ratio Lower Upper


70 100

42 511.0 76.0 114.0#

101 0.0 6.7 10.1#

130 0.0 14.6 22.0#

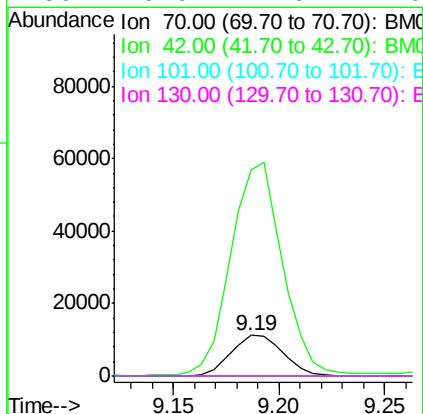

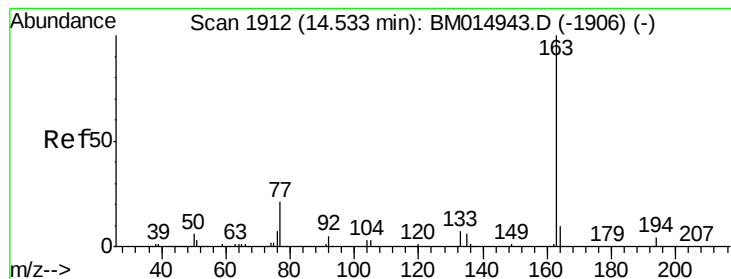

#44

Dimethylphthalate

Concen: 8.539 ng/ul

RT: 14.53 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 489892

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3




164 10.2 8.2 12.4

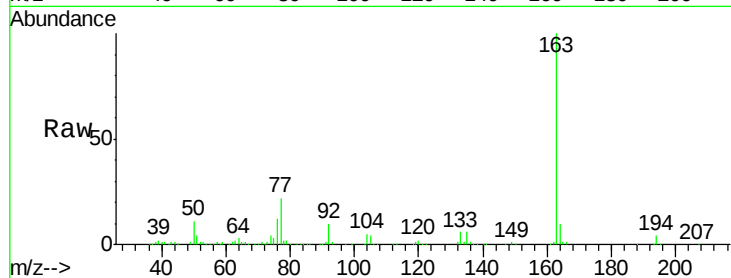

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

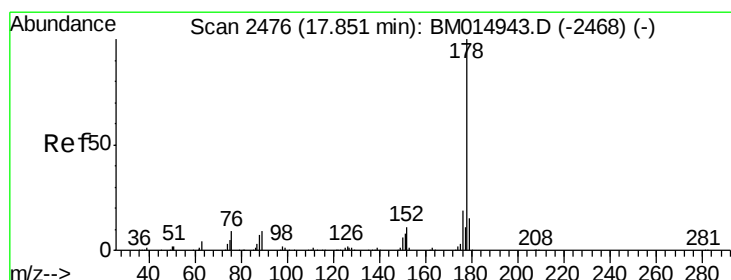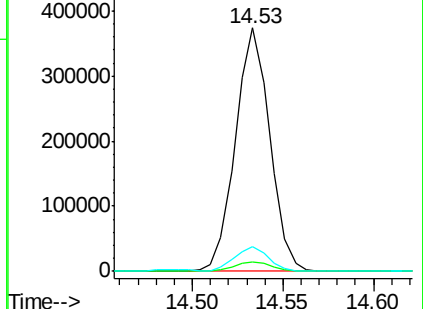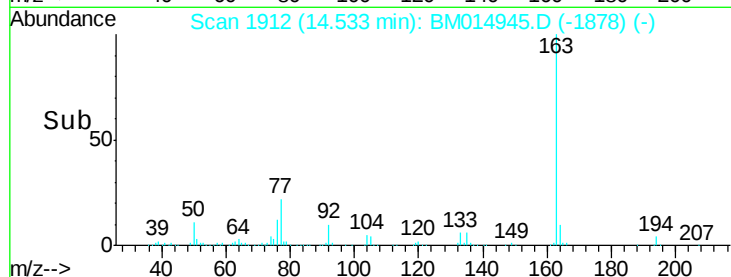

#69

Phenanthrene

Concen: 3.644 ng/ul

RT: 17.85 min Scan# 2476

Delta R.T. -0.00 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20


Tgt Ion:178 Resp: 318166

Ion Ratio Lower Upper

178 100

179 15.6 12.6 19.0



176 18.9 14.9 22.3

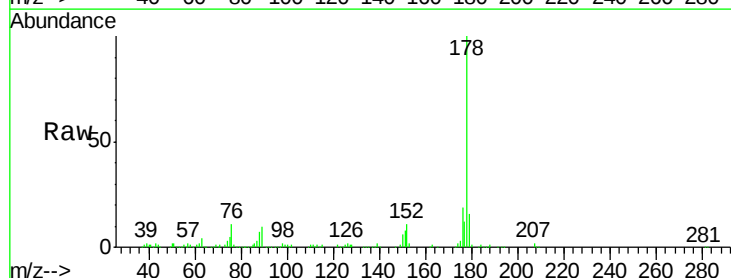


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

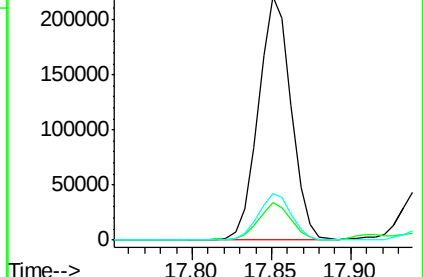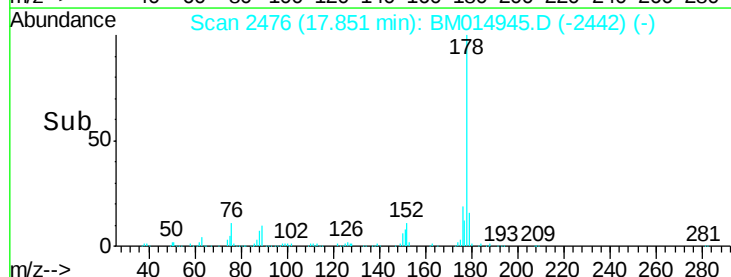

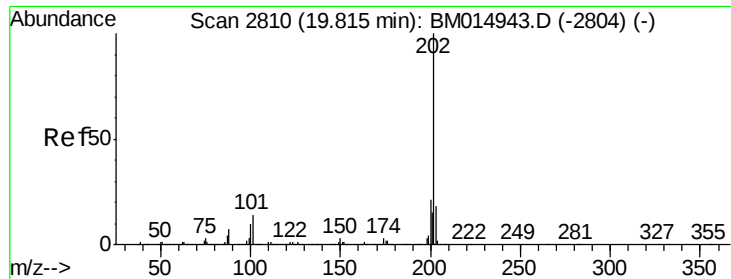

#74

Fluoranthene

Concen: 5.351 ng/ul

RT: 19.82 min Scan# 2810

Delta R.T. -0.00 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampled :


Tot Ion:202 Resp: 509448

Ion Ratio Lower Upper

202 100

101 13.3 4.6 7.0#




100 10.3 3.4 5.2#

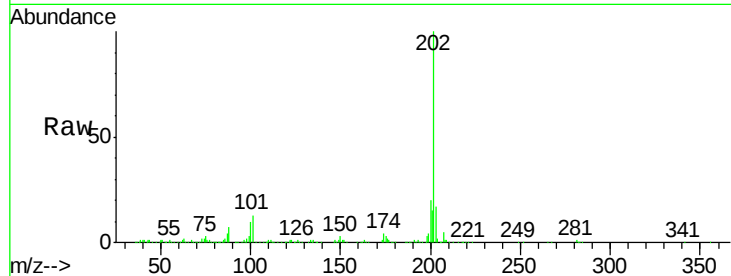

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

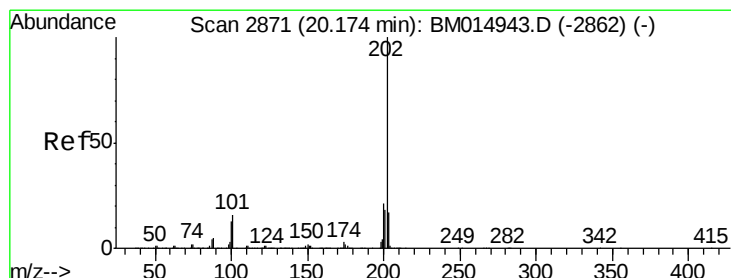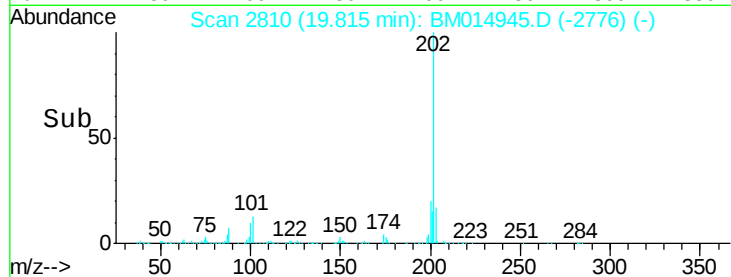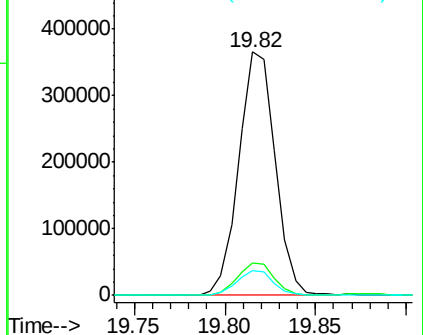

#77

Pyrene

Concen: 5.031 ng/ul

RT: 20.17 min Scan# 2871

Delta R.T. -0.00 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20


Tgt Ion:202 Resp: 423165

Ion Ratio Lower Upper

202 100

101 15.7 5.1 7.7#



100 12.7 4.9 7.3#

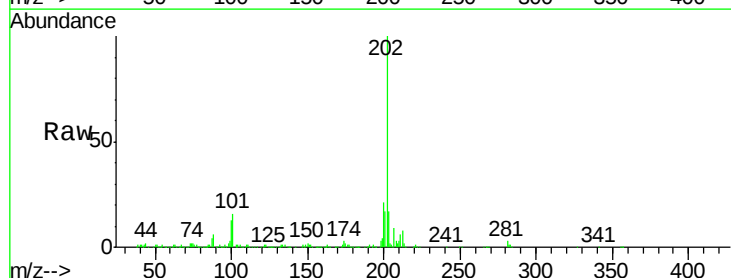


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

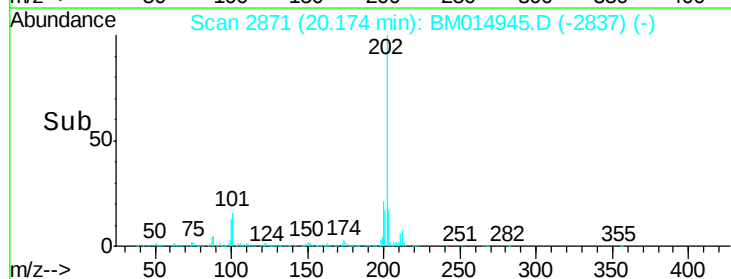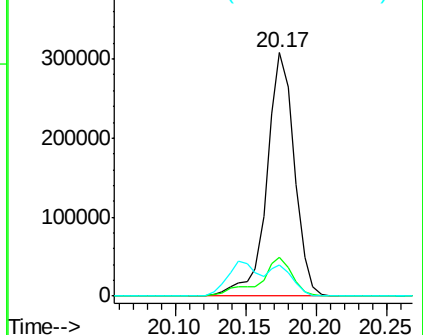

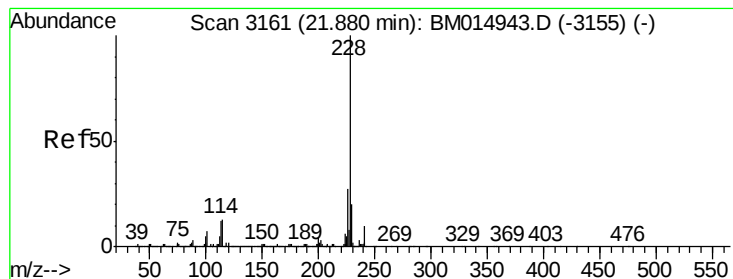

#80

Benzo(a)anthracene

Concen: 2.415 ng/ul

RT: 21.88 min Scan# 3161

Delta R.T. -0.00 min

Lab File: BM014945.D





Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampleId :

Tot Ion:228	Resp:	203280
Ion	Ratio	Lower Upper
228	100	
229	21.2	15.4 23.0
226	27.4	21.4 32.0

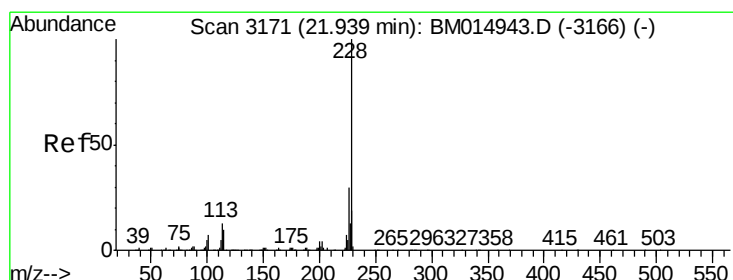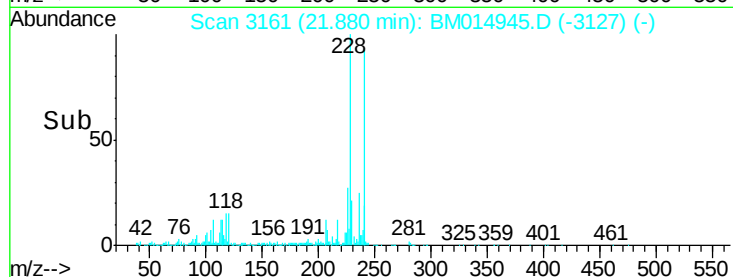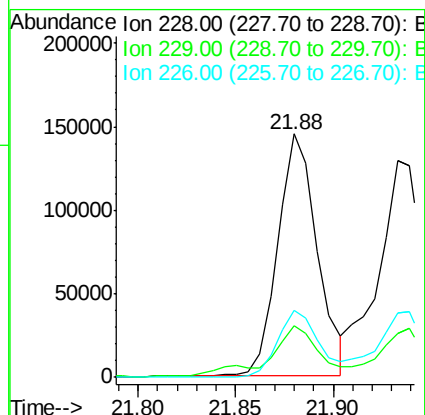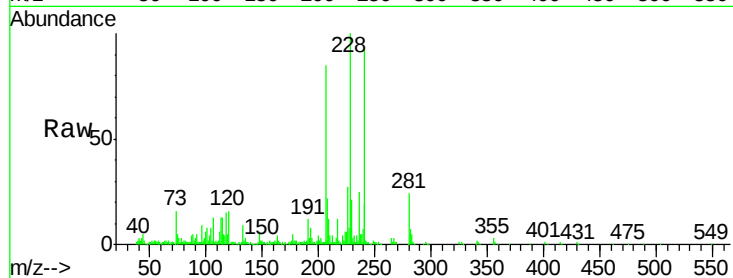

#82

Chrysene

Concen: 2.592 ng/ul




RT: 21.93 min Scan# 3170


Delta R.T. -0.01 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Tgt Ion:228	Resp:	204274
Ion	Ratio	Lower Upper
228	100	
226	29.5	23.4 35.2
229	20.2	15.5 23.3

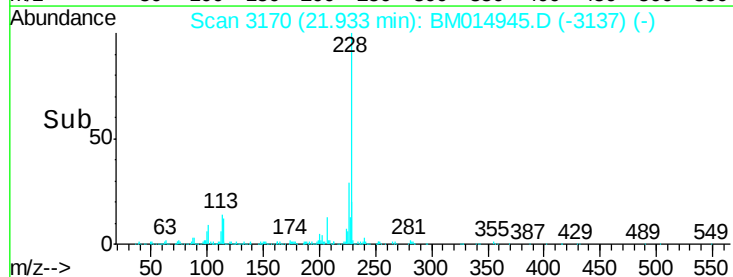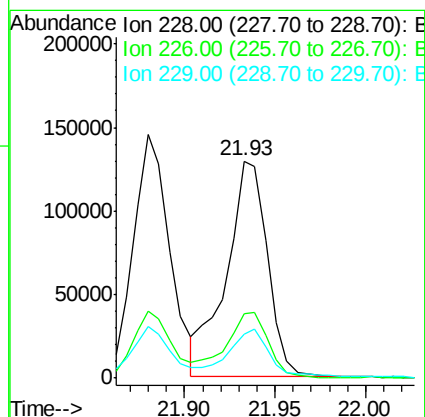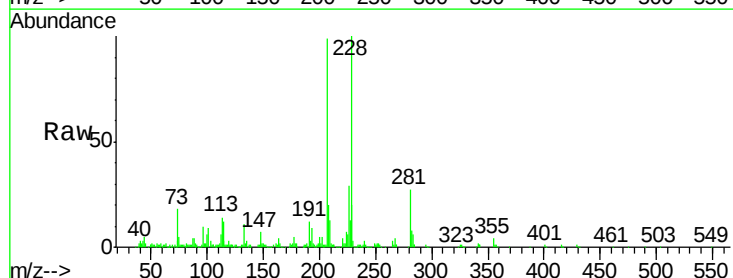

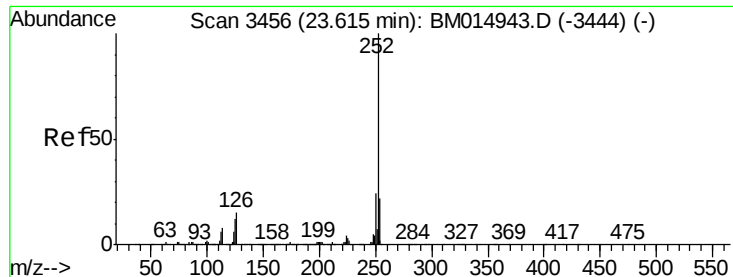

#85

Benzo(b)fluoranthene

Concen: 3.267 ng/ul

RT: 23.62 min Scan# 3457

Delta R.T. 0.01 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 247394

Ion Ratio Lower Upper

252 100

253 23.7 17.9 26.9




125 15.0 3.6 5.4#

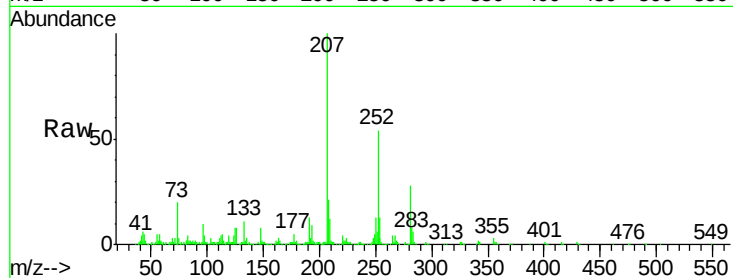

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

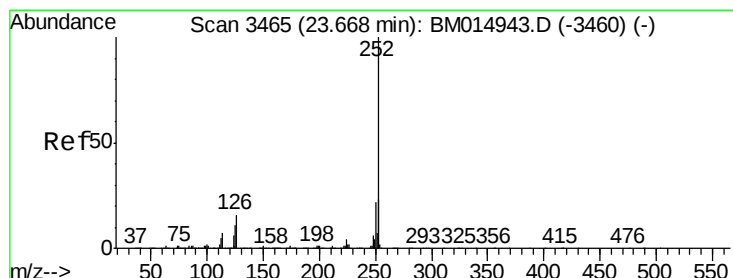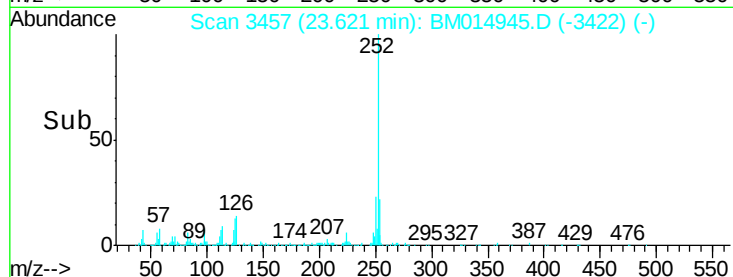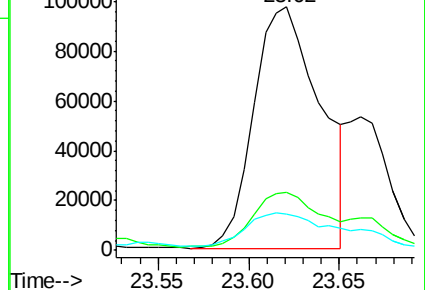

#86

Benzo(k)fluoranthene

Concen: 3.398 ng/ul

RT: 23.62 min Scan# 3457

Delta R.T. -0.05 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20


Tgt Ion:252 Resp: 247394

Ion Ratio Lower Upper

252 100

253 23.7 17.1 25.7



125 15.0 3.4 5.2#

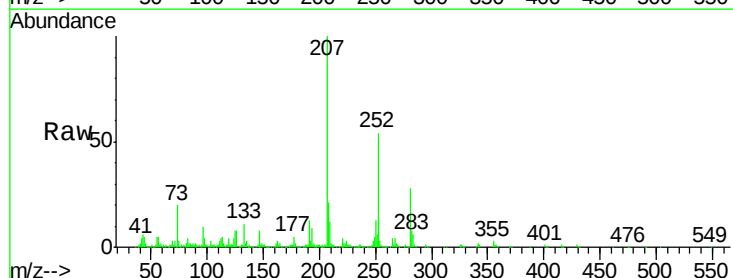


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

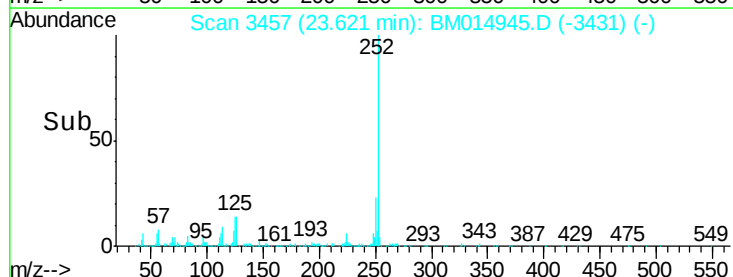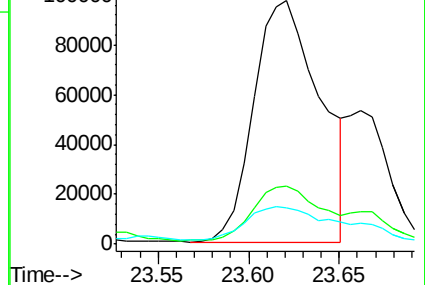

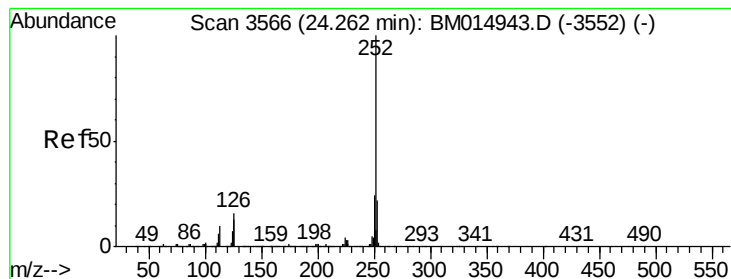

#88

Benzo(a)pyrene

Concen: 2.166 ng/ul

RT: 24.27 min Scan# 3567

Delta R.T. 0.01 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampled :


Tot Ion:252 Resp: 155556

Ion Ratio Lower Upper

252 100

253 22.9 18.2 27.2




125 13.3 4.0 6.0#

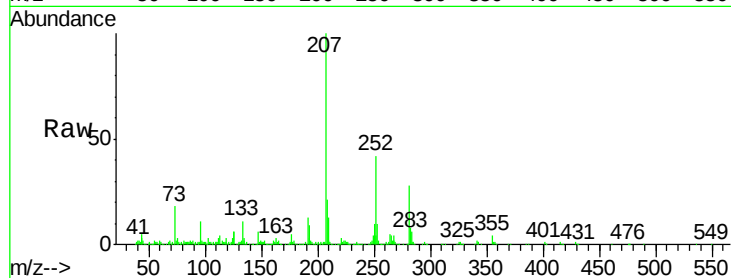

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

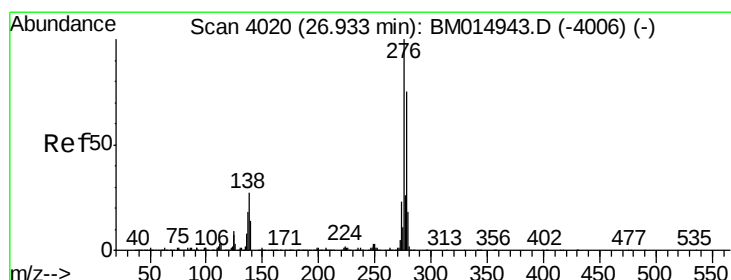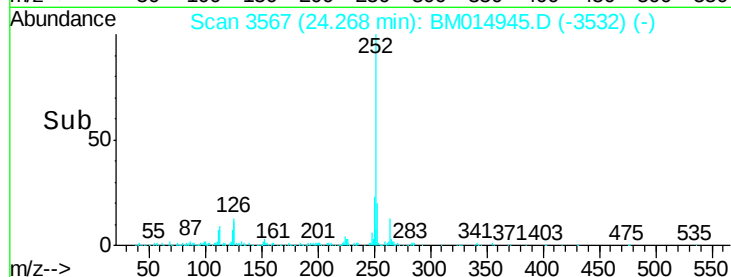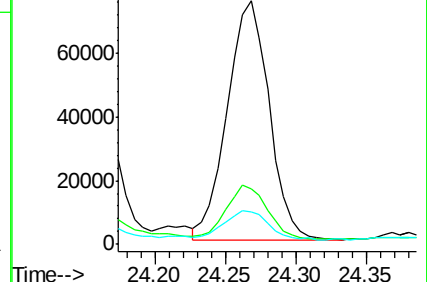

#89

Indeno(1,2,3-cd)pyrene

Concen: 1.251 ng/ul

RT: 26.93 min Scan# 4020

Delta R.T. -0.00 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20


Tgt Ion:276 Resp: 108733

Ion Ratio Lower Upper

276 100

138 24.2 9.3 13.9#



277 26.5 19.9 29.9

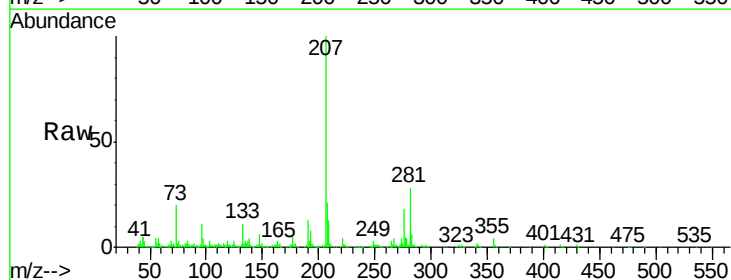


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

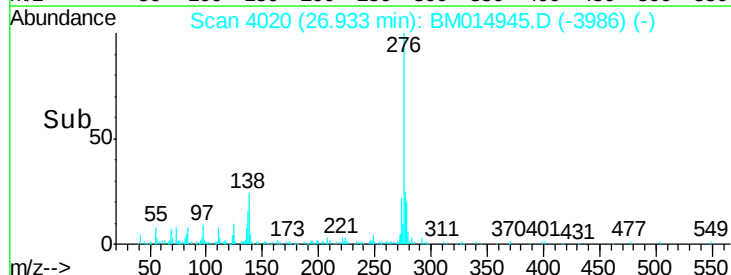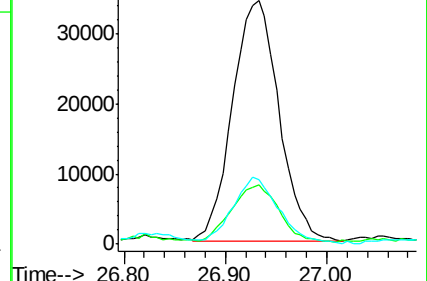

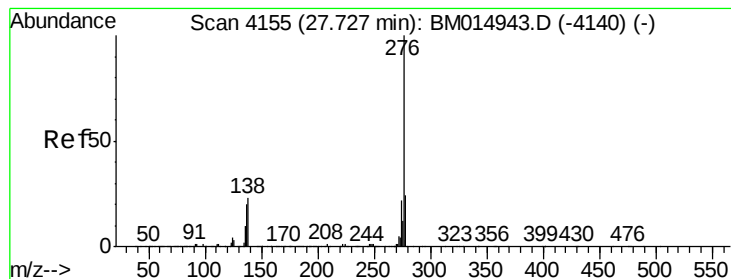

#91

Benzo(a,h,i)perylene

Concen: 1.405 ng/ul

RT: 27.72 min Scan# 4154

Delta R.T. -0.01 min

Lab File: BM014945.D

Acq: 03 May 2018 16:20

Instrument :

BNA_M

ClientSampleId :

Tot Ion:276 Resp: 100412

Ion Ratio Lower Upper

276 100

138 24.3 8.5 12.7#

277 24.8 18.6 28.0

