

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050318\
 Data File : BM014959.D
 Acq On : 04 May 2018 01:05
 Operator : SJ/JU
 Sample : J2554-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 04 05:57:22 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 04 05:51:01 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.49	152	383147	20.00	ng/ul	0.00
18) Naphthalene-d8	11.33	136	1557056	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	775664	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.81	188	1548397	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1501300	20.00	ng/ul	0.00
83) Perylene-d12	24.37	264	1650767	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.64	96	47794	5.45	ng/uL	0.00
5) Phenol-d5	7.62	99	843124	28.46	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.79	67	586582	30.88	ng/ul	0.00
9) 2-Chlorophenol-d4	8.01	132	716083	28.90	ng/ul	0.00
13) 4-Methylphenol-d8	9.19	113	544674	23.06	ng/ul	0.00
19) Nitrobenzene-d5	9.67	128	322142	28.61	ng/ul	0.00
22) 2-Nitrophenol-d4	10.40	143	333006	29.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	584680	25.67	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	735482	32.71	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	1702762	28.12	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	2021110	27.03	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	274560	24.43	ng/ul	0.00
57) Fluorene-d10	16.07	176	1438219	27.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	177627	21.20	ng/ul	0.00
70) Anthracene-d10	17.91	188	2108773	29.22	ng/ul	0.00
76) Pyrene-d10	20.15	212	2201141	30.99	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.21	264	2579004	31.80	ng/ul	0.00
Target Compounds						
6) Phenol	7.65	94	58414	2.004	ng/ul#	82
44) Dimethylphthalate	14.53	163	383898	6.559	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM050318\
Data File : BM014959.D
Acq On : 04 May 2018 01:05
Operator : SJ/JU
Sample : J2554-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 04 05:57:22 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 04 05:51:01 2018
Response via : Initial Calibration

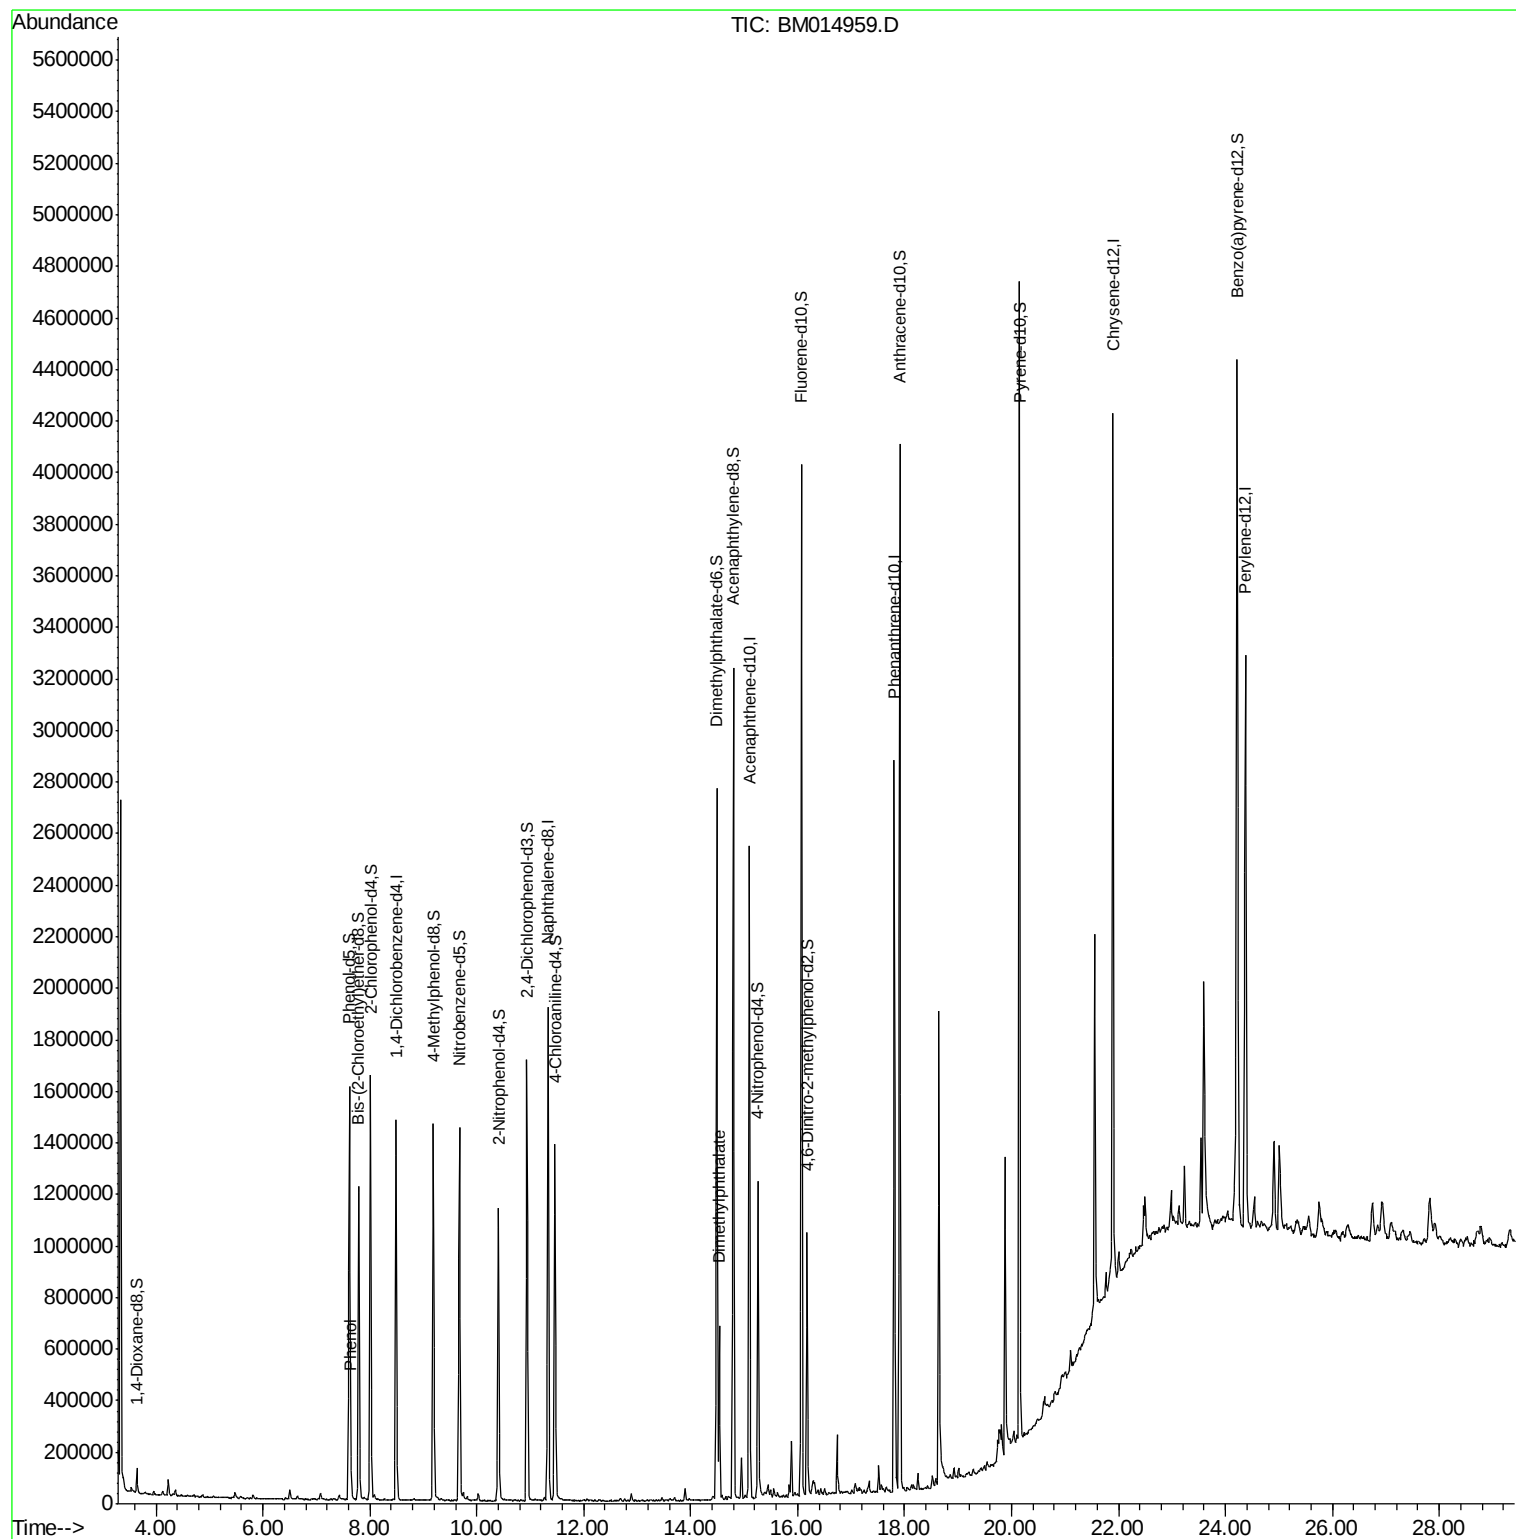

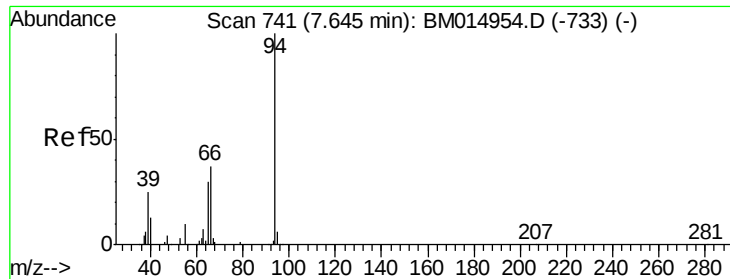





#6

Phenol

Concen: 2.004 ng/ul
 RT: 7.65 min Scan# 741
 Delta R.T. -0.00 min
 Lab File: BM014959.D
 Acq: 04 May 2018 01:05

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 94 Resp: 58414
 Ion Ratio Lower Upper
 94 100
 65 31.4 28.2 42.4
 66 40.4 47.2 70.8#

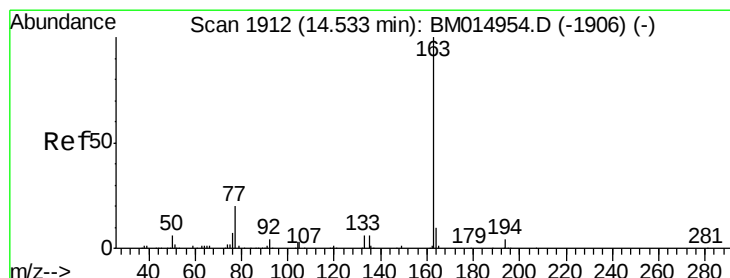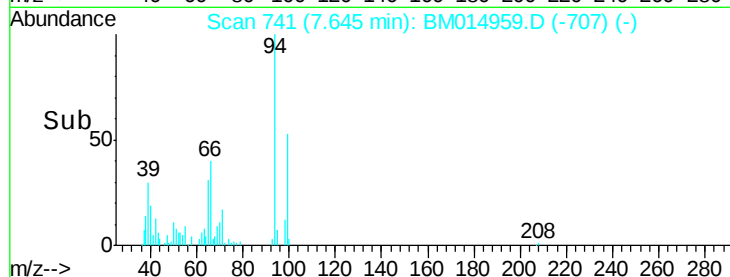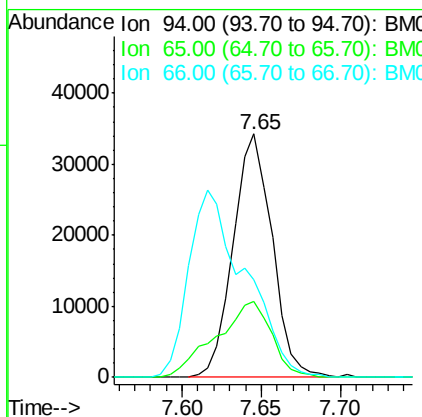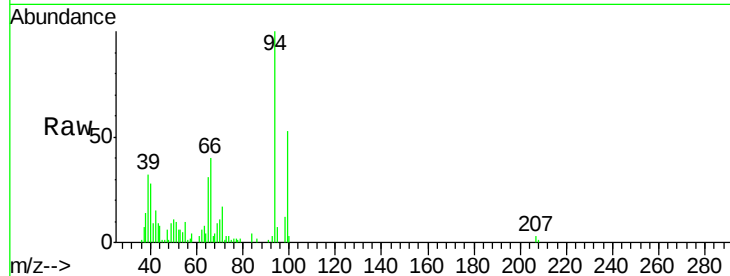

#44

Dimethylphthalate

Concen: 6.559 ng/ul
 RT: 14.53 min Scan# 1912
 Delta R.T. -0.00 min
 Lab File: BM014959.D
 Acq: 04 May 2018 01:05

Tgt Ion: 163 Resp: 383898
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.5 5.3
 164 10.0 8.2 12.4

