




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
 Data File : BM034911.D
 Acq On : 04 May 2022 03:55
 Operator : CG/JU
 Sample : N2562-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW477

Manual IntegrationsAPPROVED

Quant Time: May 04 05:54:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 02:59:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

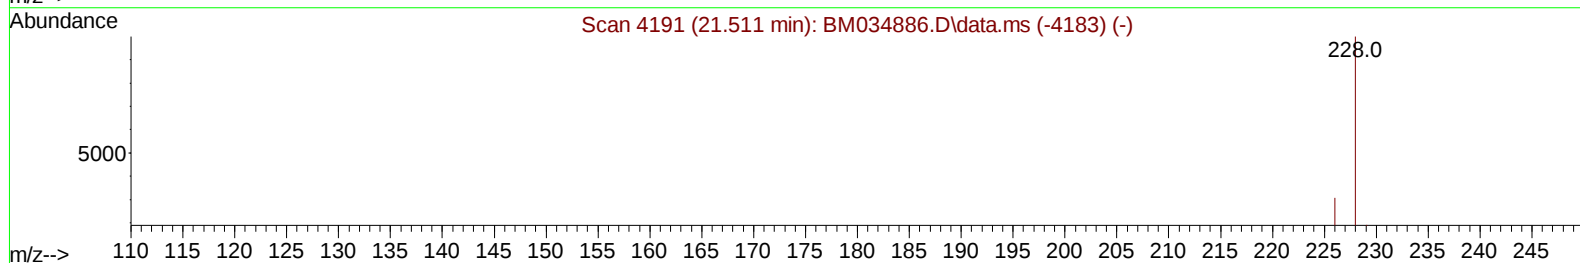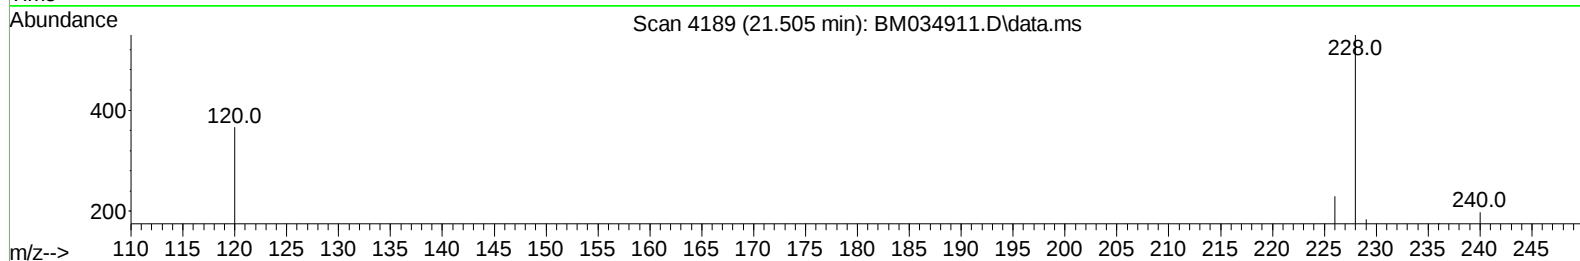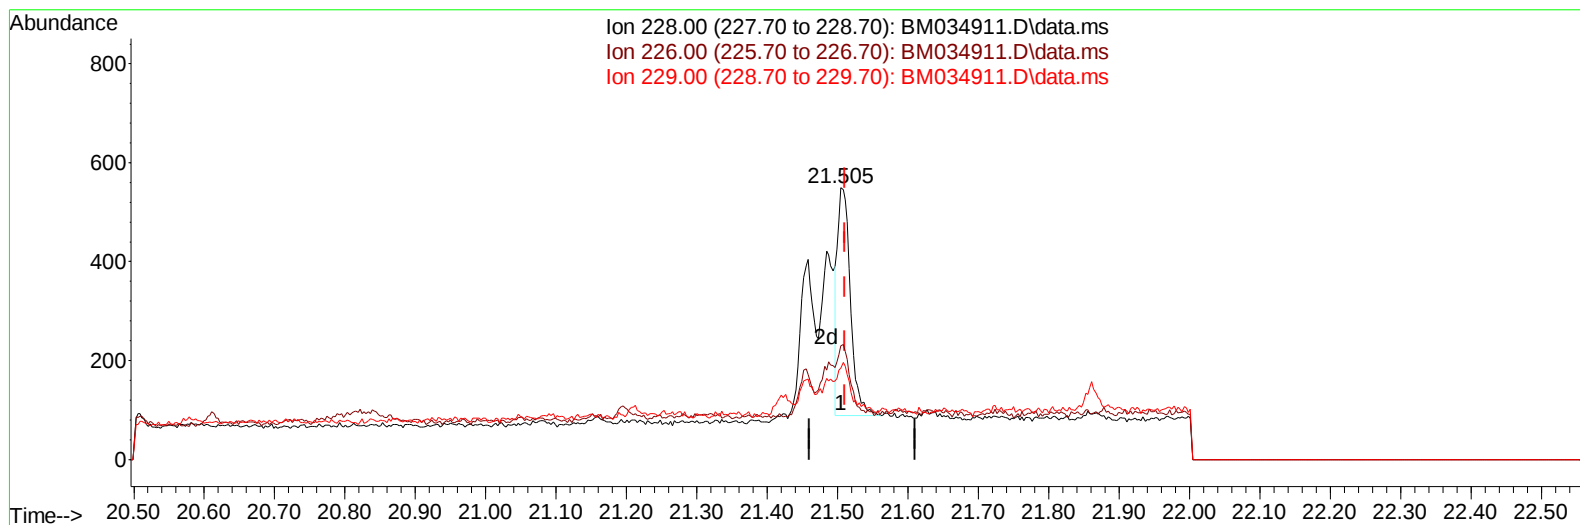

TIC: BM034911.D\data.ms

(22) Chrysene

21.505min (-0.006) 0.01 ng/u1

response 593

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	32.30	41.89#
229.00	20.90	33.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
 Data File : BM034911.D
 Acq On : 04 May 2022 03:55
 Operator : CG/JU
 Sample : N2562-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW477

Manual IntegrationsAPPROVED

Quant Time: May 04 05:54:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 02:59:36 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

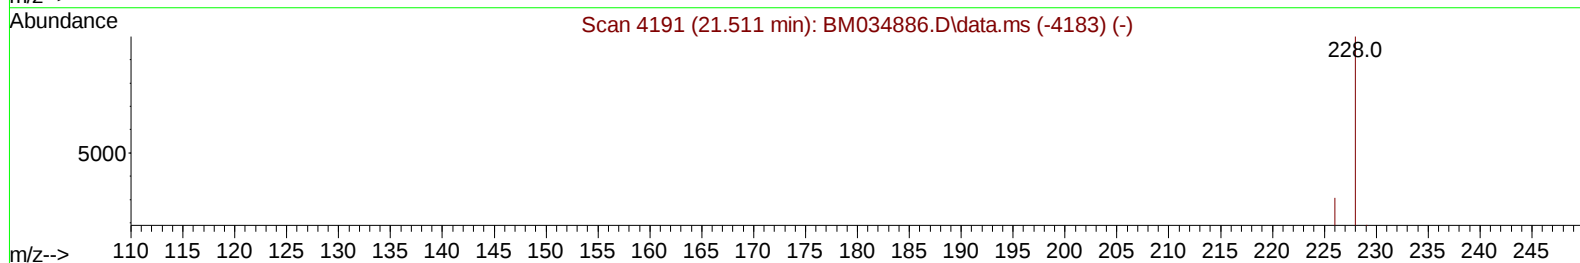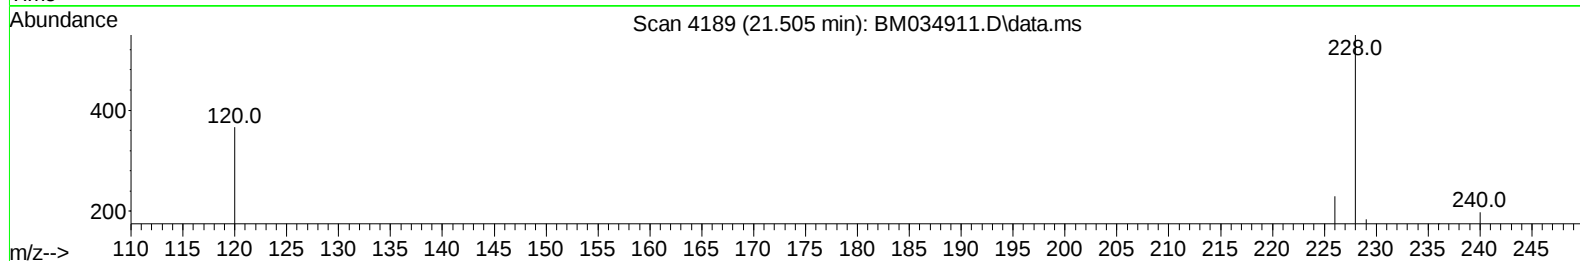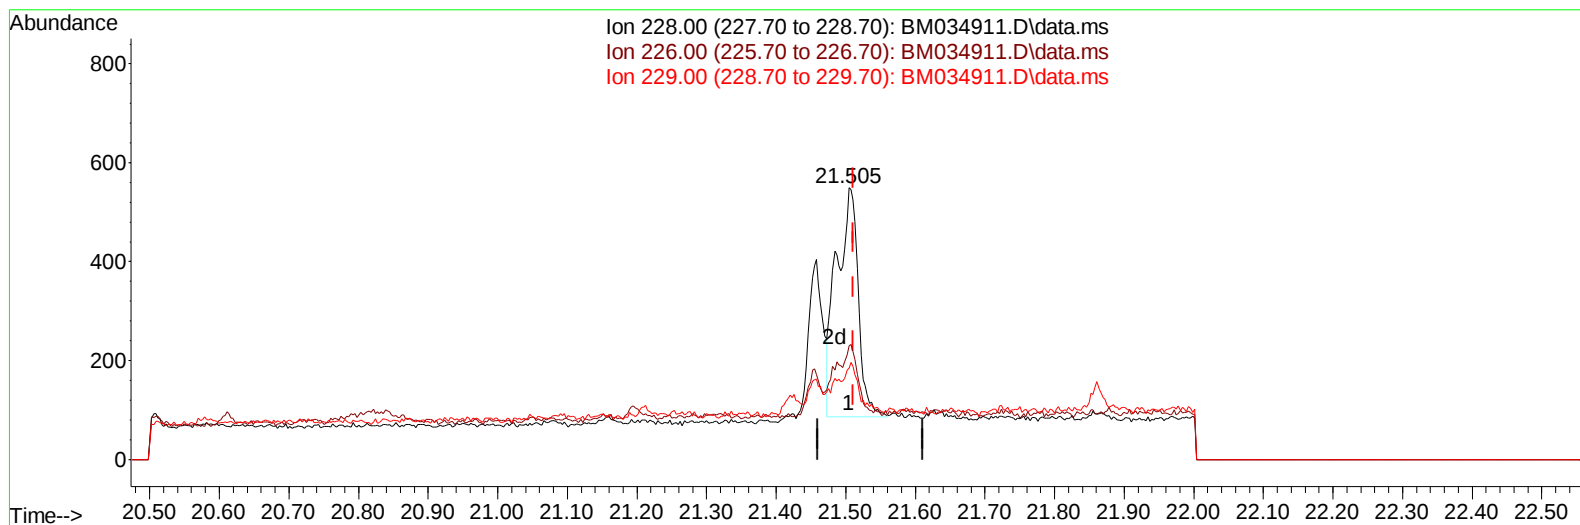

TIC: BM034911.D\data.ms

(22) Chrysene

21.505min (-0.006) 0.02 ng/u1 m

response 1006

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	32.30	41.89#
229.00	20.90	33.52#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
 Data File : BM034911.D
 Acq On : 04 May 2022 03:55
 Operator : CG/JU
 Sample : N2562-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW477

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 05:54:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 02:59:36 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.930	152		5151	0.400	ng/ul	0.00
4) Naphthalene-d8	10.726	136		13640	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.557	164		7715	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.297	188		14542	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.473	240		10450	0.400	ng/ul	# 0.00
23) Perylene-d12	23.855	264		11311	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.369	96		26945	4.730	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152		6379	0.333	ng/ul	0.00
18) Fluoranthene-d10	19.322	212		11832	0.359	ng/ul	0.00
Target Compounds							Qvalue
22) Chrysene	21.505	228		1006m	0.023	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
Data File : BM034911.D
Acq On : 04 May 2022 03:55
Operator : CG/JU
Sample : N2562-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW477

Manual IntegrationsAPPROVED

Quant Time: May 04 05:54:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 02:59:36 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

