

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
 Data File : BM034911.D
 Acq On : 04 May 2022 03:55
 Operator : CG/JU
 Sample : N2562-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW477

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 05:54:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 02:59:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5151	0.400	ng/u1	0.00
4) Naphthalene-d8	10.726	136	13640	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.557	164	7715	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.297	188	14542	0.400	ng/u1	# 0.00
17) Chrysene-d12	21.473	240	10450	0.400	ng/u1	# 0.00
23) Perylene-d12	23.855	264	11311	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	26945	4.730	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.316	152	6379	0.333	ng/u1	0.00
18) Fluoranthene-d10	19.322	212	11832	0.359	ng/u1	0.00
Target Compounds						
22) Chrysene	21.505	228	1006m	0.023	ng/u1	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
Data File : BM034911.D
Acq On : 04 May 2022 03:55
Operator : CG/JU
Sample : N2562-16
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW477

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022


Quant Time: May 04 05:54:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 02:59:36 2022
Response via : Initial Calibration

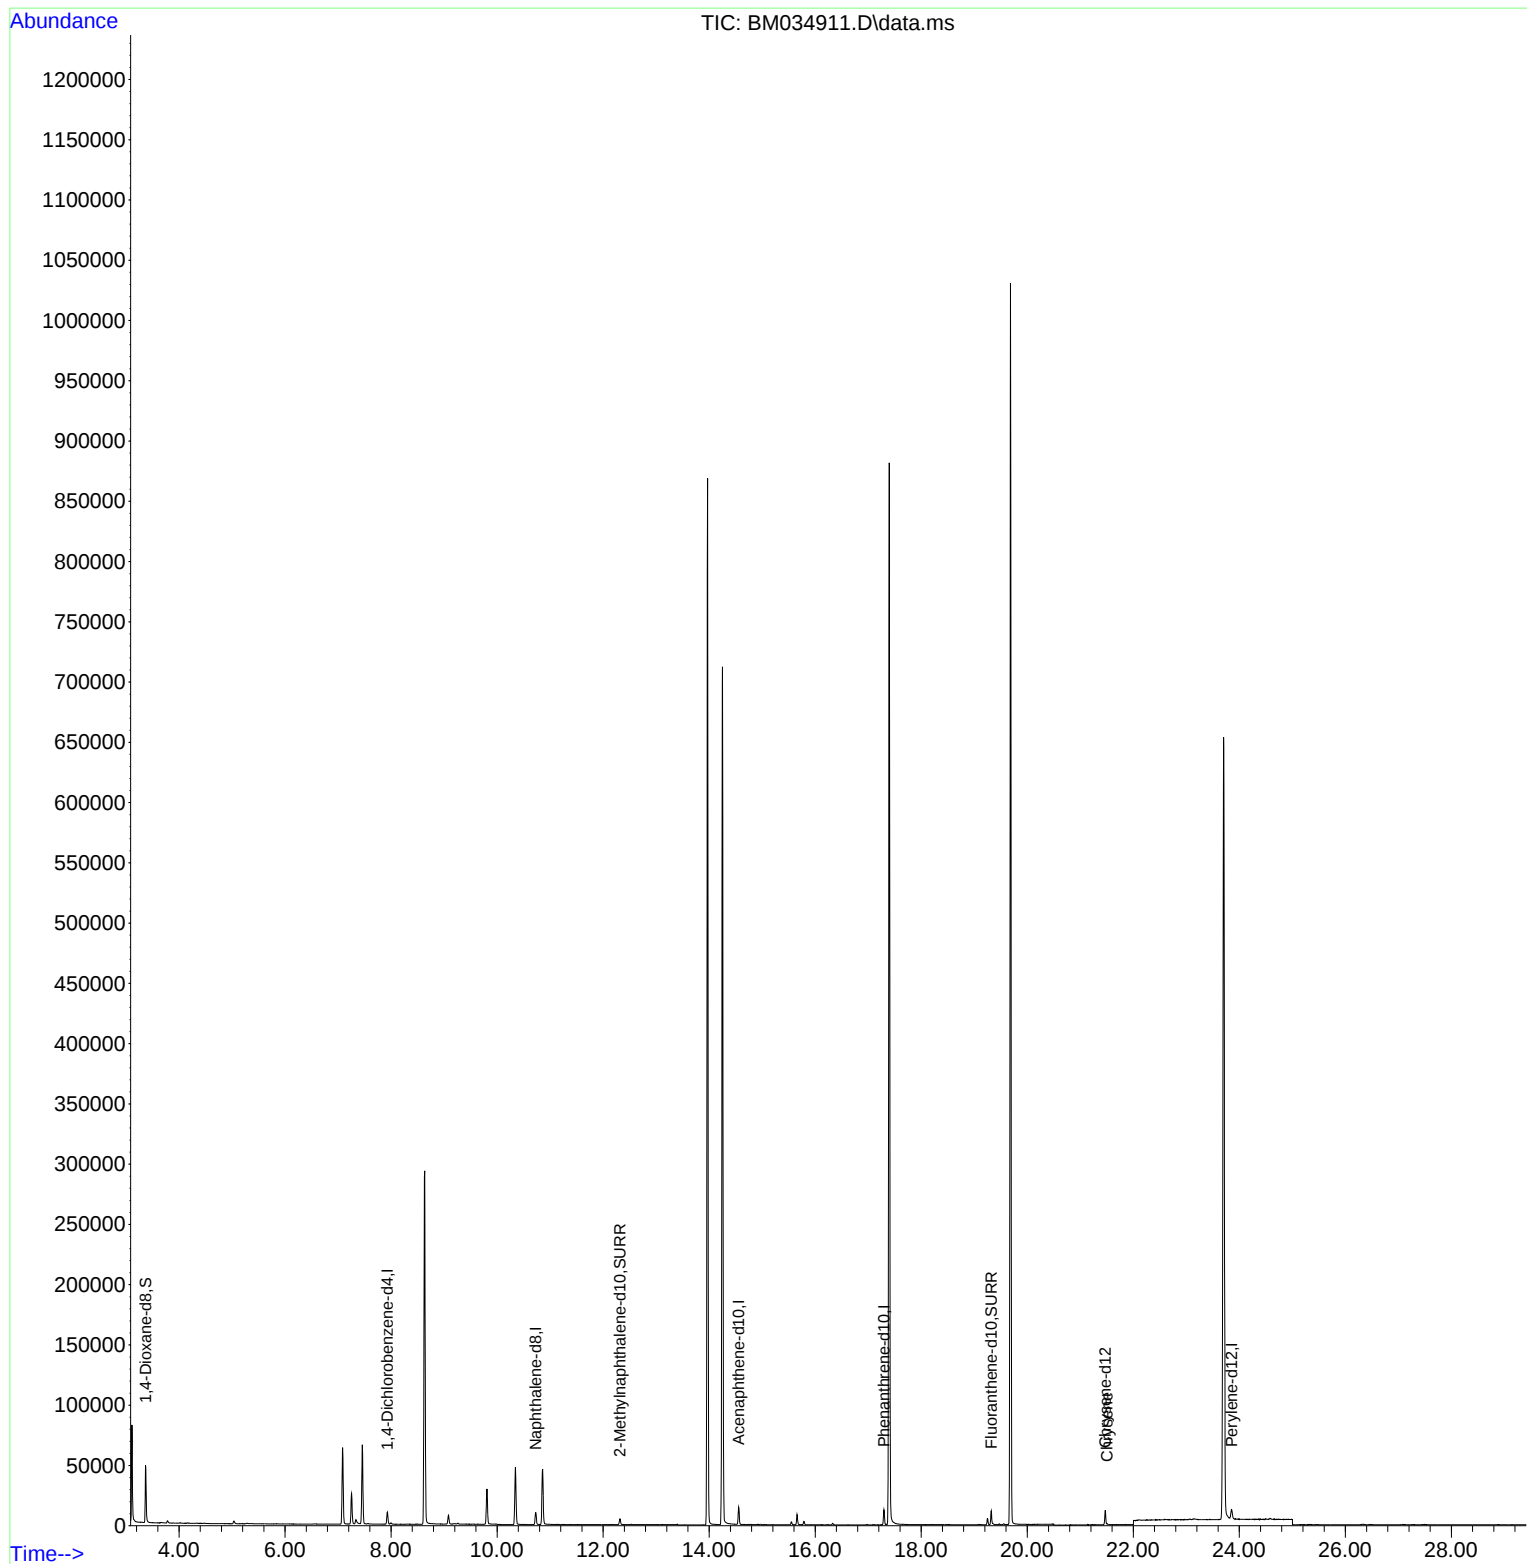

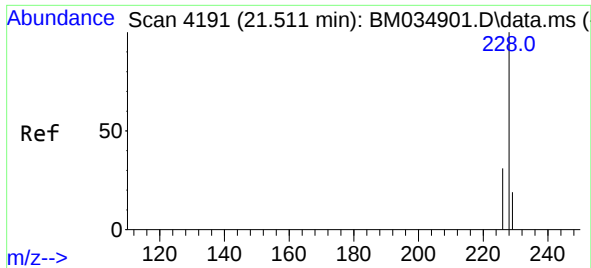

#22
Chrysene
Concen: 0.023 ng/ul m
RT: 21.505 min Scan# 41
Delta R.T. -0.006 min
Lab File: BM034911.D
Acq: 04 May 2022 03:55

Instrument :
BNA_M
ClientSampleId :
EW477

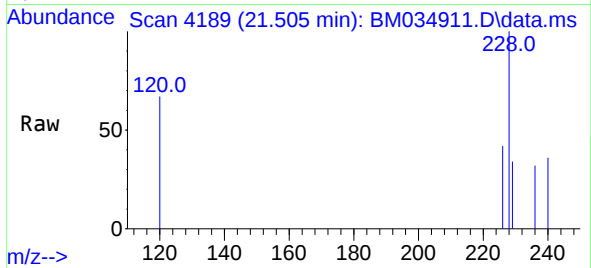

Tgt Ion:228 Resp: 1000
Ion Ratio Lower Upper
228 100
226 41.9 25.8 38.8
229 33.5 16.7 25.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

