

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
 Data File : BM034913.D
 Acq On : 04 May 2022 05:06
 Operator : CG/JU
 Sample : N2621-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFFJ0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
 Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 05:54:20 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 02:59:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5813	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.726	136	15683	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.557	164	8908	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.297	188	16316	0.400	ng/ul	0.00
17) Chrysene-d12	21.473	240	10927	0.400	ng/ul	# 0.00
23) Perylene-d12	23.855	264	11404	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	32785	5.099	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.316	152	8404	0.381	ng/ul	0.00
18) Fluoranthene-d10	19.323	212	15144	0.439	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.407	88	612m	0.100	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050322\
Data File : BM034913.D
Acq On : 04 May 2022 05:06
Operator : CG/JU
Sample : N2621-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFFJ0


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Quant Time: May 04 05:54:20 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 02:59:36 2022
Response via : Initial Calibration

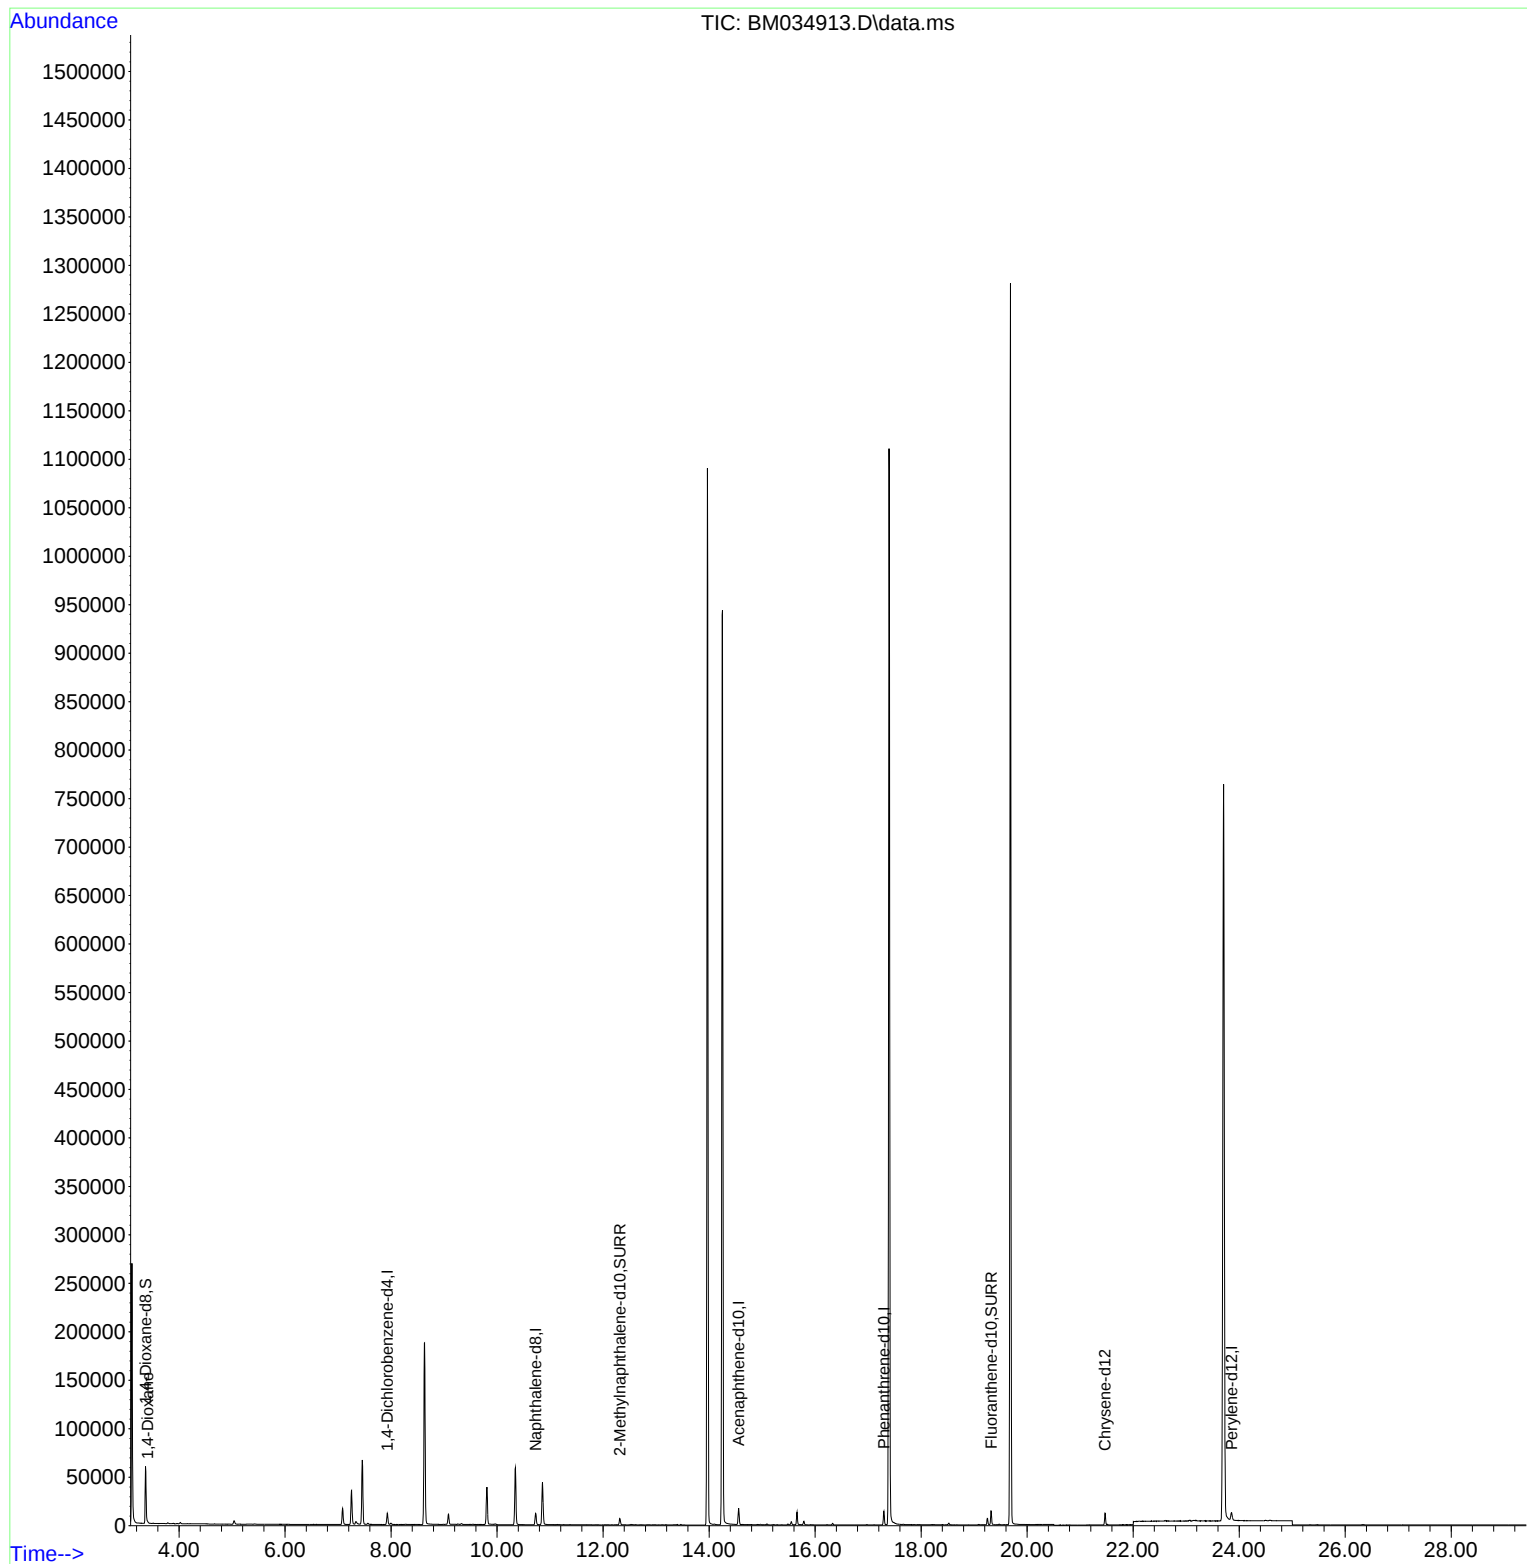


Abundance Scan 77 (3.407 min): BM034901.D\data.ms (-71) #2

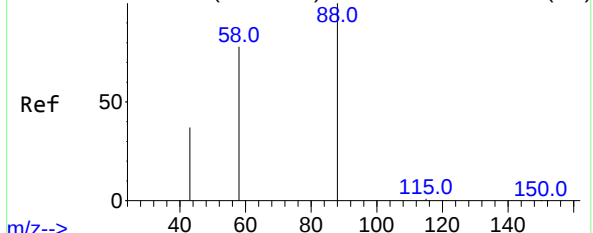

1,4-Dioxane
Concen: 0.100 ng/ul m
RT: 3.407 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM034913.D
Acq: 04 May 2022 05:06

Instrument :
BNA_M
ClientSampleId :
BFFJ0

Abundance Scan 77 (3.407 min): BM034913.D\data.ms

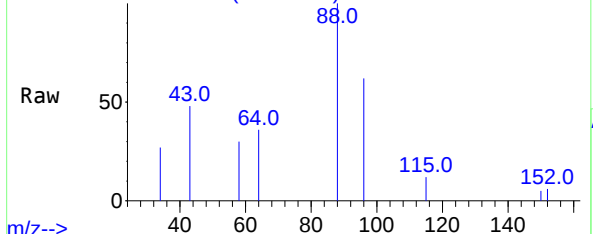

Tgt Ion: 88 Resp: 612

Ion	Ratio	Lower	Upper
88	100		
43	48.4	49.7	74.5
58	29.9	52.5	78.7

Manual Integrations
APPROVED
Reviewed By :Jagrut Upadhyay 05/04/2022
Supervised By :Yogesh Patel 05/05/2022

Abundance Scan 77 (3.407 min): BM034913.D\data.ms (-65)

