

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050322\  
 Data File : BM034914.D  
 Acq On : 04 May 2022 05:42  
 Operator : CG/JU  
 Sample : N2621-03  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BFFJ6

Quant Time: May 04 07:01:19 2022  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM042222.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed May 04 02:59:36 2022  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|--------|------|----------|-------|--------|----------|
| -----                       |        |      |          |       |        |          |
| Internal Standards          |        |      |          |       |        |          |
| 1) 1,4-Dichlorobenzene-d4   | 7.930  | 152  | 5223     | 0.400 | ng/ul  | 0.00     |
| 4) Naphthalene-d8           | 10.727 | 136  | 13792    | 0.400 | ng/ul  | # 0.00   |
| 9) Acenaphthene-d10         | 14.557 | 164  | 7902     | 0.400 | ng/ul  | 0.00     |
| 13) Phenanthrene-d10        | 17.296 | 188  | 14877    | 0.400 | ng/ul  | # 0.00   |
| 17) Chrysene-d12            | 21.471 | 240  | 10739    | 0.400 | ng/ul  | # 0.00   |
| 23) Perylene-d12            | 23.856 | 264  | 11632    | 0.400 | ng/ul  | # 0.00   |
| System Monitoring Compounds |        |      |          |       |        |          |
| 3) 1,4-Dioxane-d8           | 3.369  | 96   | 27097    | 4.691 | ng/ul  | 0.00     |
| 6) 2-Methylnaphthalene-d10  | 12.316 | 152  | 7171     | 0.370 | ng/ul  | 0.00     |
| 18) Fluoranthene-d10        | 19.322 | 212  | 13784    | 0.407 | ng/ul  | 0.00     |
| Target Compounds            |        |      |          |       |        |          |
|                             |        |      |          |       | Qvalue |          |
| 5) Naphthalene              | 10.776 | 128  | 1595     | 0.040 | ng/ul  | 97       |
| -----                       |        |      |          |       |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM050322\  
Data File : BM034914.D  
Acq On : 04 May 2022 05:42  
Operator : CG/JU  
Sample : N2621-03  
Misc :  
ALS Vial : 30 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BFFJ6


Quant Time: May 04 07:01:19 2022  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM042222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 04 02:59:36 2022  
Response via : Initial Calibration

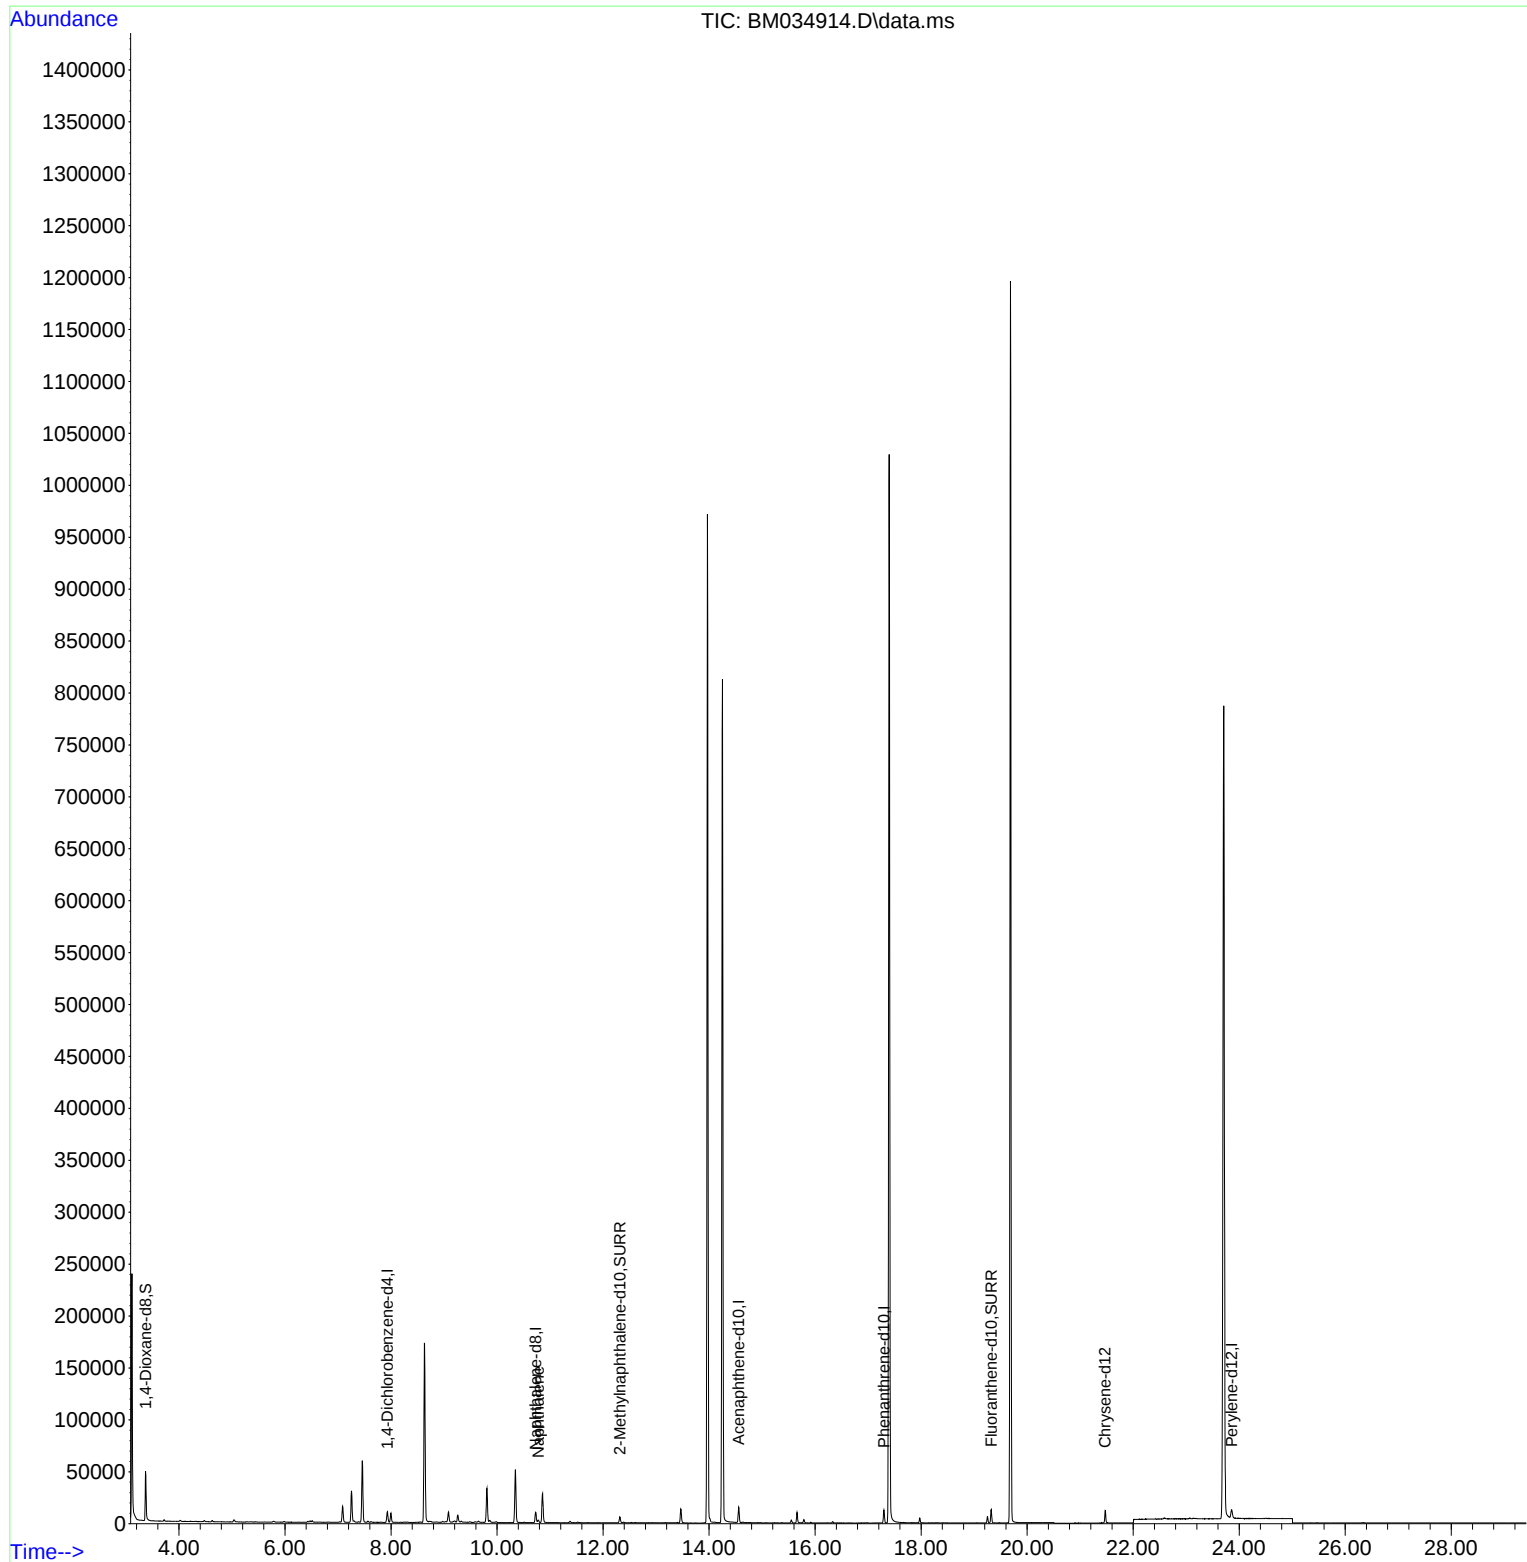

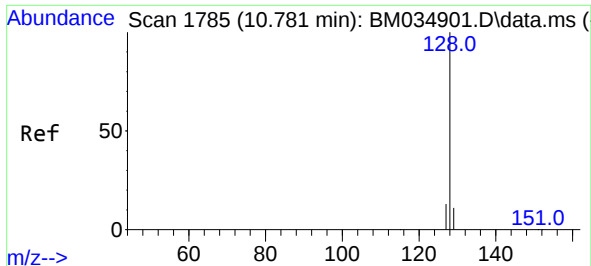

#5  
Naphthalene  
Concen: 0.040 ng/ul  
RT: 10.776 min Scan# 11  
Delta R.T. -0.005 min  
Lab File: BM034914.D  
Acq: 04 May 2022 05:42

Instrument :  
BNA\_M  
ClientSampleId :  
BFFJ6

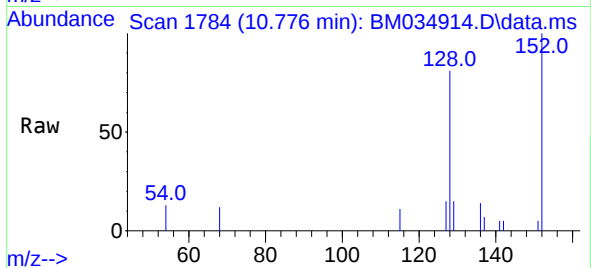

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 128   | Resp: | 1595  |
| Ion      | Ratio | Lower | Upper |
| 128      | 100   |       |       |
| 129      | 18.3  | 13.4  | 20.2  |
| 127      | 18.1  | 15.2  | 22.8  |

