


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050415\
 Data File : BM001185.D
 Acq On : 04 May 2015 09:01
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

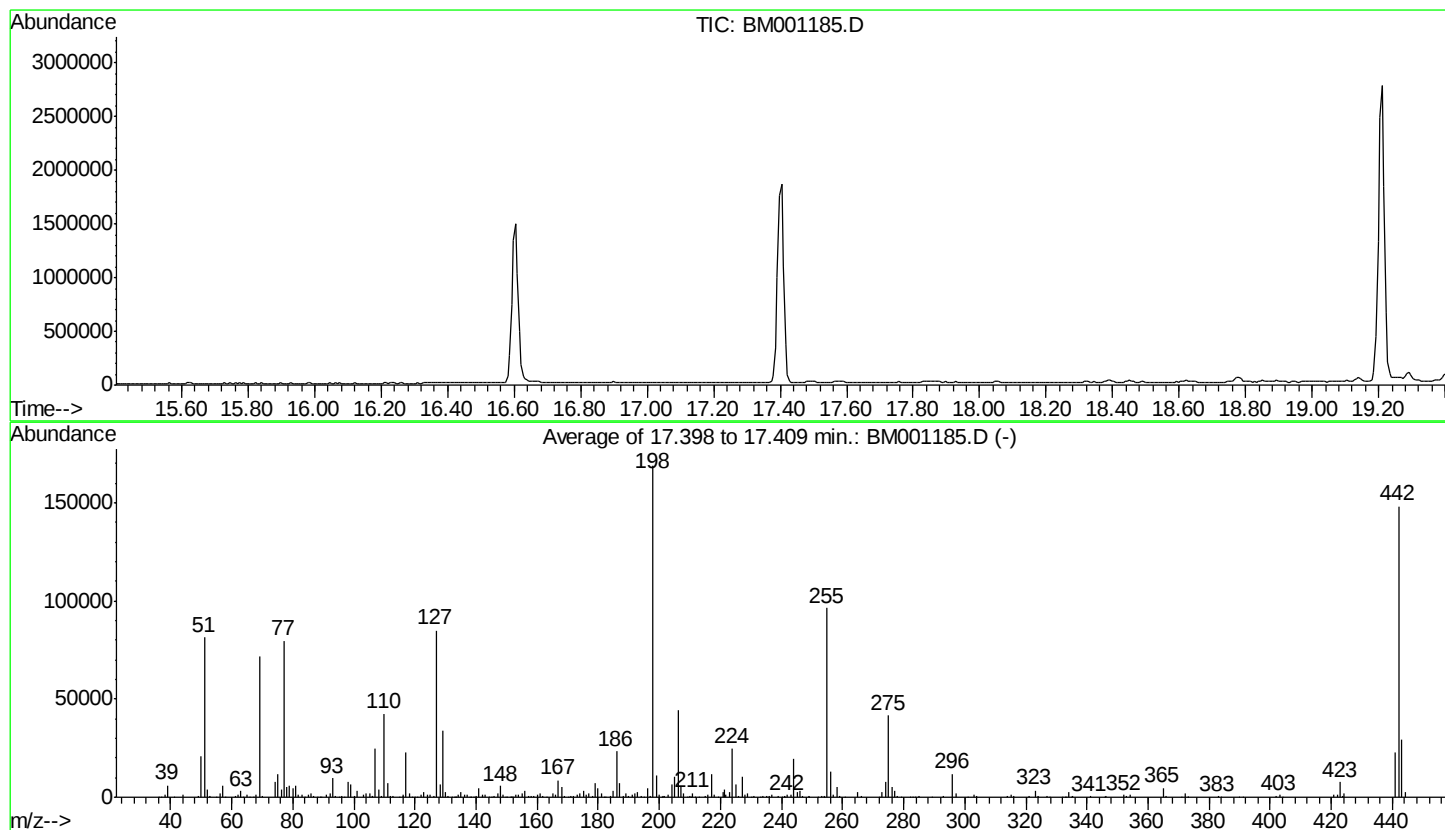

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.1	81216	PASS
68	69	0.00	2	1.6	1167	PASS
69	198	0.00	100	42.3	71464	PASS
70	69	0.00	2	0.7	505	PASS
127	198	10	80	50.3	84882	PASS
197	198	0.00	2	0.4	701	PASS
198	198	100	100	100.0	168850	PASS
199	198	5	9	6.4	10886	PASS
275	198	10	60	24.6	41557	PASS
365	198	1	100	2.8	4671	PASS
441	442	0.01	24	15.4	22792	PASS
442	198	50	100	87.7	148112	PASS
443	442	15	24	19.8	29344	PASS