


Data Path : Z:\HPCHEM1\BNA_M\Data\BM050415\
 Data File : BM001188.D
 Acq On : 04 May 2015 16:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

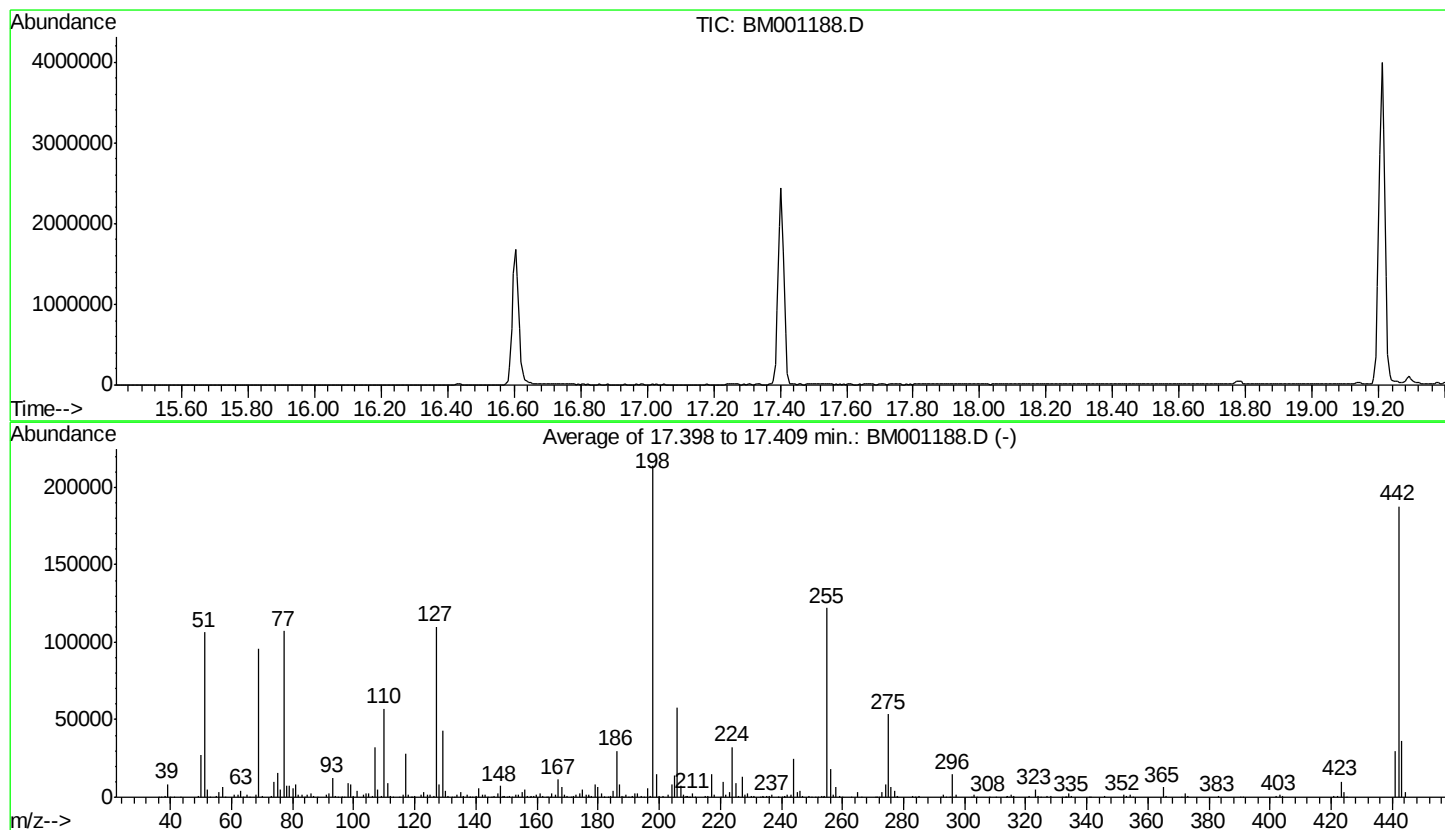

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	106277	PASS
68	69	0.00	2	1.6	1536	PASS
69	198	0.00	100	44.7	95549	PASS
70	69	0.00	2	0.6	577	PASS
127	198	10	80	51.5	110144	PASS
197	198	0.00	2	0.6	1189	PASS
198	198	100	100	100.0	213930	PASS
199	198	5	9	7.0	15074	PASS
275	198	10	60	25.1	53634	PASS
365	198	1	100	3.0	6506	PASS
441	442	0.01	24	15.7	29373	PASS
442	198	50	100	87.7	187626	PASS
443	442	15	24	19.2	36088	PASS