

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050417\
 Data File : BM009890.D
 Acq On : 04 May 2017 15:45
 Operator : SJ/MA
 Sample : I2867-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHT93

Quant Time: May 05 08:55:06 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 01:34:35 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	127538	20.00	ng/ul	0.00
18) Naphthalene-d8	10.60	136	531929	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	331815	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	814579	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	850961	20.00	ng/ul	0.01
83) Perylene-d12	23.73	264	742001	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	7273	2.63	ng/uL	0.00
5) Phenol-d5	6.99	99	210303	15.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.14	67	162562	17.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.34	132	142464	16.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	157780	14.61	ng/ul	0.00
19) Nitrobenzene-d5	8.97	128	71127	16.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.69	143	78231	17.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	149874	16.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	87479	7.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.86	166	471227	16.33	ng/ul	0.00
46) Acenaphthylene-d8	14.15	160	626836	18.01	ng/ul	0.00
51) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	
57) Fluorene-d10	15.46	176	451538	17.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	3185	0.55	ng/ul	0.01
70) Anthracene-d10	17.32	188	747090	17.86	ng/ul	0.00
76) Pyrene-d10	19.62	212	788837	21.00	ng/ul	0.01
87) Benzo(a)pyrene-d12	23.58	264	637162	17.66	ng/ul	0.02


Target Compounds					Qvalue
44) Dimethylphthalate	13.91	163	91629	3.21 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM050417\
Data File : BM009890.D
Acq On : 04 May 2017 15:45
Operator : SJ/MA
Sample : I2867-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT93

Quant Time: May 05 08:55:06 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 01:34:35 2017
Response via : Initial Calibration

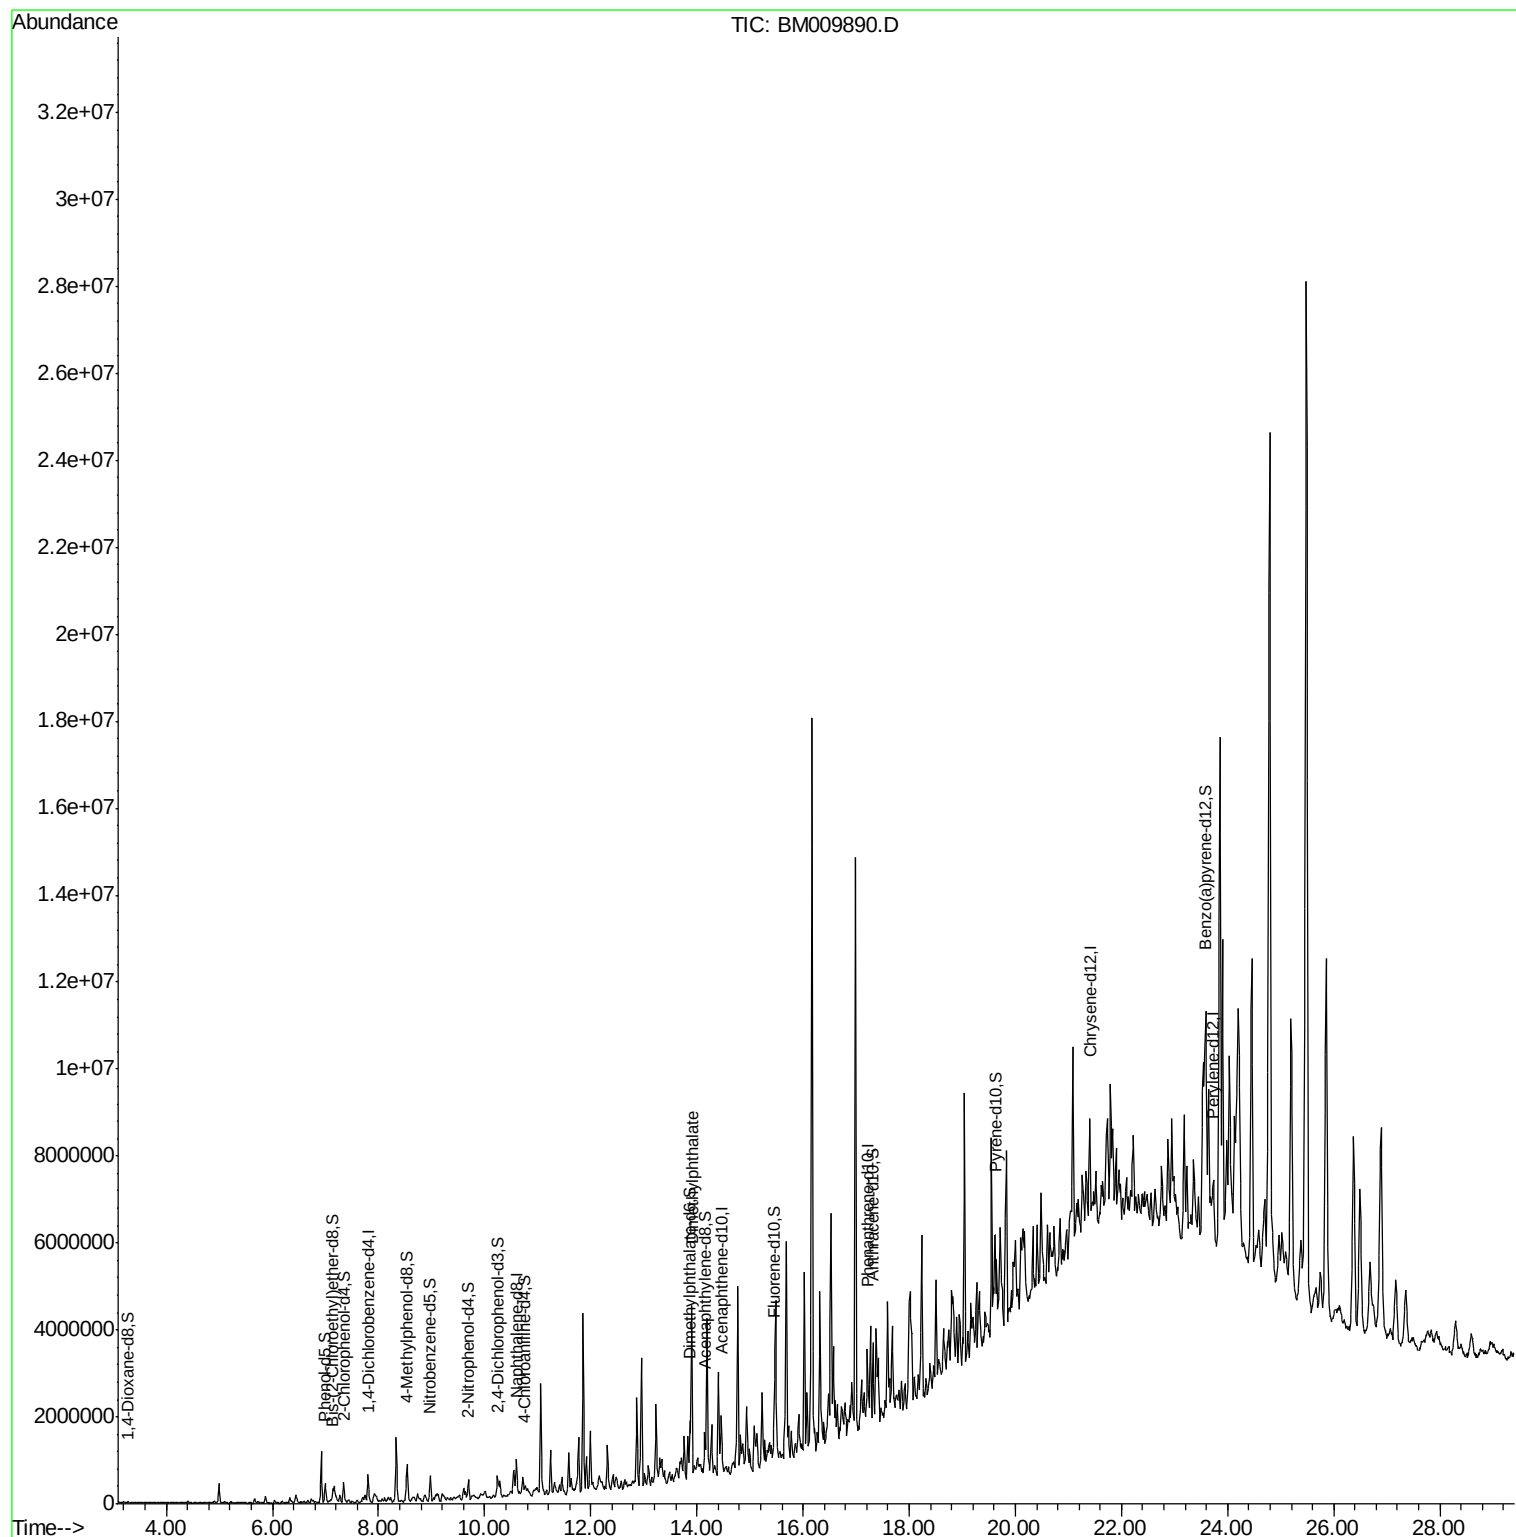

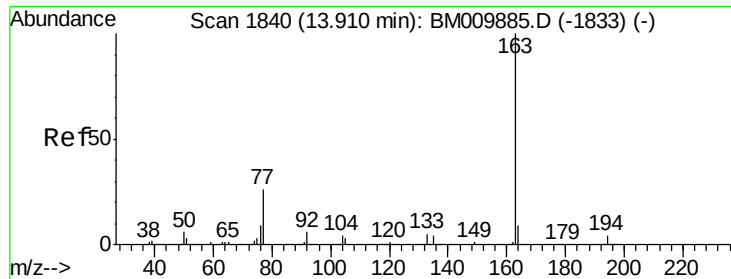

#44

Dimethylphthalate

Concen: 3.21 ng/ul

RT: 13.91 min Scan# 1840

Delta R.T. -0.00 min

Lab File: BM009890.D

Acq: 04 May 2017 15:45

Instrument :

BNA_M

ClientSampleId :

JHT93


Tgt Ion:163 Resp: 91629

Ion Ratio Lower Upper

163 100

194 4.4 3.0 4.6

164 11.1 8.6 12.8

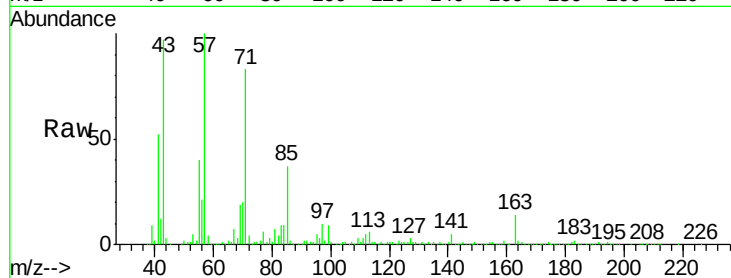

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

