

(QT Reviewed)

```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\  
Data File  : BM029788.D  
Acq On     : 04 May 2021   13:24  
Operator   : CG/JU  
Sample     : SSTD16015  
Misc       :  
ALS Vial   : 7      Sample Multiplier: 1
```


**Instrument :**  
BNA\_M  
**ClientSampleId :**  
SSTD160015

**Manual Integrations**  
**APPROVED**

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 14:03:50 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 04 12:20:39 2021  
Response via : Initial Calibration

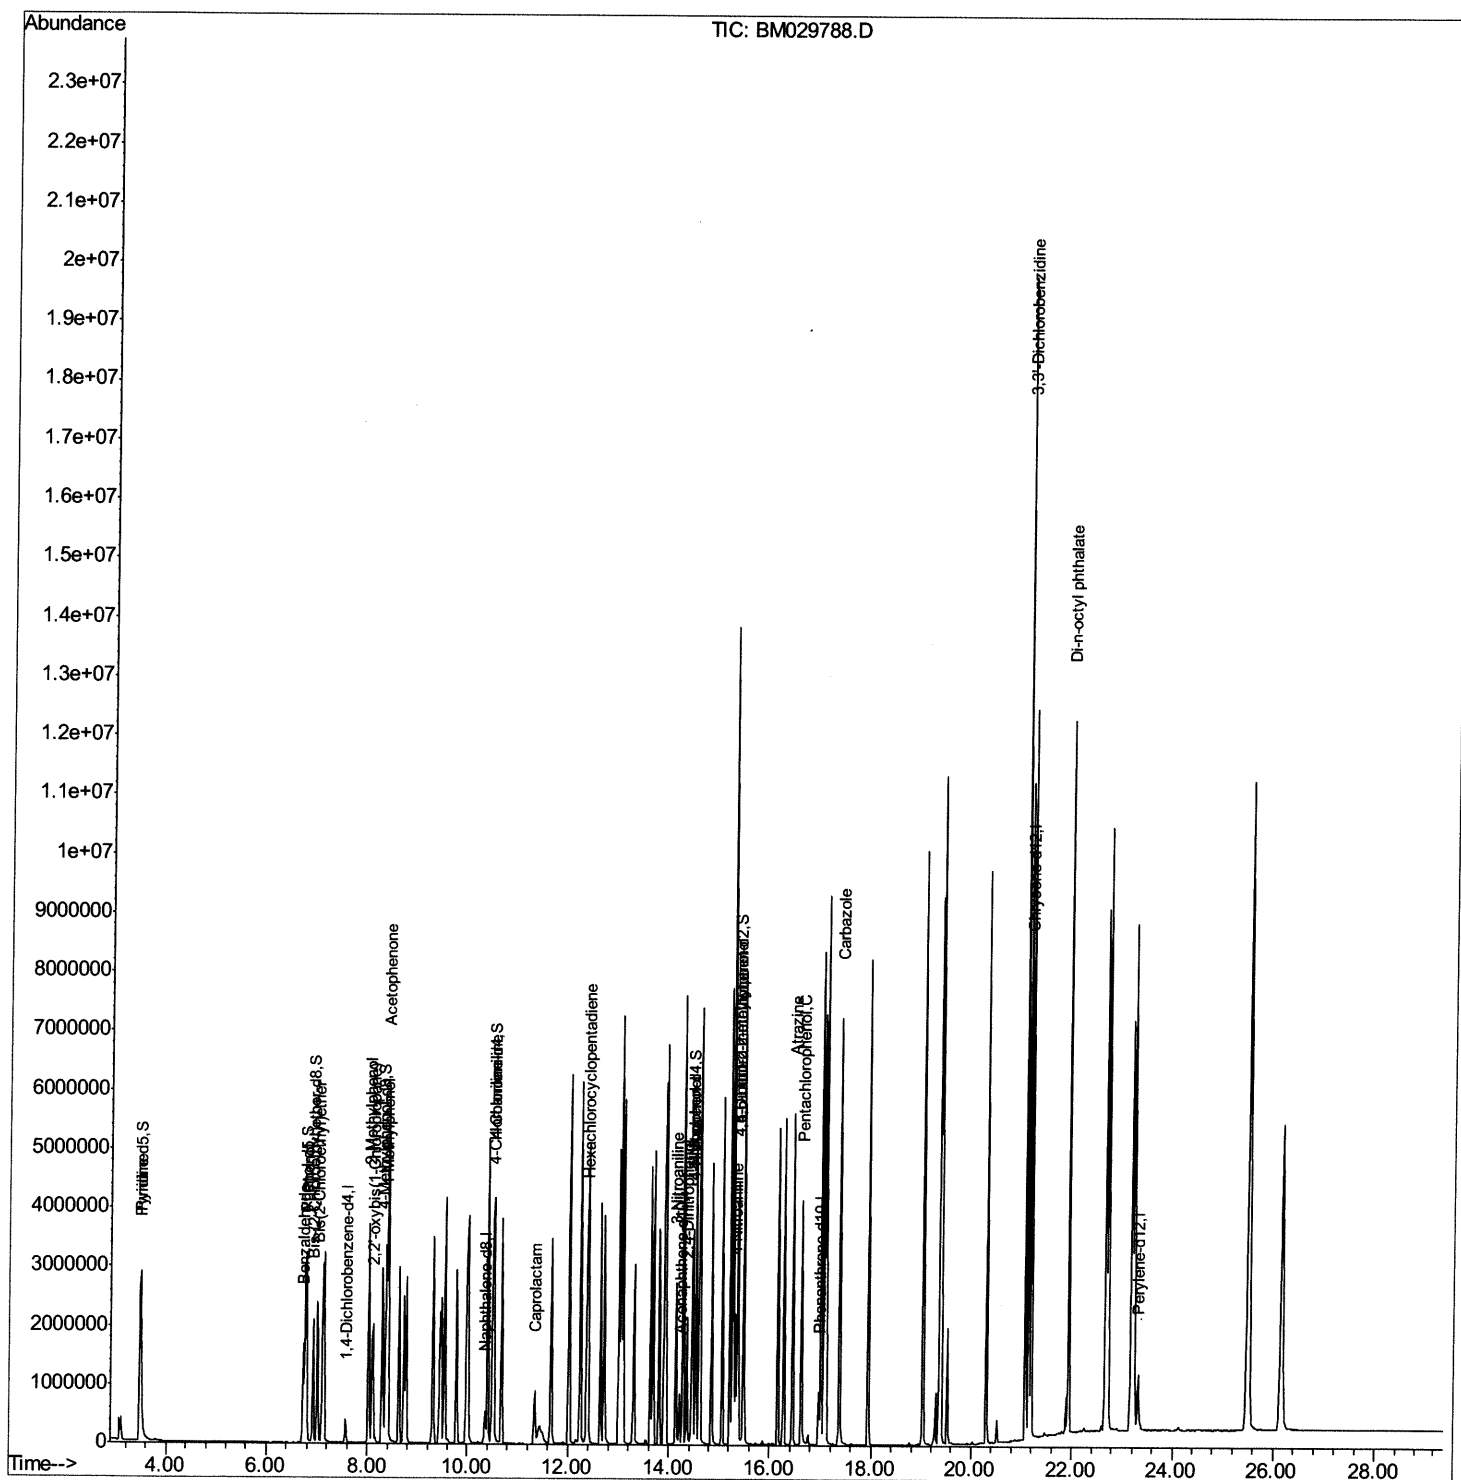

# Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\  
 Data File : BM029788.D  
 Acq On : 04 May 2021 13:24  
 Operator : CG/JU  
 Sample : SSTD16015  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1




**Instrument :**  
 BNA\_M  
**ClientSampleId :**  
 SSTD160015

**Manual Integrations**  
**APPROVED**

mohammad

5/5/2021 11:26:32 AM

Quant Time: Mav 04 13:54:31 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue May 04 12:20:39 2021  
 Response via : Initial Calibration

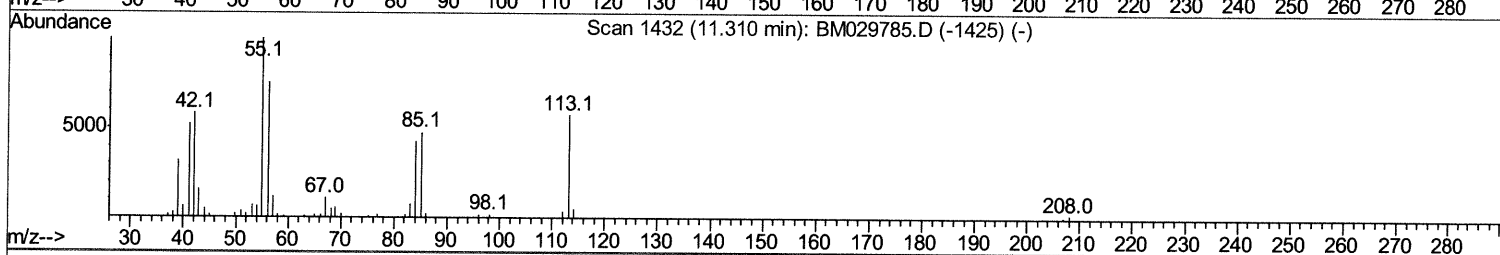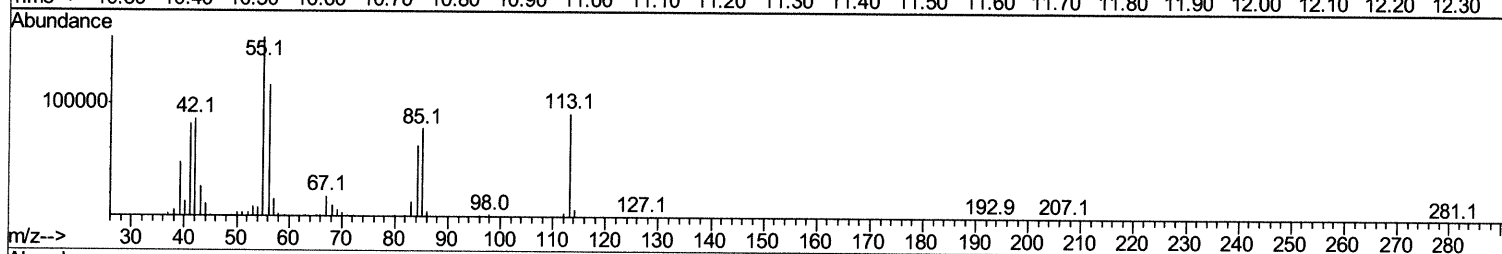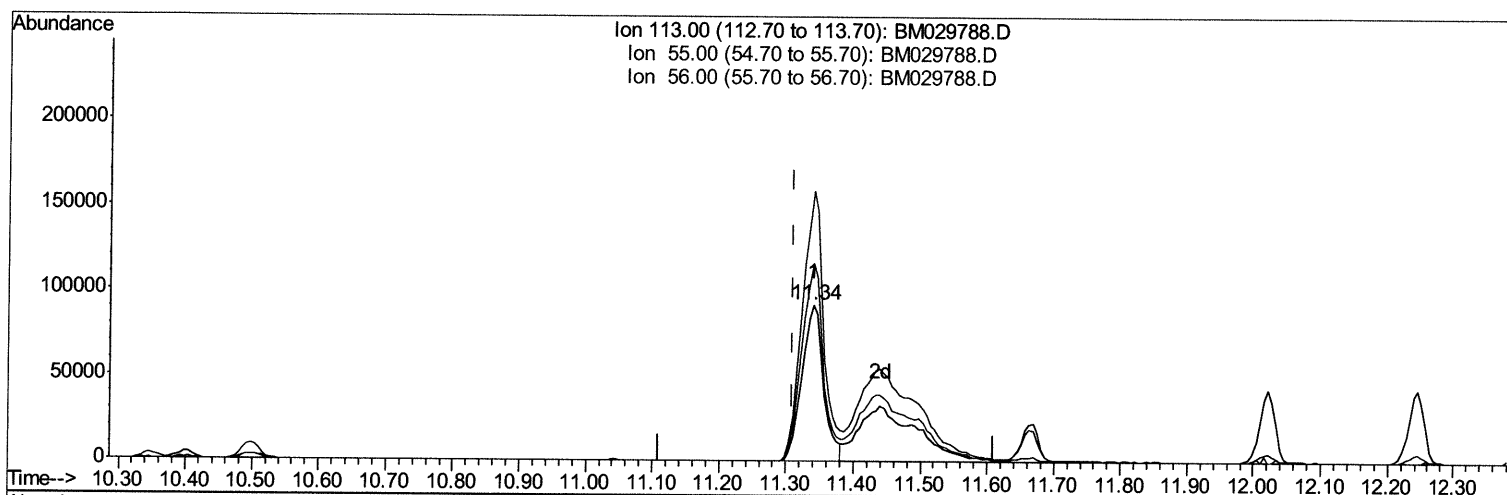

TIC: BM029788.D

(34) Caprolactam

11.339min (+0.029) 89.01ng/ul

response 204364

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 174.20 | 172.92 |
| 56.00  | 131.90 | 126.93 |
| 0.00   | 0.00   | 0.00   |

## Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\  
Data File : BM029788.D  
Acq On : 04 May 2021 13:24  
Operator : CG/JU  
Sample : SSTD16015  
Misc :  
ALS Vial : 7 Sample Multiplier: 1




Instrument :  
BNA\_M  
ClientSampleId :  
SSTD160015

Manual Integrations  
APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 13:54:31 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 04 12:20:39 2021  
Response via : Initial Calibration

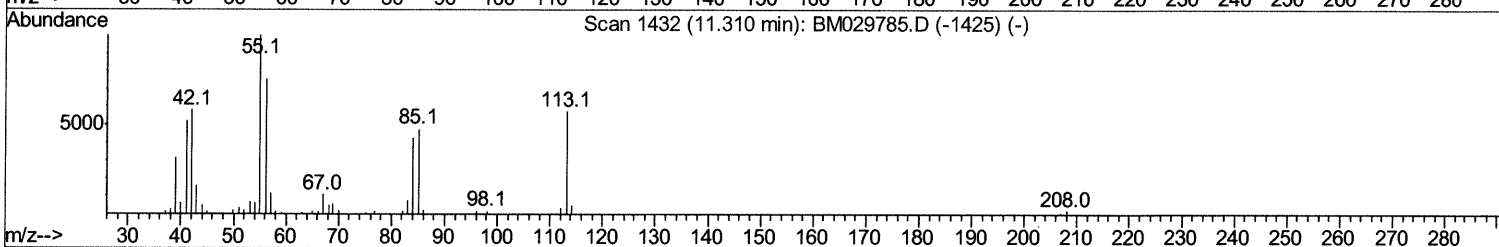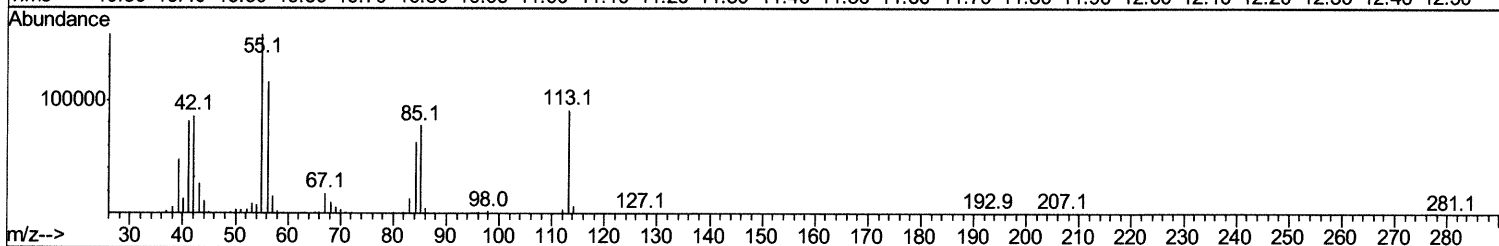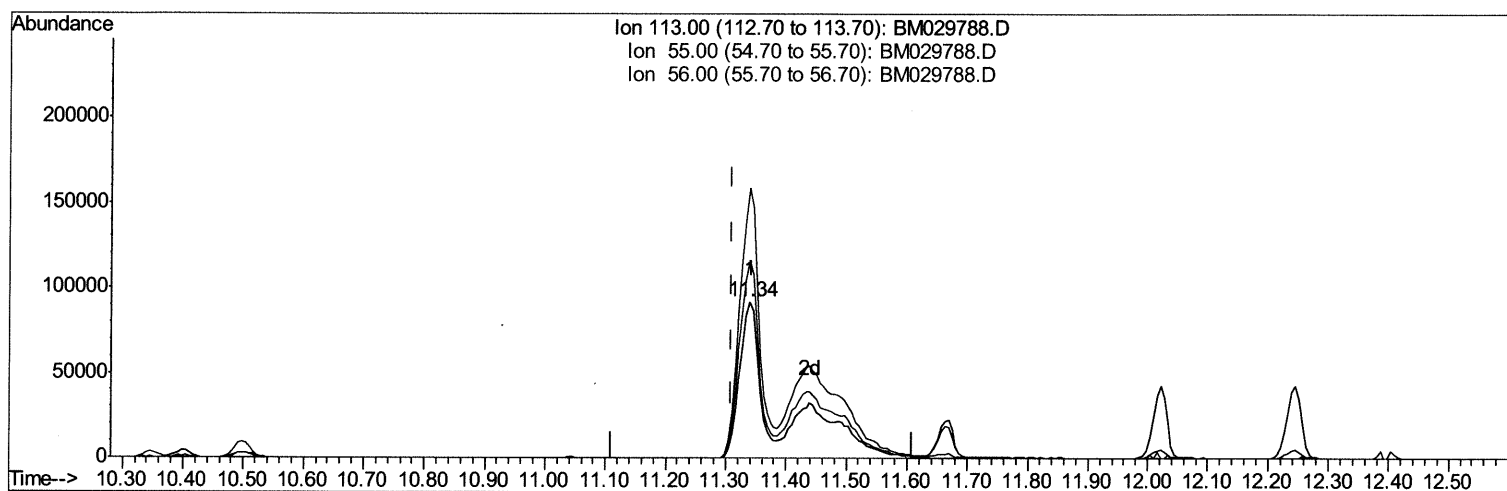

TIC: BM029788.D

(34) Caprolactam

11.339min (+0.029) 173.42ng/ul m 05/06/21 JU

response 398177

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100    | 100    |
| 55.00  | 174.20 | 172.92 |
| 56.00  | 131.90 | 126.93 |
| 0.00   | 0.00   | 0.00   |

# Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\  
 Data File : BM029788.D  
 Acq On : 04 May 2021 13:24  
 Operator : CG/JU  
 Sample : SSTD16015  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1




Instrument :  
 BNA\_M  
 ClientSampleId :  
 SSTD160015

Manual Integrations  
 APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 13:54:31 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue May 04 12:20:39 2021  
 Response via : Initial Calibration

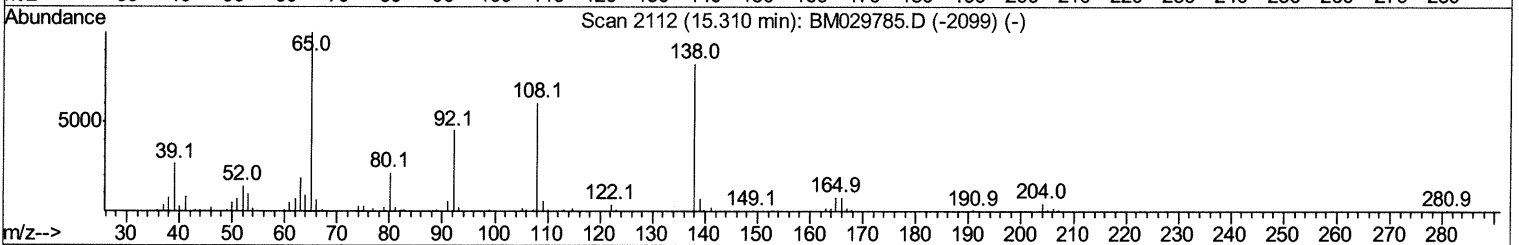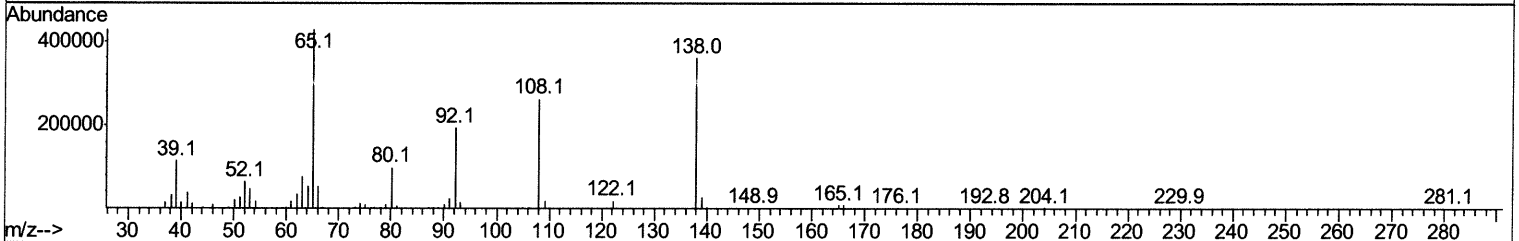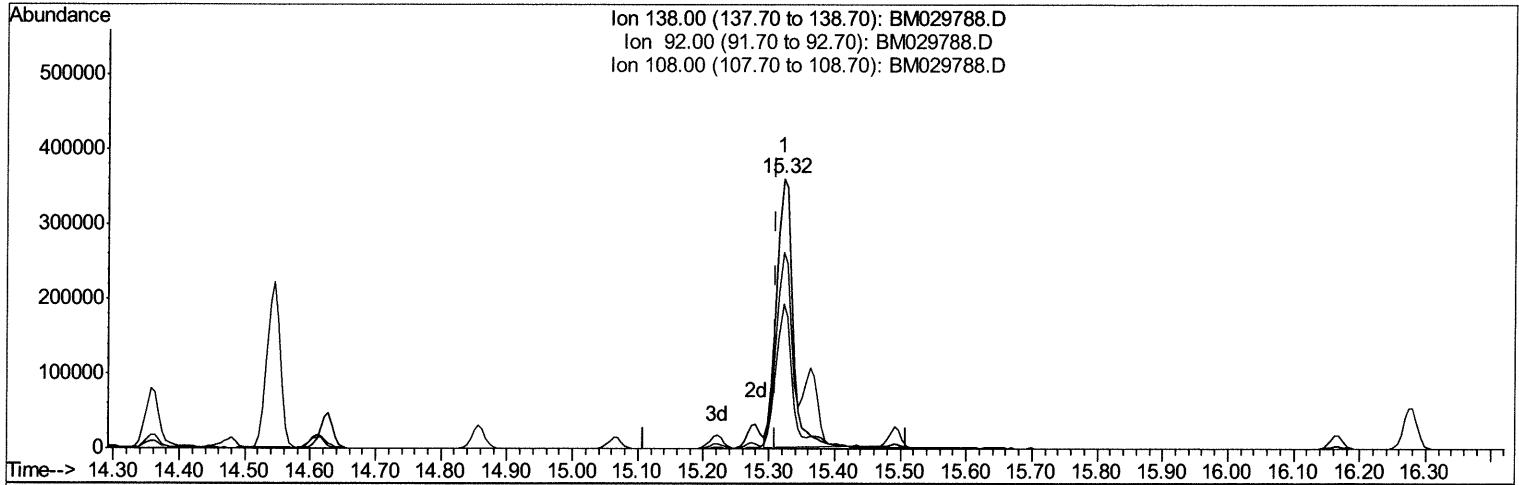

TIC: BM029788.D

(63) 4-Nitroaniline

15.321min (+0.012) 154.29ng/ul

response 621837

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 138.00 | 100   | 100   |
| 92.00  | 55.50 | 53.50 |
| 108.00 | 73.10 | 72.74 |
| 0.00   | 0.00  | 0.00  |

## Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\  
Data File : BM029788.D  
Acq On : 04 May 2021 13:24  
Operator : CG/JU  
Sample : SSTD16015  
Misc :  
ALS Vial : 7 Sample Multiplier: 1




Instrument :  
BNA\_M  
ClientSampleId :  
SSTD160015

Manual Integrations  
APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 13:54:31 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 04 12:20:39 2021  
Response via : Initial Calibration

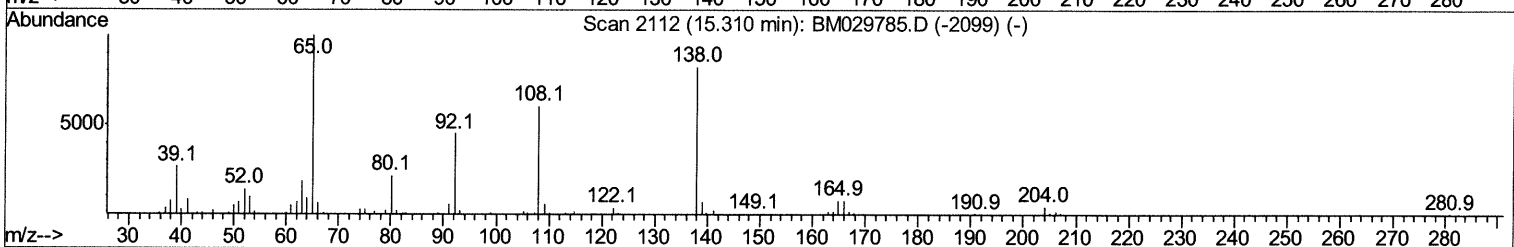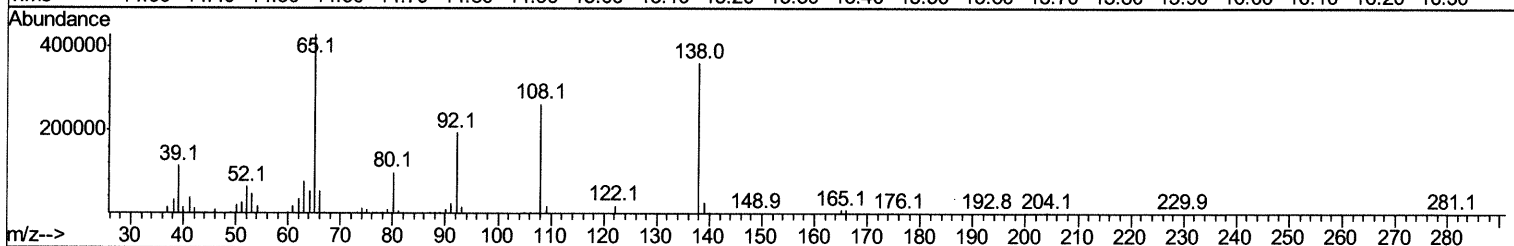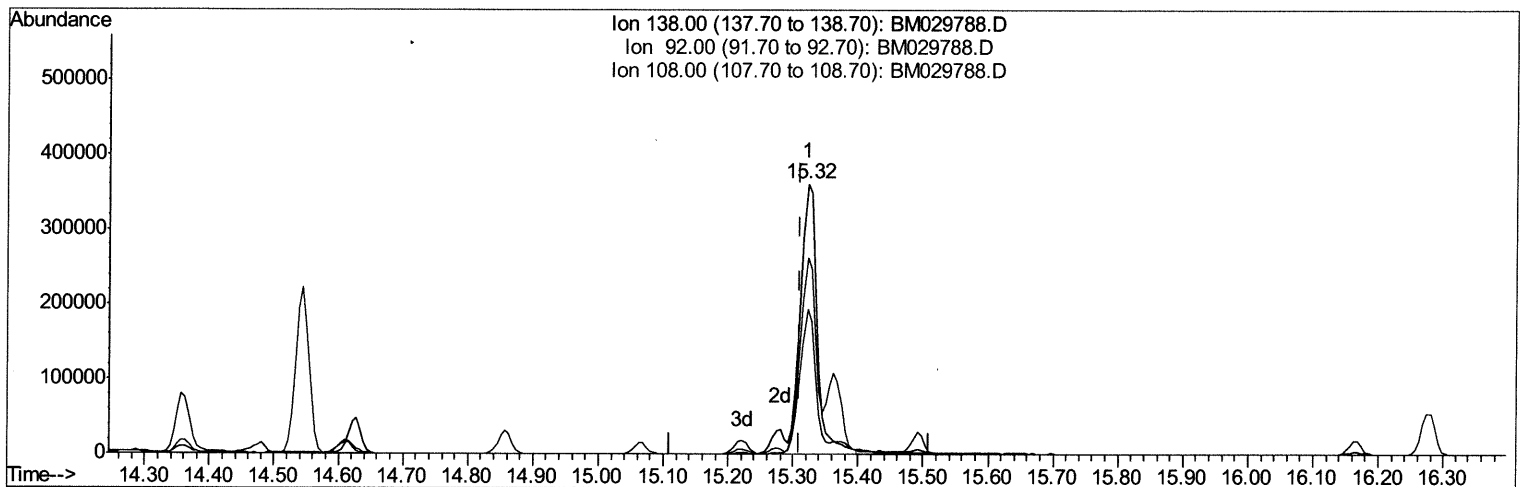

TIC: BM029788.D

(63) 4-Nitroaniline

15.321min (+0.012) 169.84ng/ul m 05/06/2021

response 684505

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 138.00 | 100   | 100   |
| 92.00  | 55.50 | 53.50 |
| 108.00 | 73.10 | 72.74 |
| 0.00   | 0.00  | 0.00  |

## Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\  
Data File : BM029783.D  
Acq On : 04 May 2021 10:22  
Operator : CG/JU  
Sample : SST00516  
Misc :  
ALS Vial : 2 Sample Multiplier: 1




Instrument :  
BNA\_M  
ClientSampleId :  
SSTD160015

Manual Integrations  
APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 14:16:15 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 04 14:13:54 2021  
Response via : Initial Calibration

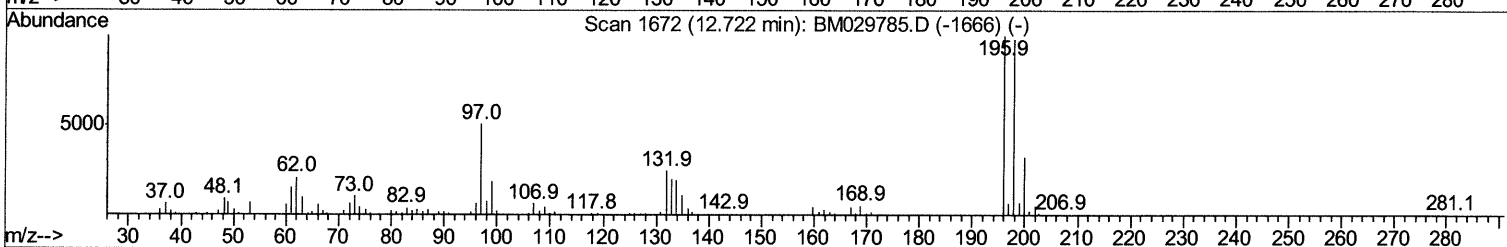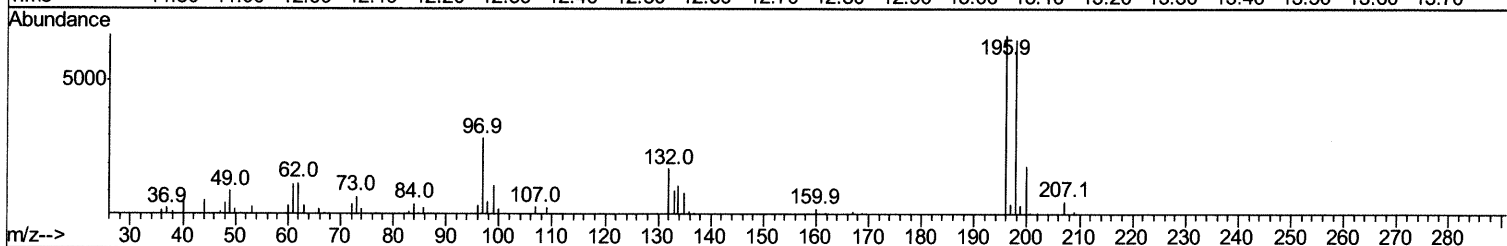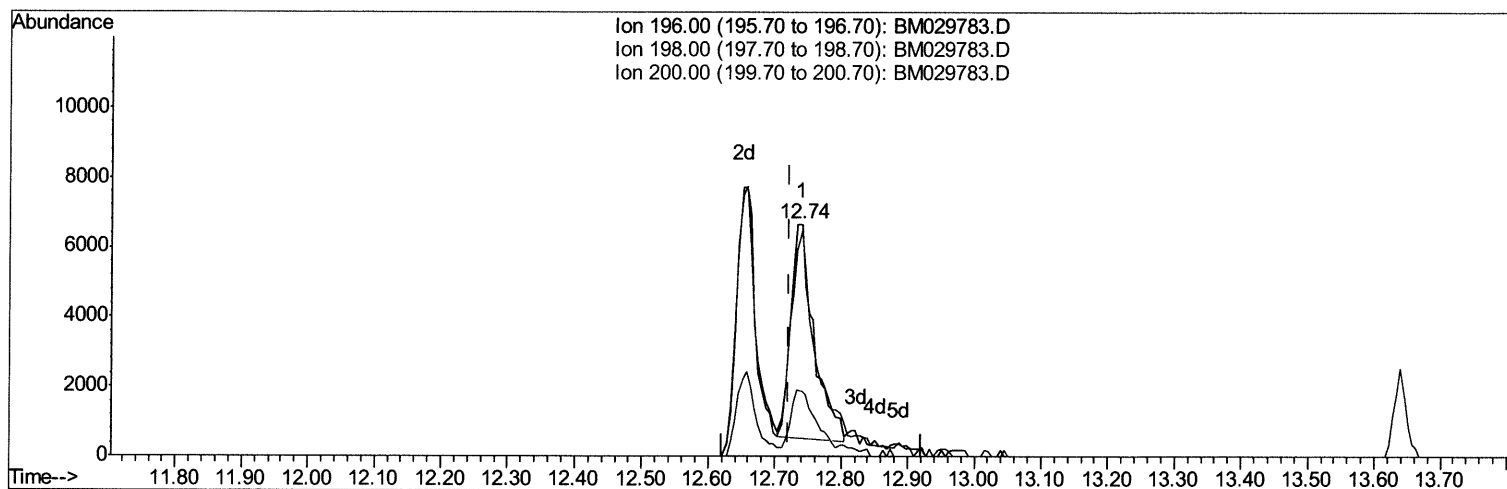

TIC: BM029783.D

(42) 2,4,5-Trichlorophenol

12.739min (+0.018) 3.26ng/ul

response 14853

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 196.00 | 100   | 100   |
| 198.00 | 97.30 | 97.10 |
| 200.00 | 32.60 | 31.08 |
| 0.00   | 0.00  | 0.00  |

# Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\  
 Data File : BM029783.D  
 Acq On : 04 May 2021 10:22  
 Operator : CG/JU  
 Sample : SST00516  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1




Instrument :  
 BNA\_M  
 ClientSampleId :  
 SST0160015

Manual Integrations  
 APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 14:16:15 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue May 04 14:13:54 2021  
 Response via : Initial Calibration

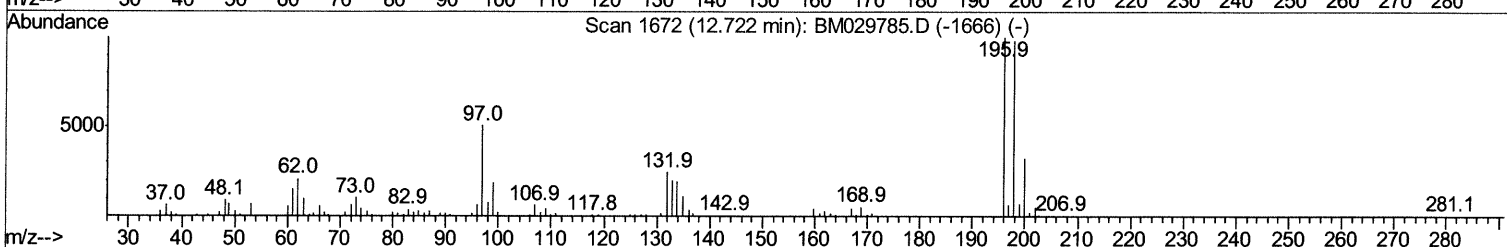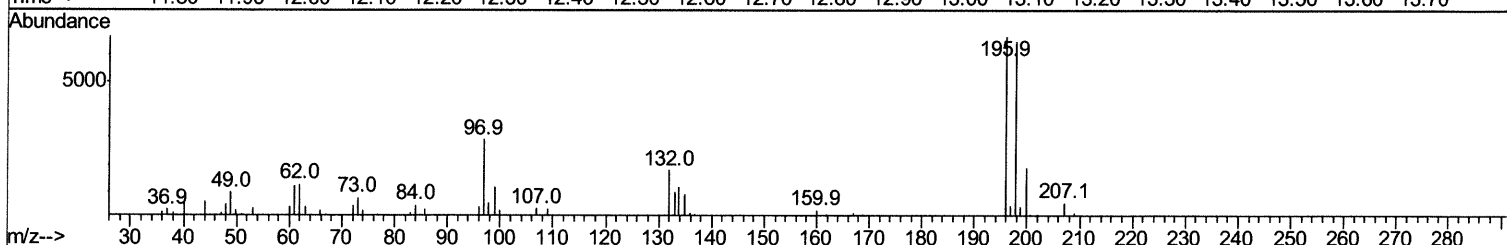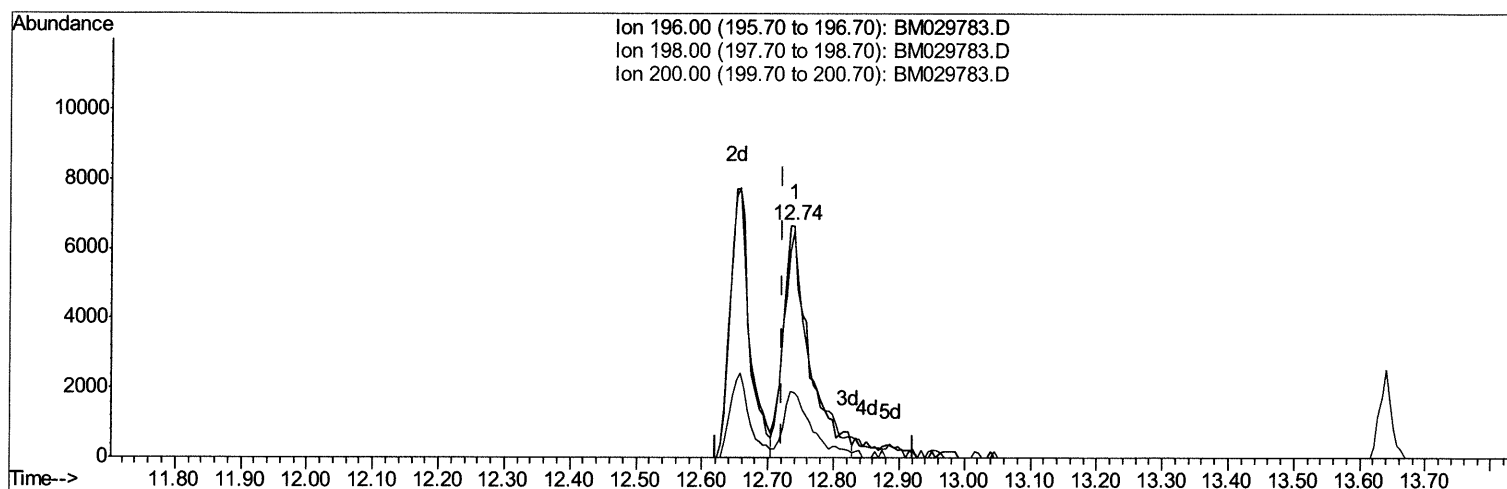

TIC: BM029783.D

(42) 2,4,5-Trichlorophenol

12.739min (+0.018) 4.10ng/ul m 05/06/21 JU

response 18683

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 196.00 | 100   | 100   |
| 198.00 | 97.30 | 97.10 |
| 200.00 | 32.60 | 28.15 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\  
 Data File : BM029788.D  
 Acq On : 04 May 2021 13:24  
 Operator : CG/JU  
 Sample : SSTD16015  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 SSTD160015

Manual Integrations  
 APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 14:03:50 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue May 04 12:20:39 2021  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.57  | 152  | 113194   | 20.00 | ng/ul | 0.00     |
| 20) Naphthalene-d8        | 10.35 | 136  | 462224   | 20.00 | ng/ul | 0.00     |
| 38) Acenaphthene-d10      | 14.22 | 164  | 274836   | 20.00 | ng/ul | 0.00     |
| 64) Phenanthrene-d10      | 16.97 | 188  | 534984   | 20.00 | ng/ul | 0.00     |
| 79) Chrysene-d12          | 21.16 | 240  | 576024   | 20.00 | ng/ul | 0.00     |
| 88) Perylene-d12          | 23.32 | 264  | 606291   | 20.00 | ng/ul | 0.00     |

## System Monitoring Compounds

|                                |       |     |         |        |       |       |
|--------------------------------|-------|-----|---------|--------|-------|-------|
| 3) 1,4-Dioxane-d8              | 0.00  | 96  | 0d      | 0.00   | ng/uL |       |
| 4) Pyridine-d5                 | 3.48  | 84  | 1300947 | 259.47 | ng/ul | -0.02 |
| 7) Phenol-d5                   | 6.76  | 99  | 1681564 | 220.61 | ng/ul | 0.00  |
| 9) Bis-(2-Chloroethyl)ether-d  | 6.92  | 67  | 983349  | 246.33 | ng/ul | 0.00  |
| 11) 2-Chlorophenol-d4          | 0.00  | 132 | 0d      | 0.00   | ng/ul |       |
| 15) 4-Methylphenol-d8          | 8.30  | 113 | 1323410 | 202.72 | ng/ul | 0.01  |
| 21) Nitrobenzene-d5            | 0.00  | 128 | 0d      | 0.00   | ng/ul |       |
| 24) 2-Nitrophenol-d4           | 0.00  | 143 | 0d      | 0.00   | ng/ul |       |
| 28) 2,4-Dichlorophenol-d3      | 0.00  | 165 | 0d      | 0.00   | ng/ul |       |
| 31) 4-Chloroaniline-d4         | 10.50 | 131 | 1769106 | 176.20 | ng/ul | 0.00  |
| 46) Dimethylphthalate-d6       | 0.00  | 166 | 0d      | 0.00   | ng/ul |       |
| 49) Acenaphthylene-d8          | 0.00  | 160 | 0d      | 0.00   | ng/ul |       |
| 54) 4-Nitrophenol-d4           | 14.46 | 143 | 640595  | 222.44 | ng/ul | 0.02  |
| 60) Fluorene-d10               | 0.00  | 176 | 0d      | 0.00   | ng/ul |       |
| 65) 4,6-Dinitro-2-methylphenol | 15.36 | 200 | 666831  | 171.43 | ng/ul | 0.01  |
| 73) Anthracene-d10             | 0.00  | 188 | 0d      | 0.00   | ng/ul |       |
| 81) Pyrene-d10                 | 0.00  | 212 | 0d      | 0.00   | ng/ul |       |
| 92) Benzo(a)pyrene-d12         | 0.00  | 264 | 0d      | 0.00   | ng/ul |       |

## Target Compounds

|                                |       |     |         |               | Ovalue      |
|--------------------------------|-------|-----|---------|---------------|-------------|
| 5) Pyridine                    | 3.50  | 79  | 1346713 | 252.359 ng/ul | 90          |
| 6) Benzaldehyde                | 6.72  | 77  | 603543  | 138.070 ng/ul | 96          |
| 8) Phenol                      | 6.79  | 94  | 1696177 | 224.528 ng/ul | 98          |
| 10) Bis(2-Chloroethyl)ether    | 7.02  | 93  | 1283574 | 222.019 ng/ul | 99          |
| 13) 2-Methylphenol             | 8.02  | 108 | 1260896 | 207.939 ng/ul | 97          |
| 14) 2,2'-oxybis(1-Chloropropan | 8.11  | 45  | 1871314 | 329.742 ng/ul | 100         |
| 16) Acetophenone               | 8.40  | 105 | 2010522 | 199.801 ng/ul | 95          |
| 18) 4-Methylphenol             | 8.37  | 108 | 1344995 | 203.580 ng/ul | 96          |
| 32) 4-Chloroaniline            | 10.52 | 127 | 1816535 | 179.745 ng/ul | 99          |
| 34) Caprolactam                | 11.34 | 113 | 398177m | 173.423 ng/ul | 95/06/21 JU |
| 40) Hexachlorocyclopentadiene  | 12.37 | 237 | 902117  | 171.578 ng/ul | 95          |
| 51) 3-Nitroaniline             | 14.15 | 138 | 736576  | 194.413 ng/ul | 92          |
| 53) 2,4-Dinitrophenol          | 14.36 | 184 | 478399  | 188.545 ng/ul | 88          |
| 55) 4-Nitrophenol              | 14.48 | 109 | 442463  | 217.241 ng/ul | 94          |
| 63) 4-Nitroaniline             | 15.32 | 138 | 684505m | 169.837 ng/ul | 95/06/21 JU |
| 66) 4,6-Dinitro-2-methylphenol | 15.38 | 198 | 645627  | 172.283 ng/ul | 93          |
| 70) Atrazine                   | 16.46 | 200 | 1033373 | 151.811 ng/ul | 99          |
| 71) Pentachlorophenol          | 16.63 | 266 | 730898  | 183.271 ng/ul | 94          |
| 77) Carbazole                  | 17.38 | 167 | 4850051 | 176.254 ng/ul | 99          |
| 84) 3,3'-Dichlorobenzidine     | 21.08 | 252 | 2024463 | 136.929 ng/ul | 99          |
| 89) Di-n-octyl phthalate       | 21.94 | 149 | 7021597 | 201.801 ng/ul | 100         |



Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\  
Data File : BM029788.D  
Acq On : 04 May 2021 13:24  
Operator : CG/JU  
Sample : SSTD16015  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SSTD160015

Manual Integrations  
APPROVED

mohammad

5/5/2021 11:26:32 AM

Quant Time: May 04 14:03:50 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-BM050421.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue May 04 12:20:39 2021  
Response via : Initial Calibration

| Internal Standards | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|--------------------|------|------|----------|------|-------|----------|
|--------------------|------|------|----------|------|-------|----------|

-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed