

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 07:42:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

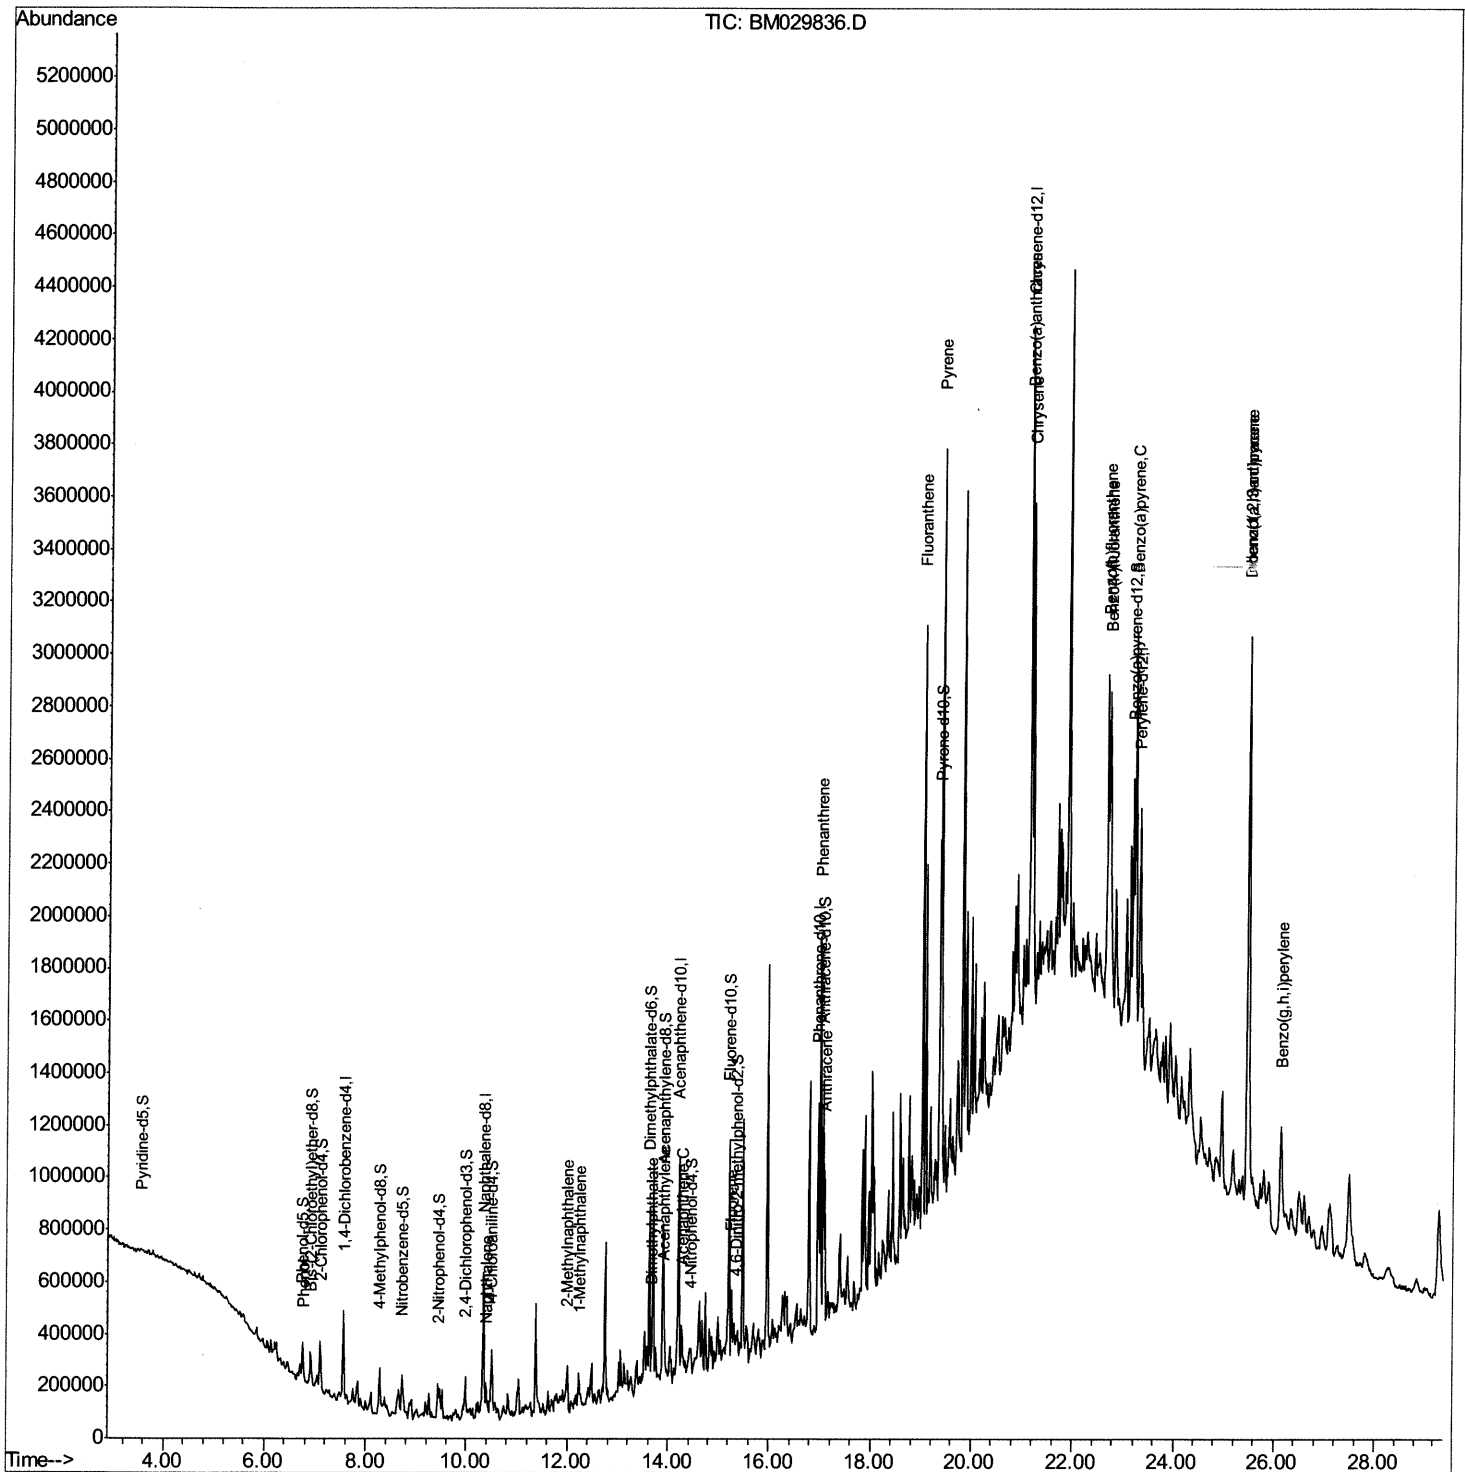

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 02:17:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

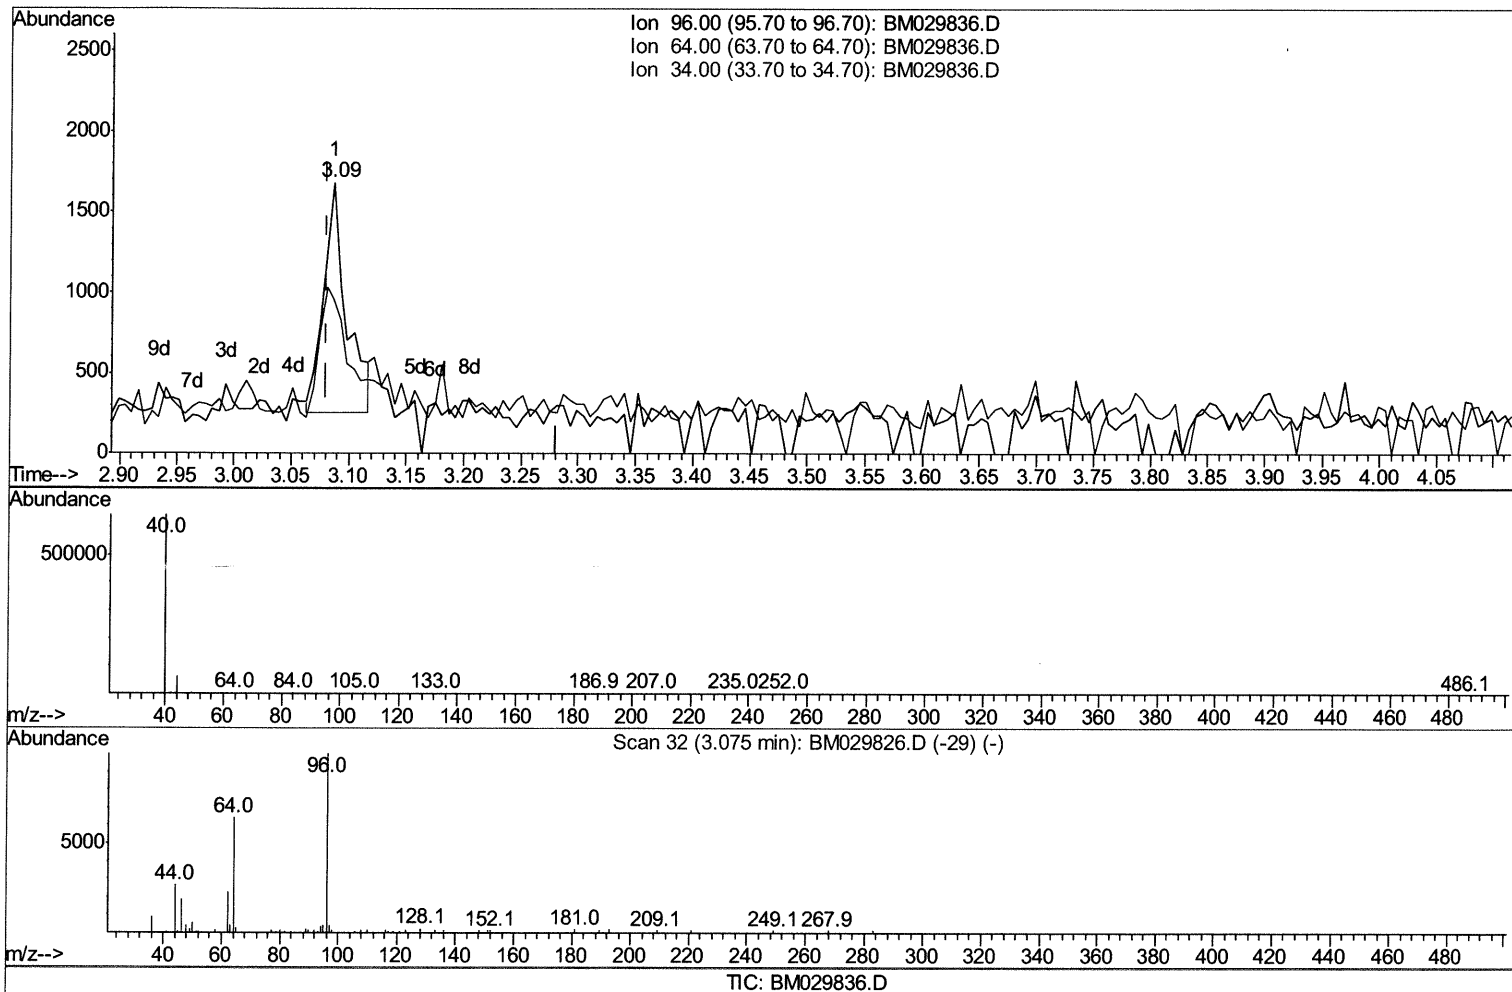

(3) 1,4-Dioxane-d8 (S)

3.087min (+0.006) 0.75ng/uL

response 1978

Ion	Exp%	Act%
96.00	100	100
64.00	70.90	56.94
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
 Data File : BM029836.D
 Acq On : 05 May 2021 20:46
 Operator : CG/JU
 Sample : M2192-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 BG595

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:16 PM

Quant Time: May 06 02:17:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

5/6/2021 4:49:16 PM

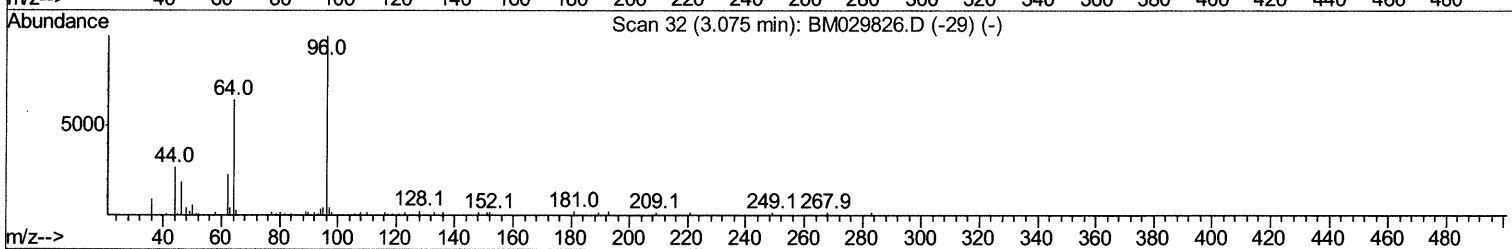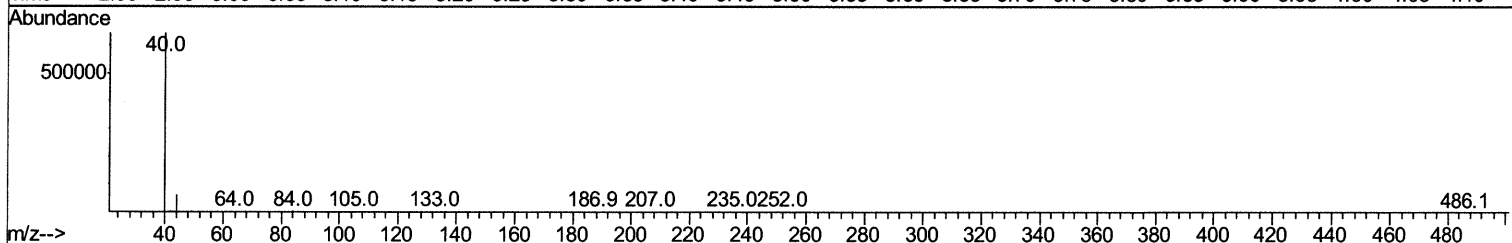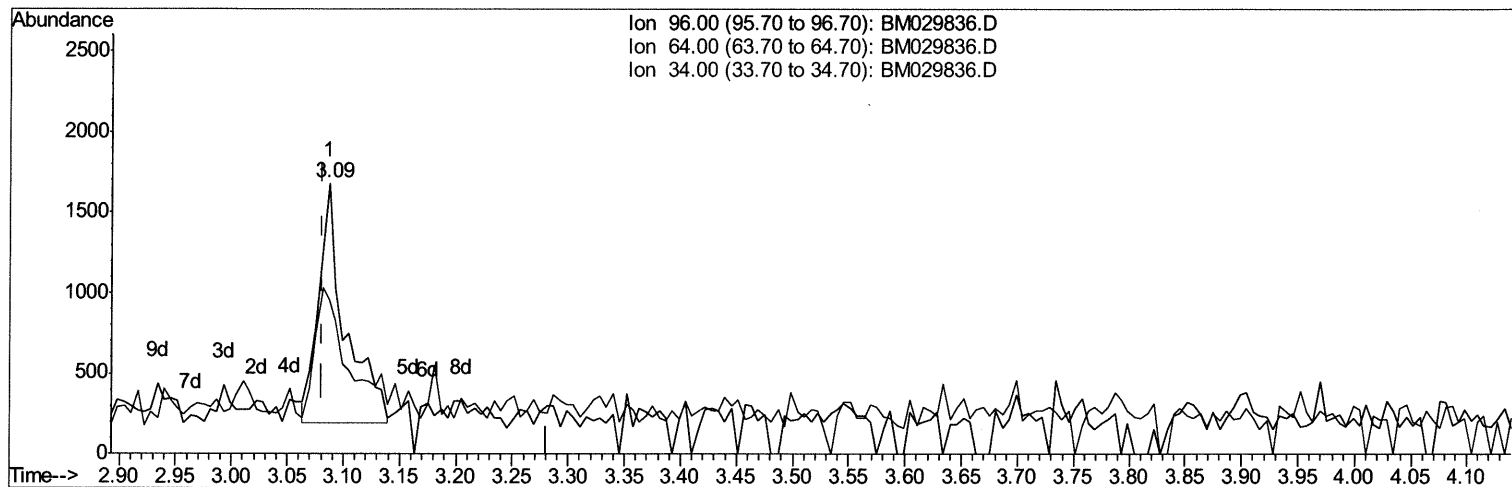

TIC: BM029836.D

(3) 1,4-Dioxane-d8 (S)

3.087min (+0.006) 0.95ng/uL m 05/07/21 JU

response 2484

Ion	Exp%	Act%
96.00	100	100
64.00	70.90	56.94
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 02:19:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

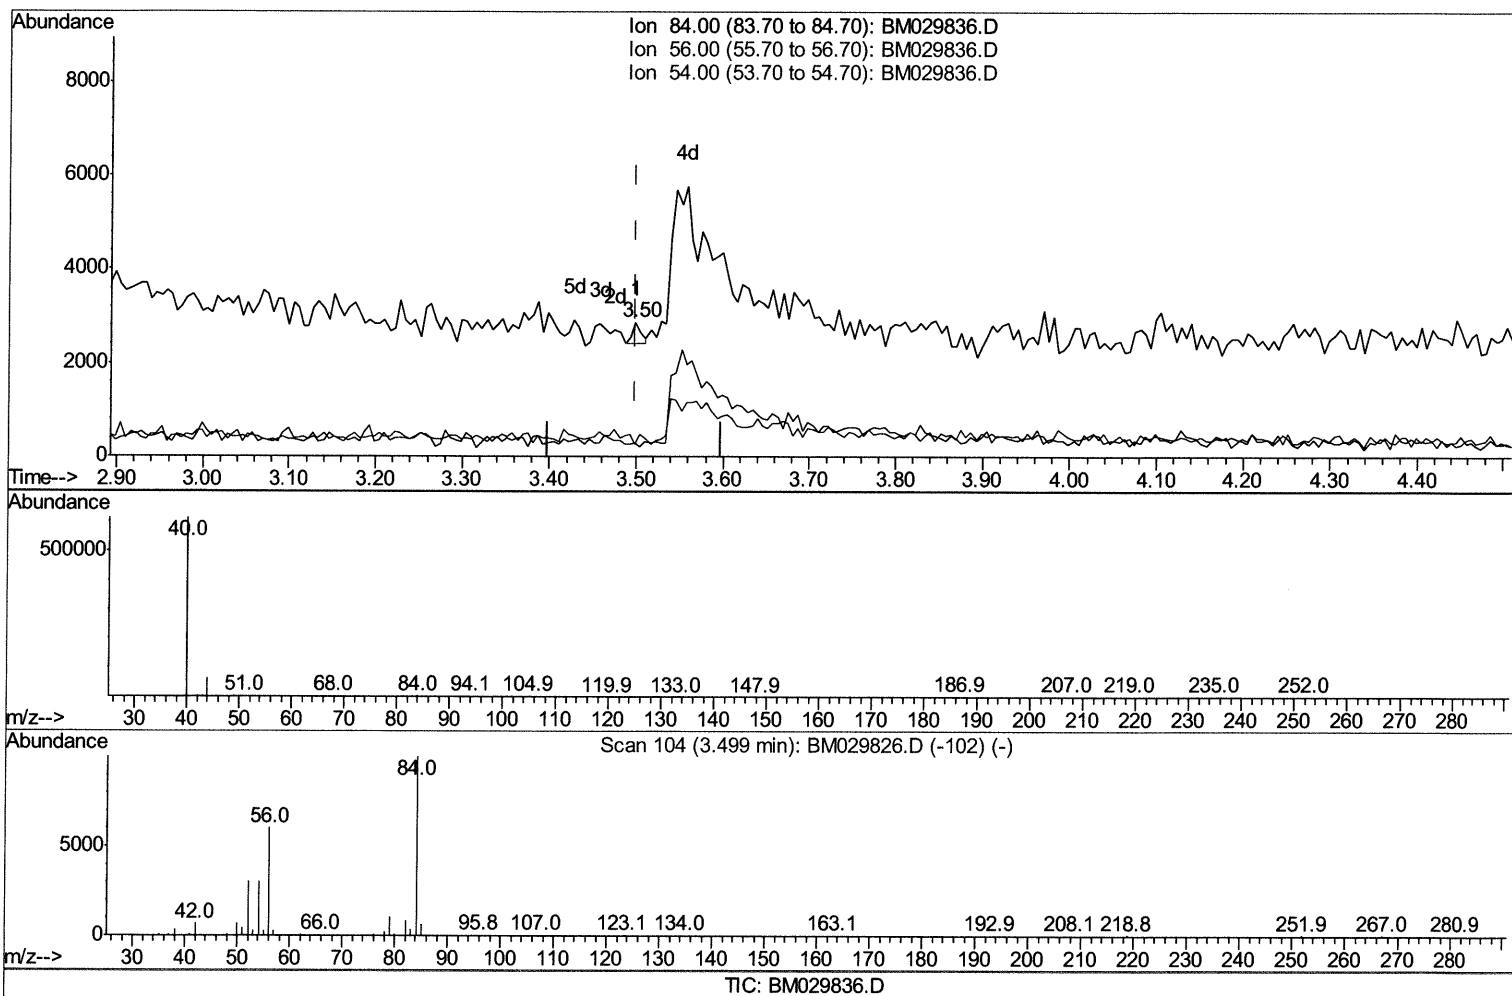

(4) Pyridine-d5 (S)

3.499min (+0.000) 0.06ng/ul

response 346

Ion	Exp%	Act%
84.00	100	100
56.00	66.30	10.10#
54.00	32.40	9.27#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 02:19:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

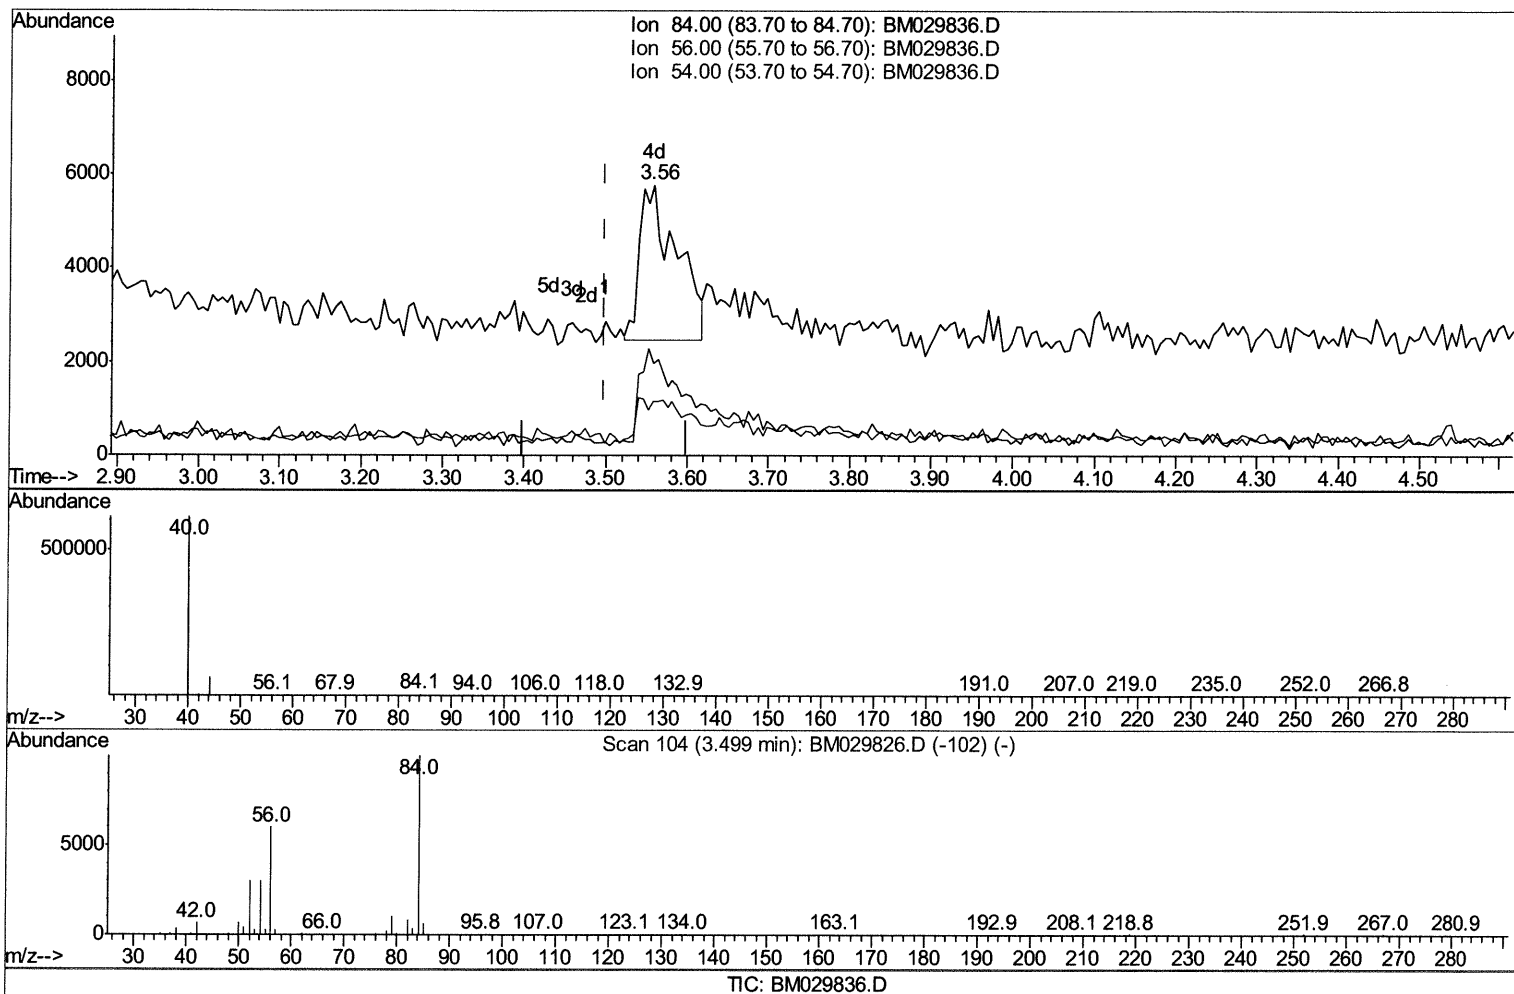

(4) Pyridine-d5 (S)

3.557min (+0.059) 1.73ng/ul m 0.5/0.1/1.0

response 10409

Ion	Exp%	Act%
84.00	100	100
56.00	66.30	34.00#
54.00	32.40	20.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

5/6/2021 4:49:16 PM

Quant Time: Mav 06 02:20:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

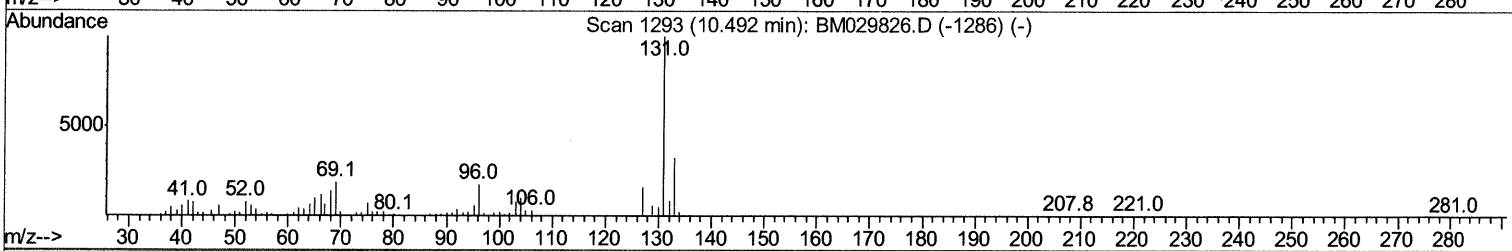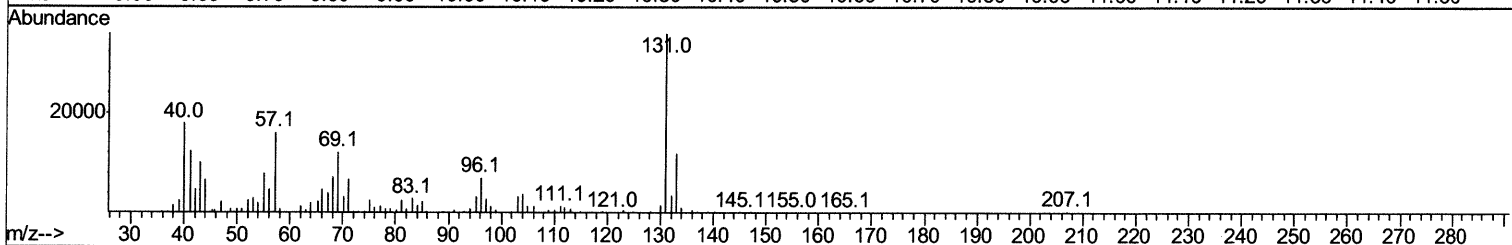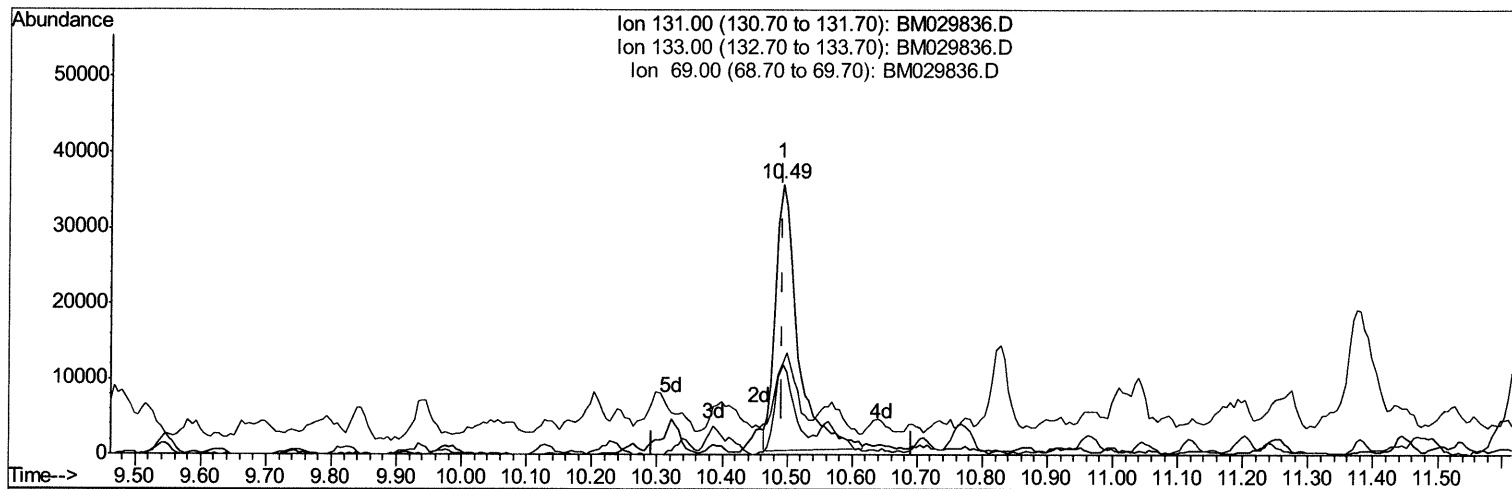

TIC: BM029836.D

(31) 4-Chloroaniline-d4 (S)

10.492min (0.000) 9.77ng/ul

response 84019

Ion	Exp%	Act%
131.00	100	100
133.00	32.00	33.01
69.00	18.30	34.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
 Data File : BM029836.D
 Acq On : 05 May 2021 20:46
 Operator : CG/JU
 Sample : M2192-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1




Instrument :
 BNA_M
ClientSampleId :
 BG595

Manual Integrations
APPROVED

mohammad
 5/6/2021 4:49:16 PM

Quant Time: Mav 06 02:20:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

5/6/2021 4:49:16 PM

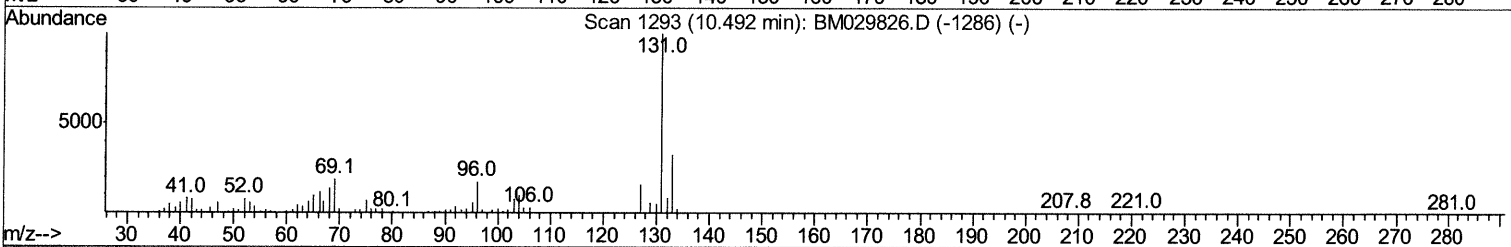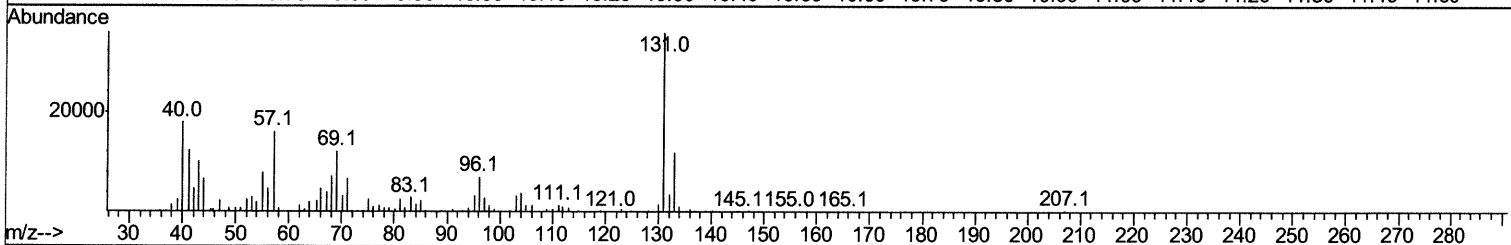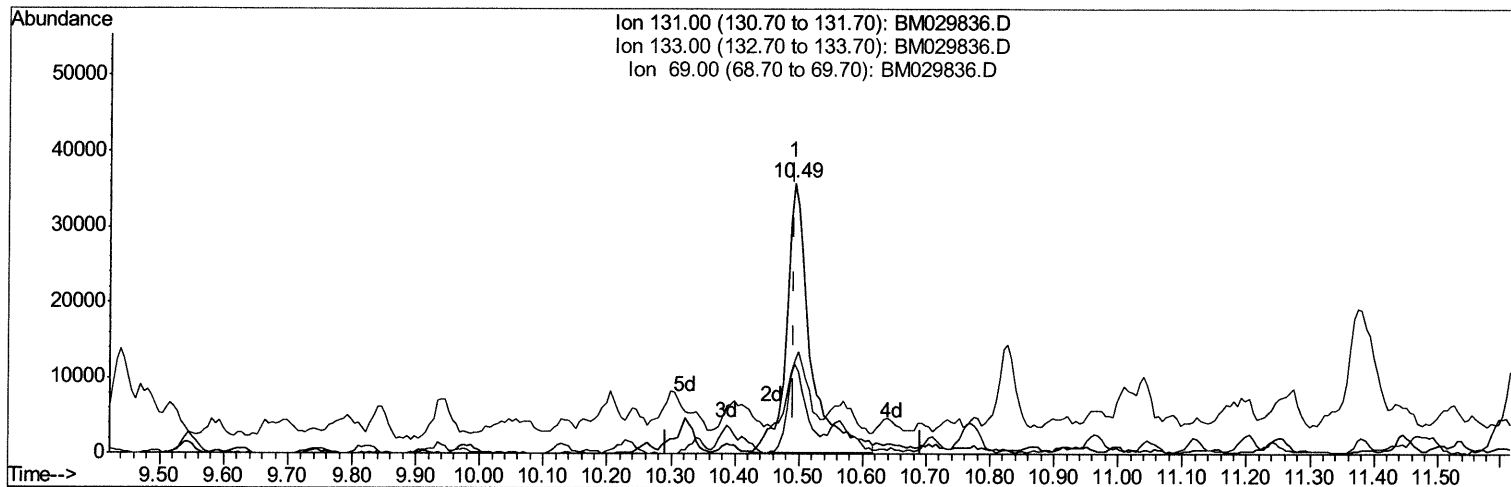

TIC: BM029836.D

(31) 4-Chloroaniline-d4 (S)

10.492min (0.000) 10.78ng/ul m 05/07/21 JU

response 92692

Ion	Exp%	Act%
131.00	100	100
133.00	32.00	33.01
69.00	18.30	34.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 02:24:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

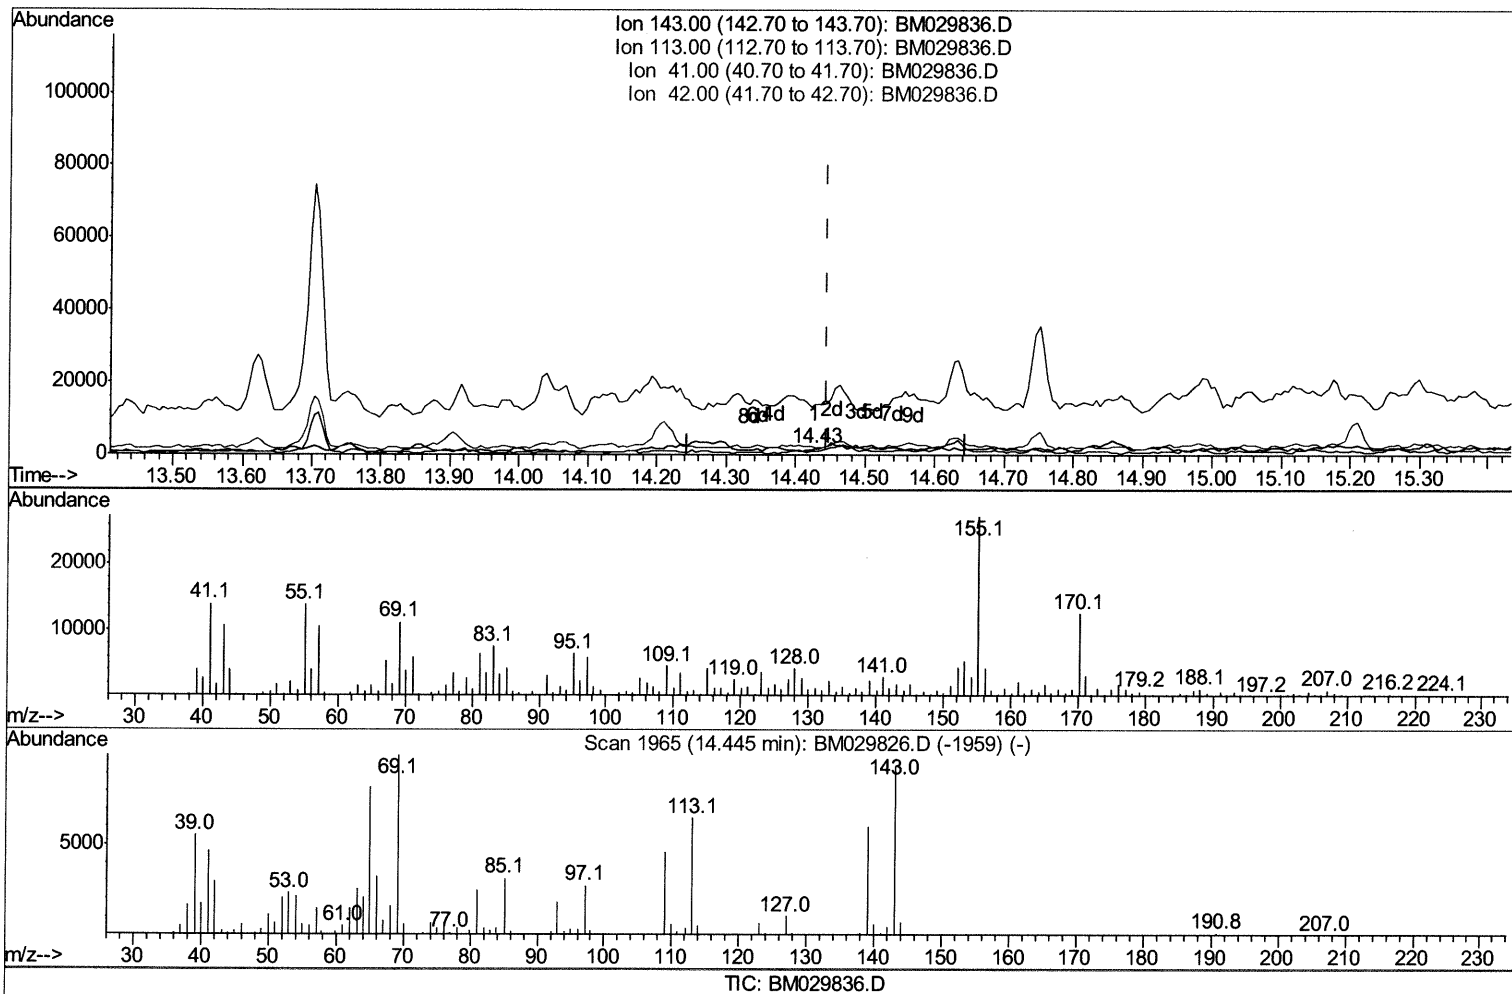

(54) 4-Nitrophenol-d4 (S)

14.427min (-0.018) 0.28ng/ul

response 773

Ion	Exp%	Act%
143.00	100	100
113.00	67.10	51.09#
41.00	45.40	741.50#
42.00	30.10	100.53#

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 02:24:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

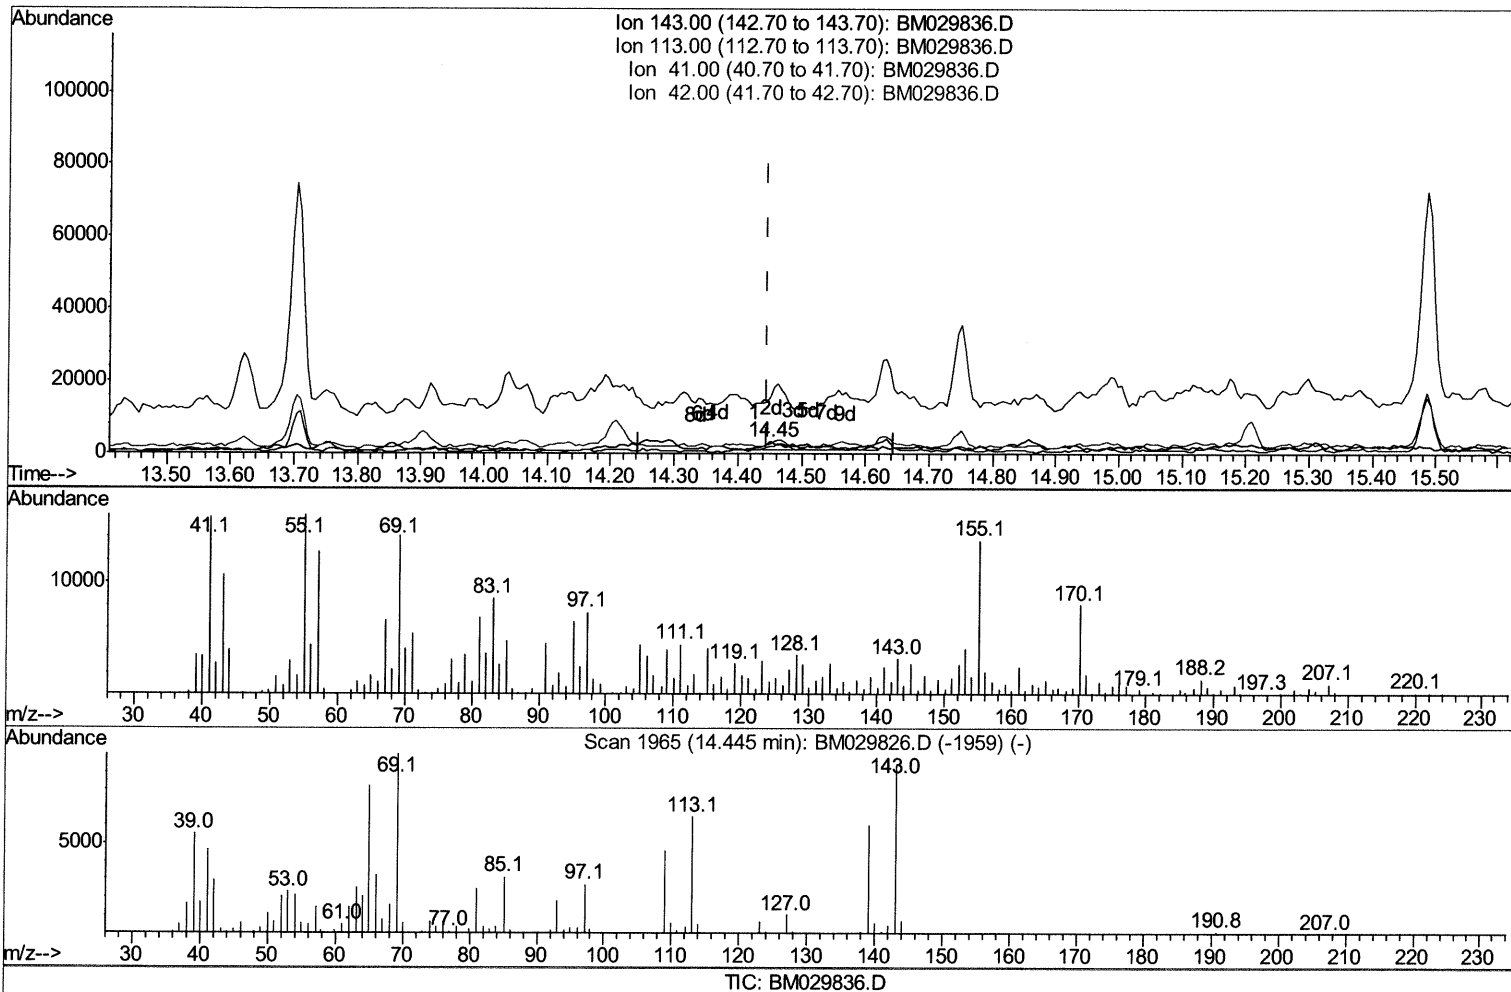

(54) 4-Nitrophenol-d4 (S)

14.451min (+0.006) 5.06ng/ul m 05/07/2021

response 14093

Ion	Exp%	Act%
143.00	100	100
113.00	67.10	59.02
41.00	45.40	483.95#
42.00	30.10	87.83#

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: Mav 06 02:26:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

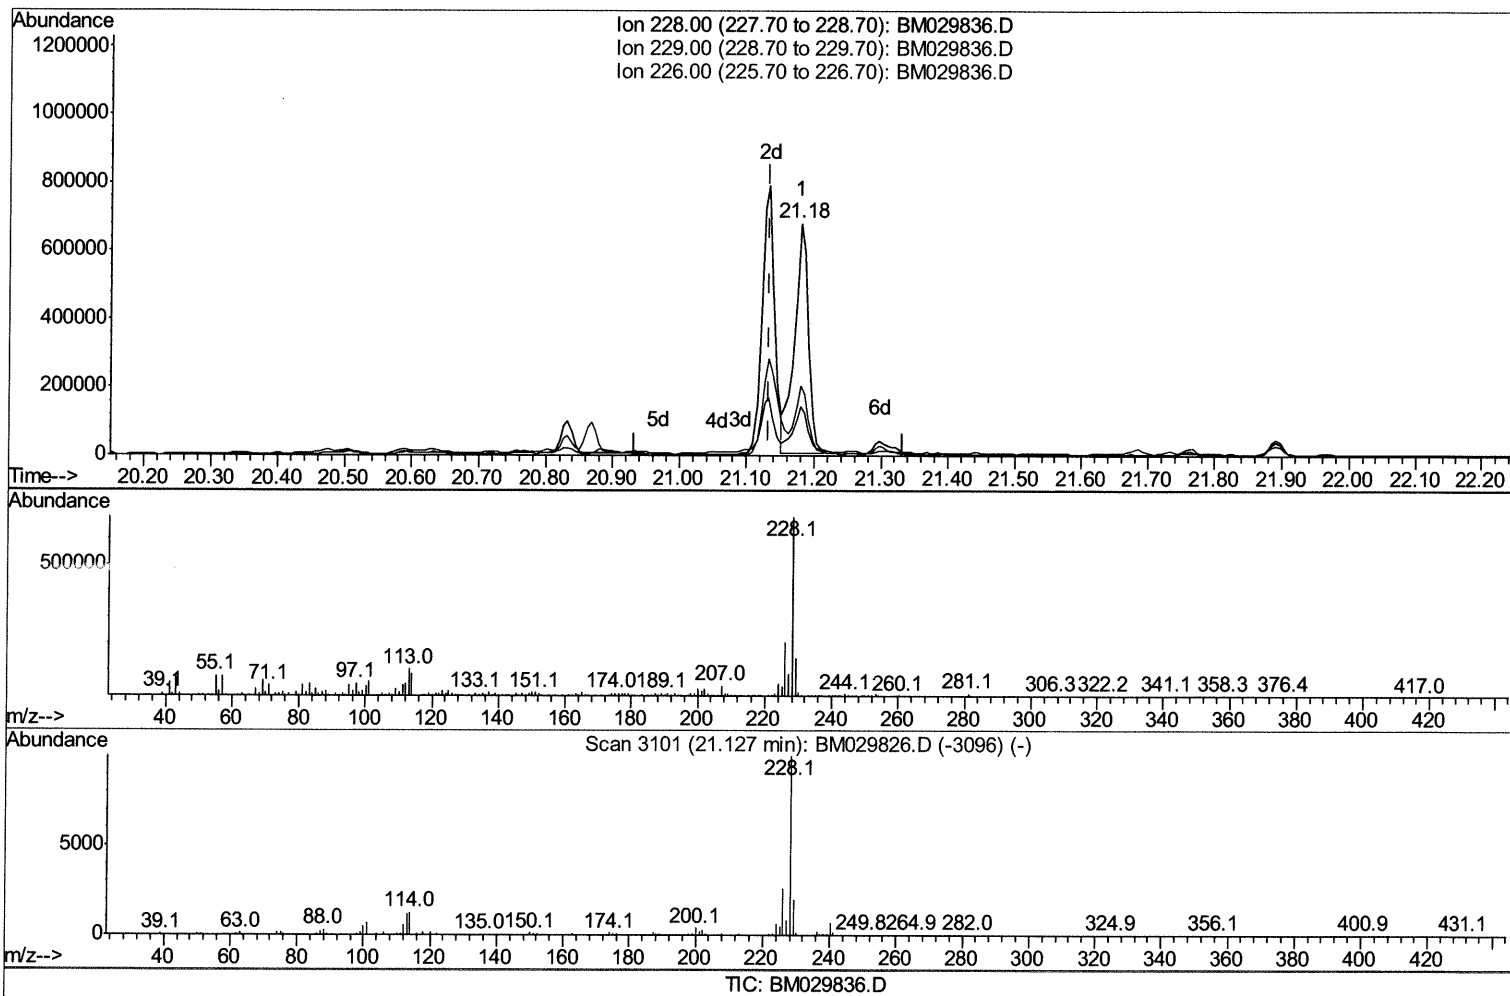

(85) Benzo(a)anthracene

21.180min (+0.047) 28.12ng/ul

response 978305

Ion	Exp%	Act%
228.00	100	100
229.00	19.70	20.99
226.00	26.30	30.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

Quant Time: May 06 02:26:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

5/6/2021 4:49:16 PM

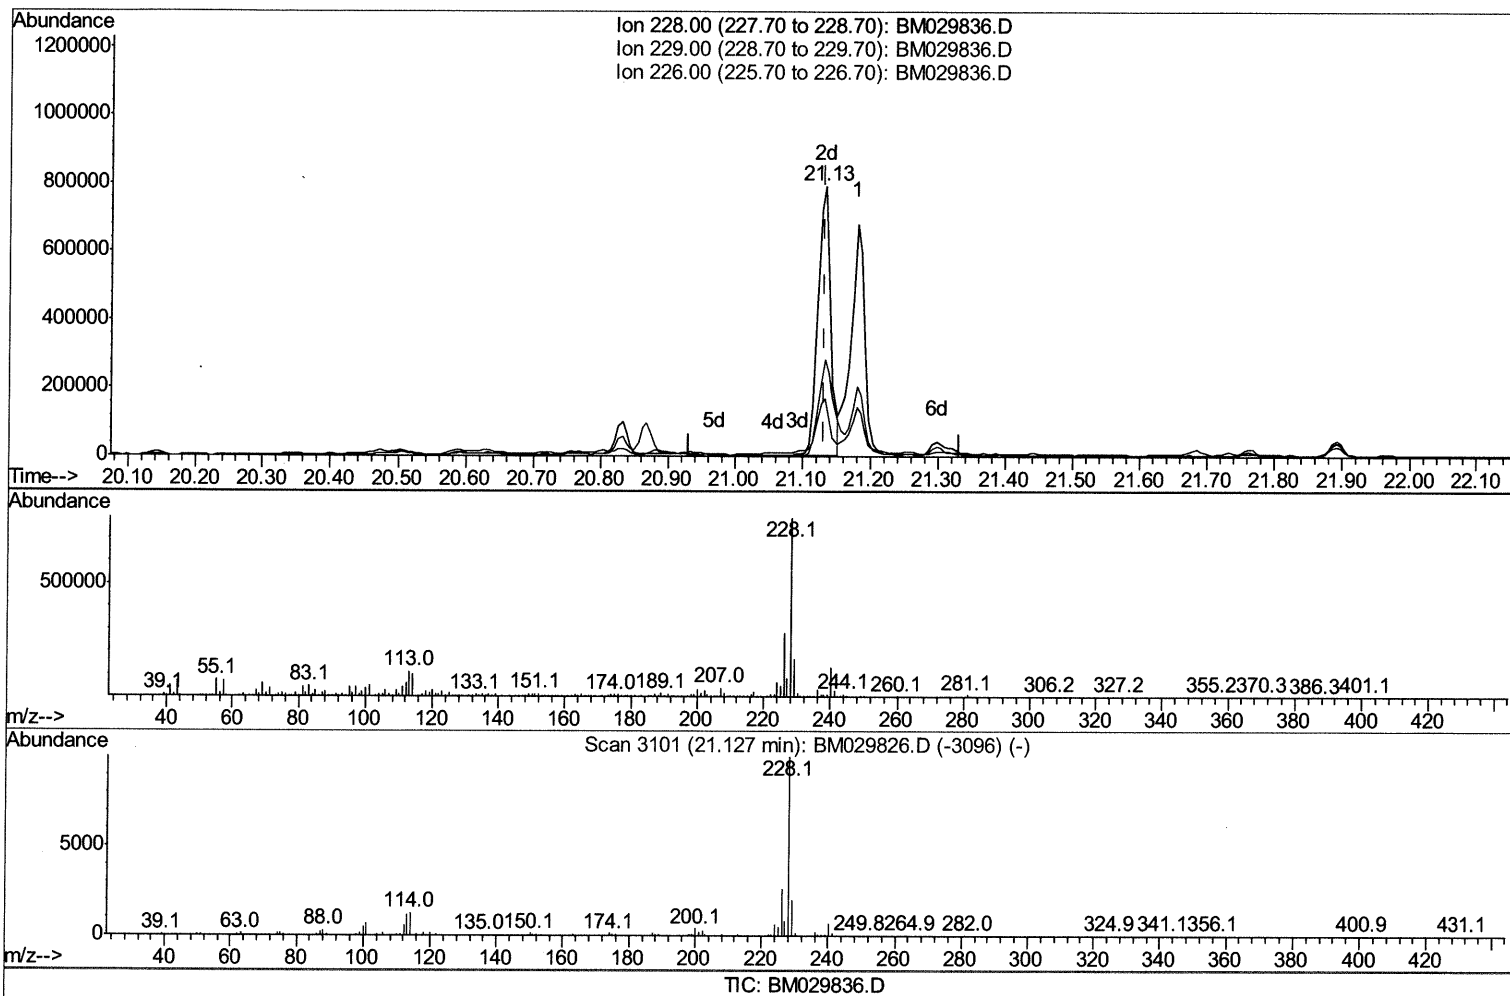

(85) Benzo(a)anthracene

21.133min (0.000) 29.75ng/ul m 05/07/21 JU

response 1035027

Ion	Exp%	Act%
228.00	100	100
229.00	19.70	21.34
226.00	26.30	35.78#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
 Data File : BM029836.D
 Acq On : 05 May 2021 20:46
 Operator : CG/JU
 Sample : M2192-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampleId :
 BG595

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:16 PM

Quant Time: May 06 02:27:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

5/6/2021 4:49:16 PM

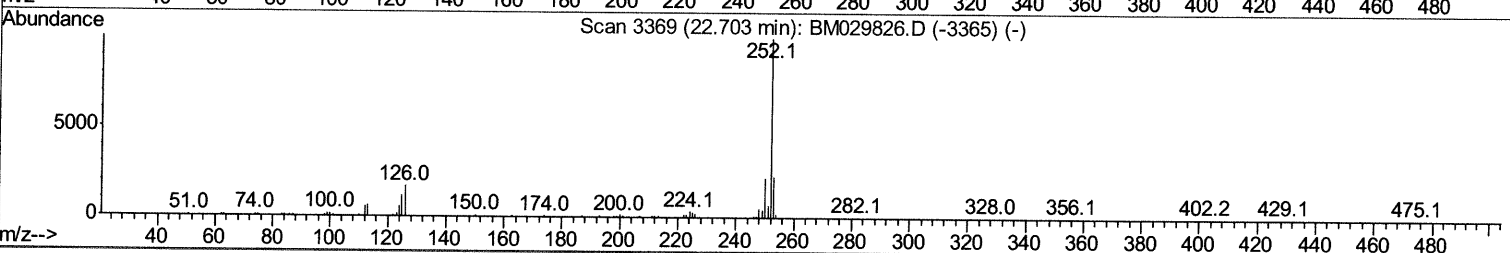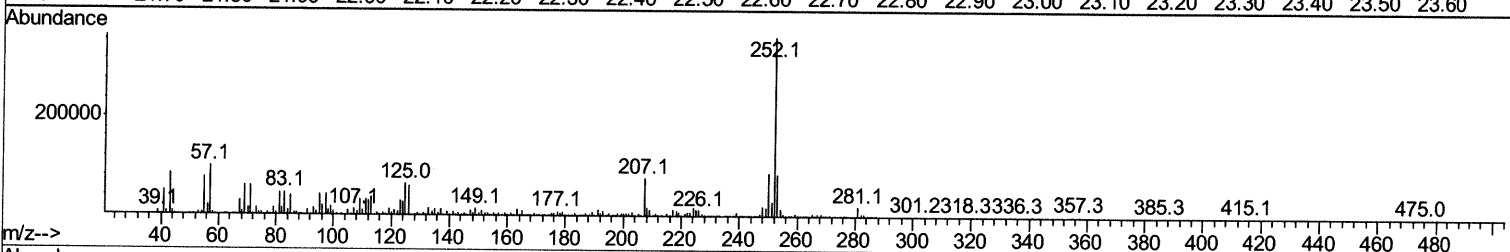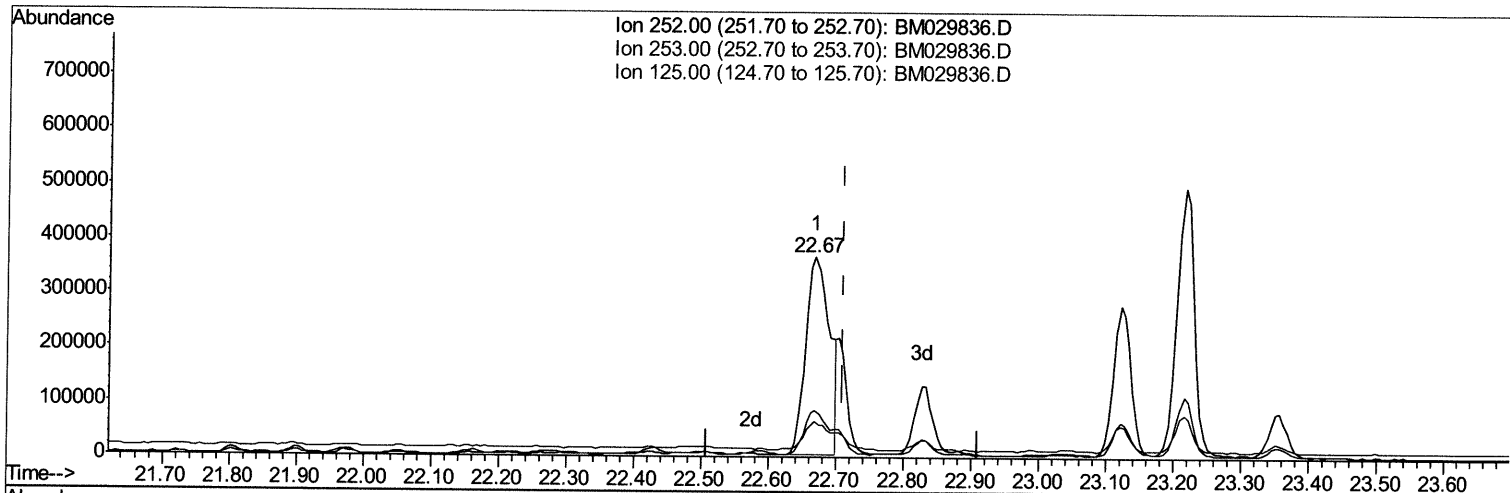

TIC: BM029836.D

(91) Benzo(k)fluoranthene

22.668min (-0.041) 23.57ng/ul

response 892695

Ion Exp% Act%

252.00 100 100

253.00 22.40 23.61

125.00 11.10 17.64#

0.00 0.00 0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
 Data File : BM029836.D
 Acq On : 05 May 2021 20:46
 Operator : CG/JU
 Sample : M2192-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1




Instrument :
 BNA_M
 ClientSampled :
 BG595

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:16 PM

Quant Time: May 06 02:27:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

5/6/2021 4:49:16 PM

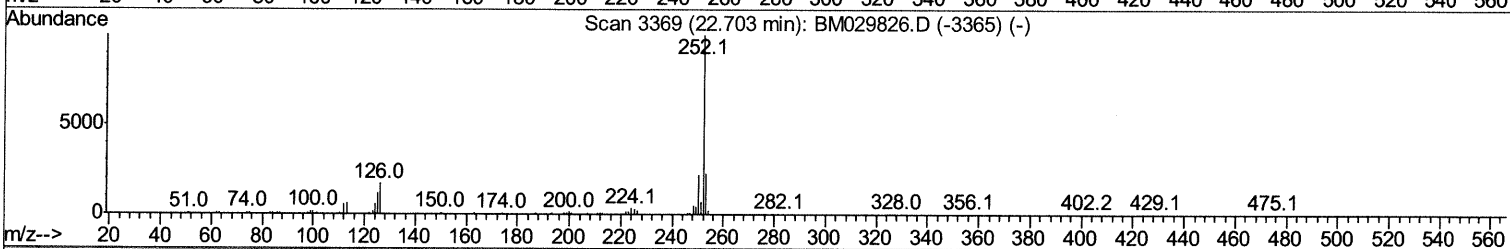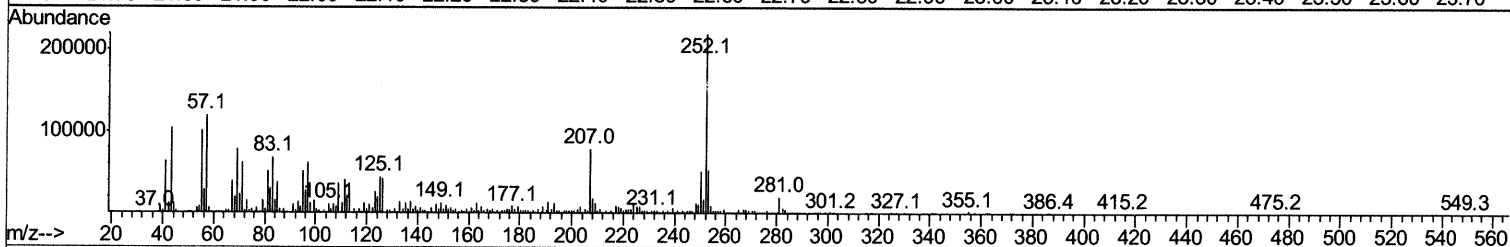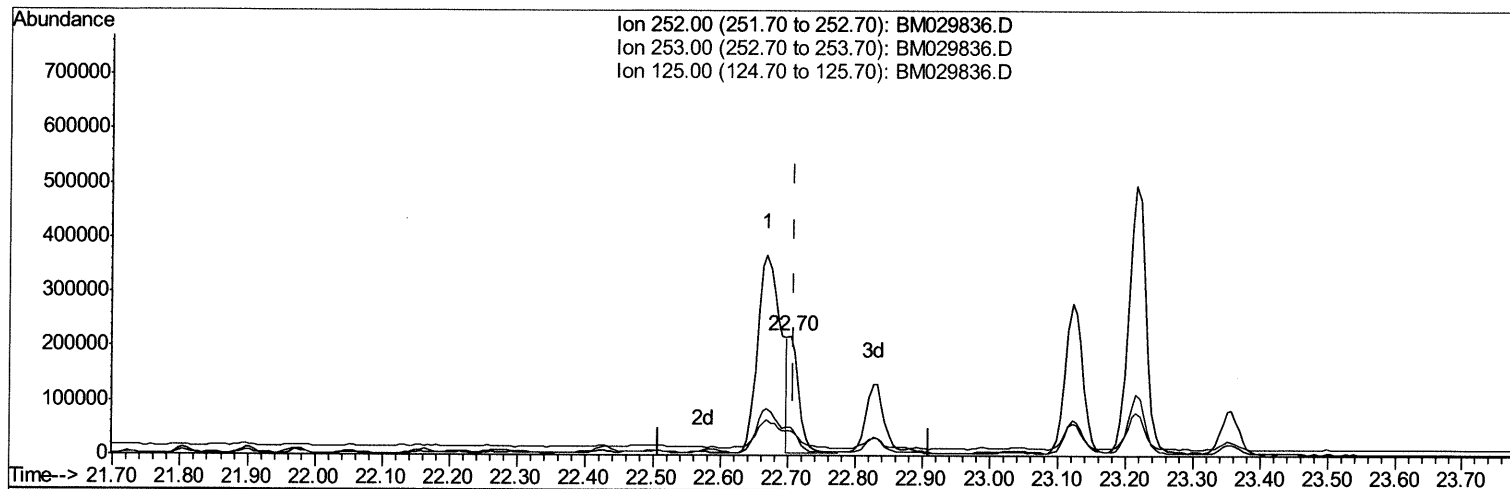

TIC: BM029836.D

(91) Benzo(k)fluoranthene

22.703min (-0.006) 5.84ng/ul m 05/07/21 JU

response 221406

Ion	Exp%	Act%
252.00	100	100
253.00	22.40	23.76
125.00	11.10	20.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
 Data File : BM029836.D
 Acq On : 05 May 2021 20:46
 Operator : CG/JU
 Sample : M2192-01
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG595

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:16 PM

Quant Time: May 06 07:42:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

5/6/2021 4:49:16 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	97118	20.00	ng/ul	0.00
20) Naphthalene-d8	10.34	136	389010	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.21	164	242324	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.96	188	488883	20.00	ng/ul	0.00
79) Chrysene-d12	21.14	240	535814	20.00	ng/ul	0.00
88) Perylene-d12	23.30	264	590186	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.09	96	2484m	0.95	ng/uL	0.00	05/07/21JU
4) Pyridine-d5	3.56	84	10409m	1.73	ng/ul	0.06	
7) Phenol-d5	6.75	99	96840	11.48	ng/ul	0.00	
9) Bis-(2-Chloroethyl)ether-d	6.91	67	71521	13.73	ng/ul	0.00	05/07/21JU
11) 2-Chlorophenol-d4	7.10	132	90304	13.44	ng/ul	0.00	
15) 4-Methylphenol-d8	8.28	113	78000	11.59	ng/ul	0.00	
21) Nitrobenzene-d5	8.72	128	31987	11.07	ng/ul	0.00	05/07/21JU
24) 2-Nitrophenol-d4	9.44	143	31268	9.91	ng/ul	0.00	
28) 2,4-Dichlorophenol-d3	9.98	165	72700	12.32	ng/ul	0.00	
31) 4-Chloroaniline-d4	10.49	131	92692m	10.78	ng/ul	0.00	05/07/21JU
46) Dimethylphthalate-d6	13.63	166	295675	16.34	ng/ul	0.00	
49) Acenaphthylene-d8	13.90	160	400401	16.92	ng/ul	0.00	
54) 4-Nitrophenol-d4	14.45	143	14093m	5.06	ng/ul	0.00	05/07/21JU
60) Fluorene-d10	15.21	176	295275	19.17	ng/ul	0.00	
65) 4,6-Dinitro-2-methylphenol	15.34	200	8466	2.58	ng/ul	0.00	
73) Anthracene-d10	17.06	188	459566	19.01	ng/ul	0.00	05/07/21JU
81) Pyrene-d10	19.36	212	539804	19.64	ng/ul	0.00	
92) Benzo(a)pyrene-d12	23.17	264	625596	18.88	ng/ul	0.00	

Target Compounds

					Ovalue	
8) Phenol	6.78	94	8760	1.021	ng/ul#	84
30) Naphthalene	10.39	128	83774	3.915	ng/ul	98
36) 2-Methylnaphthalene	12.01	142	25922	1.777	ng/ul	98
37) 1-Methylnaphthalene	12.23	142	45732	3.143	ng/ul#	94
47) Dimethylphthalate	13.67	163	36306	2.010	ng/ul	99
50) Acenaphthylene	13.93	152	107602	4.664	ng/ul#	94
52) Acenaphthene	14.27	153	66419	4.076	ng/ul	95
61) Fluorene	15.26	166	80650	4.389	ng/ul	95
72) Phenanthrene	17.00	178	827600	28.532	ng/ul	99
74) Anthracene	17.09	178	333566	11.294	ng/ul	98
80) Fluoranthene	19.02	202	1171395	35.105	ng/ul	96
82) Pyrene	19.39	202	1554153	43.750	ng/ul	97
85) Benzo(a)anthracene	21.13	228	1035027m	29.746	ng/ul	05/07/21JU
87) Chrysene	21.18	228	979282	27.813	ng/ul	98
90) Benzo(b)fluoranthene	22.67	252	892695	23.127	ng/ul#	92
91) Benzo(k)fluoranthene	22.70	252	221406m	5.845	ng/ul	05/07/21JU
93) Benzo(a)pyrene	23.21	252	877262	25.375	ng/ul#	95
94) Indeno(1,2,3-cd)pyrene	25.47	276	396123	8.631	ng/ul	96
95) Dibenzo(a,h)anthracene	25.47	278	127853	3.333	ng/ul#	82
96) Benzo(a,h,i)perylene	26.13	276	395683	10.333	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050421\
Data File : BM029836.D
Acq On : 05 May 2021 20:46
Operator : CG/JU
Sample : M2192-01
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG595

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:16 PM

5/6/2021 4:49:16 PM

Quant Time: May 06 07:42:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)

(#) = qualifier out of range (m) = manual integration (+) = signals summed						