

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029845.D
 Acq On : 06 May 2021 02:55
 Operator : CG/JU
 Sample : M2161-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ3

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:44 PM

Quant Time: May 06 04:13:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 06 03:37:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	87912	20.00	ng/ul	0.00
20) Naphthalene-d8	10.34	136	353702	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.21	164	214662	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.96	188	436573	20.00	ng/ul	0.00
79) Chrysene-d12	21.14	240	500496	20.00	ng/ul	-0.01
88) Perylene-d12	23.30	264	561093	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.07	96	2796	1.18	ng/uL	-0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.76	99	39571	5.18	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.91	67	166249	35.26	ng/ul	0.00
11) 2-Chlorophenol-d4	7.10	132	154315	25.38	ng/ul	-0.01
15) 4-Methylphenol-d8	8.28	113	76906	12.62	ng/ul	0.00
21) Nitrobenzene-d5	8.72	128	99459	37.84	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.43	143	77978	27.17	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	137772	25.68	ng/ul	0.00
31) 4-Chloroaniline-d4	10.51	131	6430m	0.82	ng/ul	0.02
46) Dimethylphthalate-d6	13.63	166	592356	36.94	ng/ul	0.00
49) Acenaphthylene-d8	13.90	160	880420	41.99	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.47	143	3759m	1.52	ng/ul	0.02
60) Fluorene-d10	15.21	176	610179	44.73	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	49462	16.88	ng/ul	0.00
73) Anthracene-d10	17.06	188	1039293	48.13	ng/ul	0.00
81) Pyrene-d10	19.35	212	1183058	46.07	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.17	264	1417251	44.98	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.67	163	25905	1.619	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029845.D
Acq On : 06 May 2021 02:55
Operator : CG/JU
Sample : M2161-03
Misc :
ALS Vial : 64 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AQ3

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:44 PM

Quant Time: May 06 04:13:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 06 03:37:00 2021
Response via : Initial Calibration

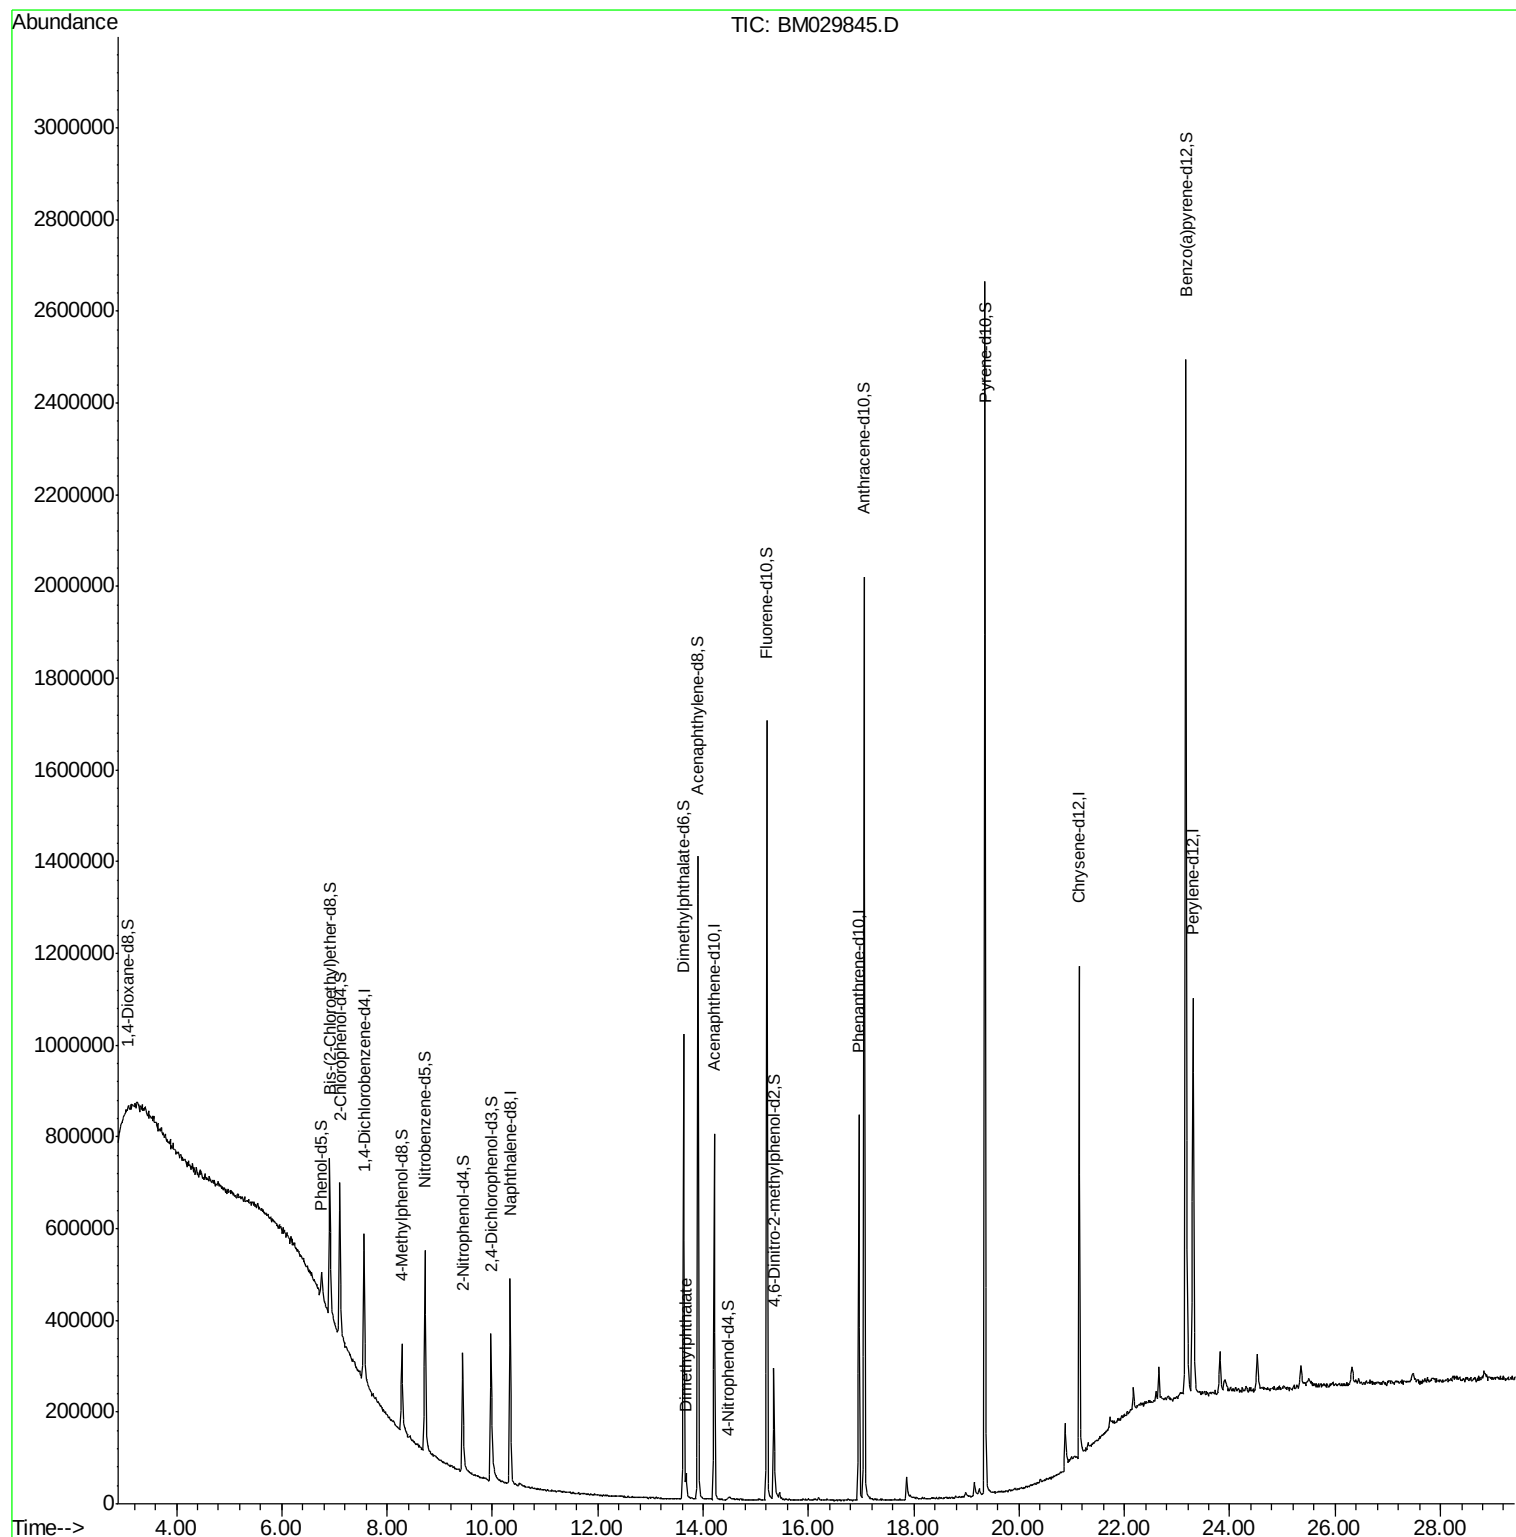

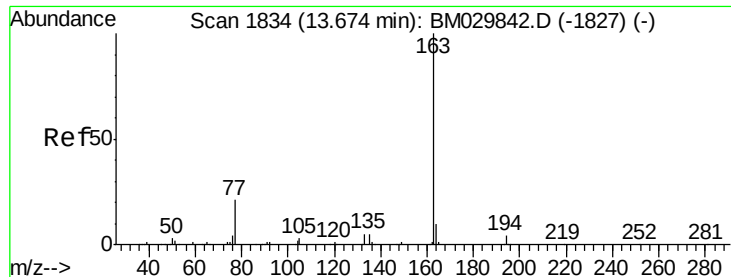

#47
 Dimethylphthalate
 Concen: 1.619 ng/ul
 RT: 13.67 min Scan# 1834
 Delta R.T. -0.01 min
 Lab File: BM029845.D
 Acq: 06 May 2021 02:55

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ3

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.4	3.4	5.0
164	10.3	7.9	11.9

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:44 PM

