

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029846.D
 Acq On : 06 May 2021 03:31
 Operator : CG/JU
 Sample : M2161-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ1

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:46 PM

Quant Time: May 06 04:20:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	89271	20.00	ng/ul	0.00
20) Naphthalene-d8	10.34	136	329713	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.21	164	187207	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.96	188	369726	20.00	ng/ul	0.00
79) Chrysene-d12	21.14	240	458697	20.00	ng/ul	0.00
88) Perylene-d12	23.30	264	546727	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	2590	1.07	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.75	99	23851	3.08	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.91	67	114002	23.81	ng/ul	0.00
11) 2-Chlorophenol-d4	7.10	132	100505	16.28	ng/ul	-0.01
15) 4-Methylphenol-d8	8.28	113	45110	7.29	ng/ul	0.00
21) Nitrobenzene-d5	8.72	128	65942	26.92	ng/ul	0.00
24) 2-Nitrophenol-d4	9.44	143	49336	18.44	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	84229	16.84	ng/ul	0.00
31) 4-Chloroaniline-d4	10.52	131	3393m	0.47	ng/ul	0.03
46) Dimethylphthalate-d6	13.63	166	376366	26.92	ng/ul	0.00
49) Acenaphthylene-d8	13.90	160	562793	30.78	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.49	143	2667m	1.24	ng/ul	0.05
60) Fluorene-d10	15.21	176	400391	33.65	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	29261	11.79	ng/ul	0.00
73) Anthracene-d10	17.06	188	707247	38.68	ng/ul	0.00
81) Pyrene-d10	19.35	212	851512	36.18	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.16	264	1086260	35.38	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	13.68	163	20359	1.459	ng/ul#	Ovalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029846.D
Acq On : 06 May 2021 03:31
Operator : CG/JU
Sample : M2161-01
Misc :
ALS Vial : 65 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AQ1

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:46 PM

Quant Time: May 06 04:20:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

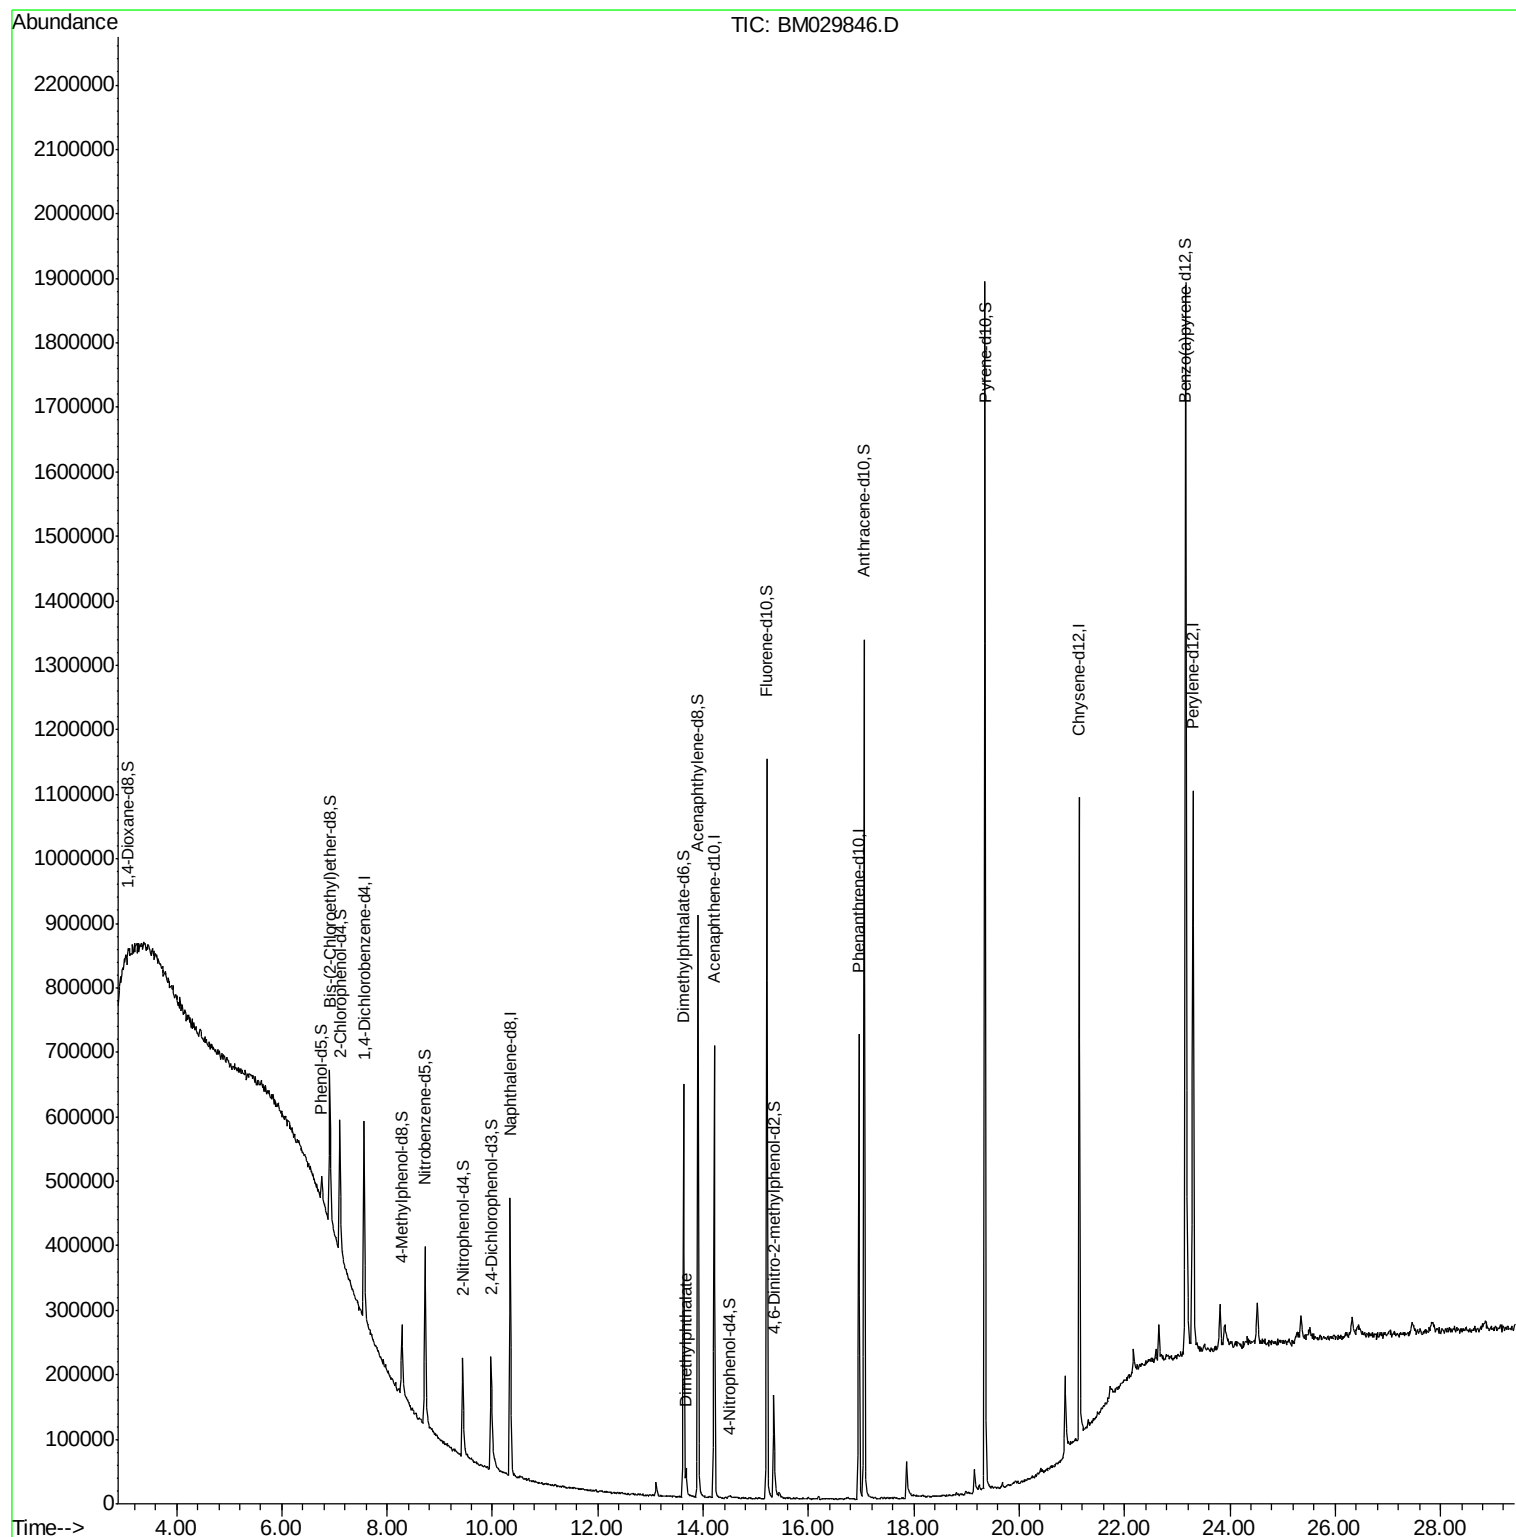

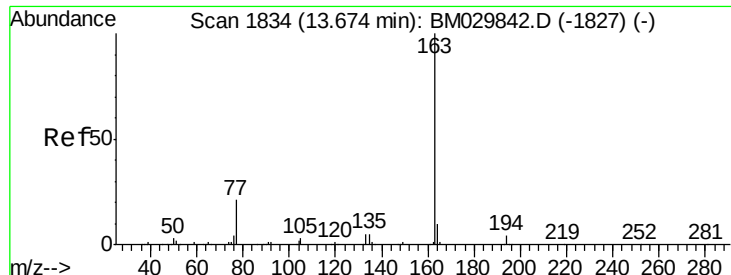

#47
 Dimethylphthalate
 Concen: 1.459 ng/ul
 RT: 13.68 min Scan# 1835
 Delta R.T. -0.01 min
 Lab File: BM029846.D
 Acq: 06 May 2021 03:31

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ1

Tot Ion	Ratio	Lower	Upper
163	100		
194	5.5	3.4	5.0#
164	12.4	7.9	11.9#

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:46 PM

