

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029848.D
 Acq On : 06 May 2021 04:43
 Operator : CG/JU
 Sample : M2161-02
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ2

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:52 PM

Quant Time: May 06 06:48:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	118725	20.00	ng/ul	0.00
20) Naphthalene-d8	10.33	136	476818	20.00	ng/ul	-0.01
38) Acenaphthene-d10	14.21	164	291649	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.96	188	602448	20.00	ng/ul	0.00
79) Chrysene-d12	21.14	240	696587	20.00	ng/ul	0.00
88) Perylene-d12	23.30	264	797445	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	2842m	0.89	ng/uL	-0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.75	99	37734	3.66	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.91	67	167963	26.38	ng/ul	0.00
11) 2-Chlorophenol-d4	7.10	132	154076	18.76	ng/ul	-0.01
15) 4-Methylphenol-d8	8.28	113	71613	8.70	ng/ul	0.00
21) Nitrobenzene-d5	8.72	128	109047	30.78	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.43	143	82496	21.33	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	144653	20.00	ng/ul	0.00
31) 4-Chloroaniline-d4	10.52	131	4252m	0.40	ng/ul	0.03
46) Dimethylphthalate-d6	13.63	166	610874	28.04	ng/ul	0.00
49) Acenaphthylene-d8	13.90	160	936034	32.86	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.47	143	5545m	1.65	ng/ul	0.03
60) Fluorene-d10	15.21	176	669297	36.11	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	62513	15.46	ng/ul	0.00
73) Anthracene-d10	17.06	188	1127974	37.86	ng/ul	0.00
81) Pyrene-d10	19.35	212	1403197	39.26	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.17	264	1654120	36.94	ng/ul	0.00

Target Compounds					Ovalue	
47) Dimethylphthalate	13.67	163	36818	1.694	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029848.D
Acq On : 06 May 2021 04:43
Operator : CG/JU
Sample : M2161-02
Misc :
ALS Vial : 67 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AQ2

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:52 PM

Quant Time: May 06 06:48:23 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

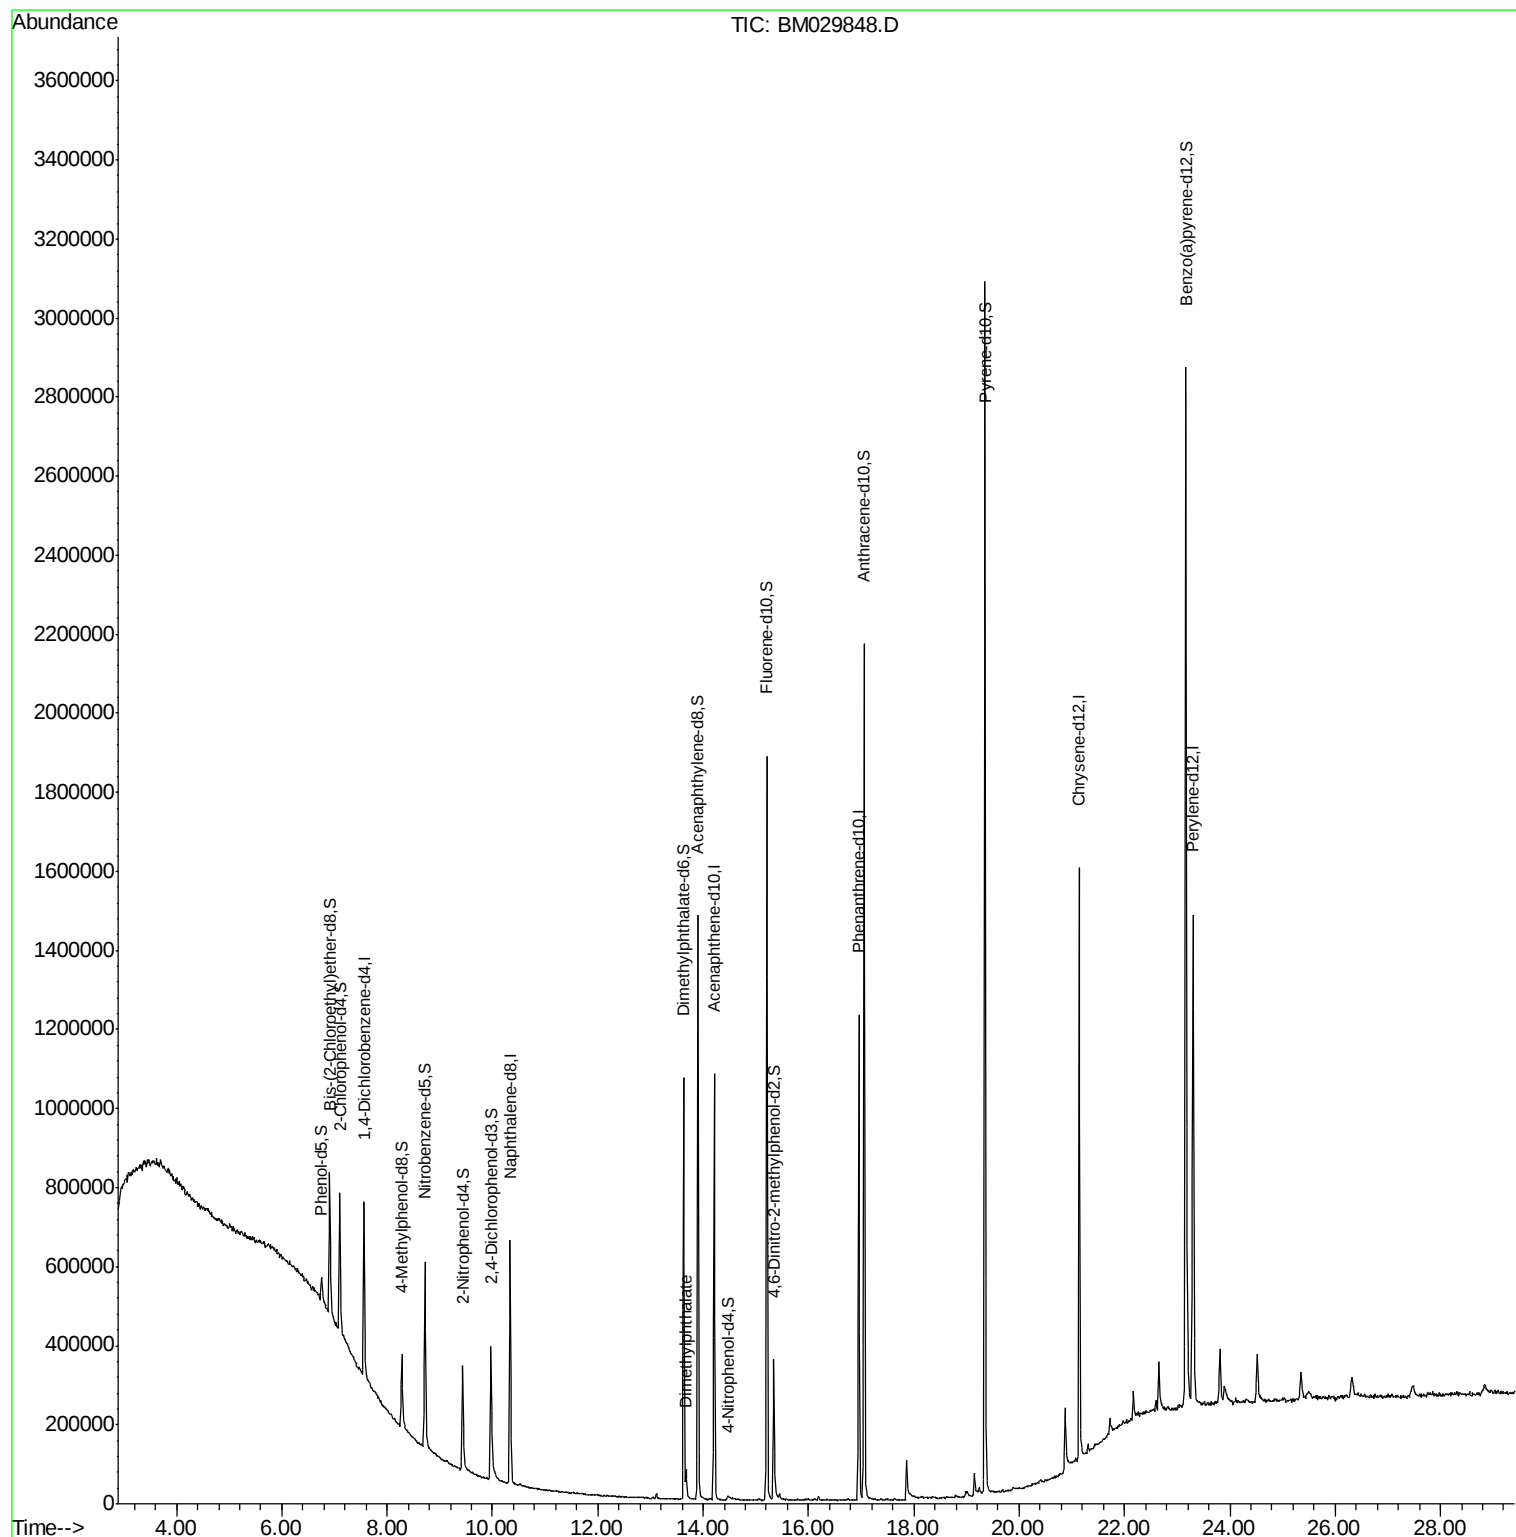

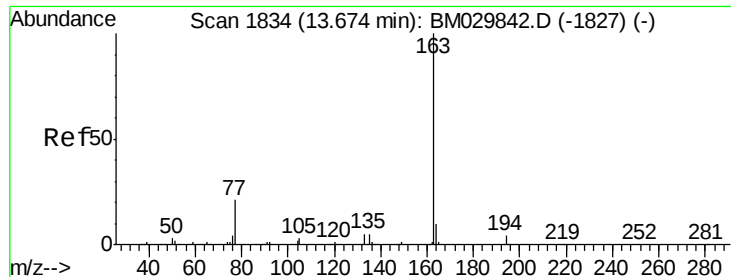

#47
 Dimethylphthalate
 Concen: 1.694 ng/ul
 RT: 13.67 min Scan# 1834
 Delta R.T. -0.01 min
 Lab File: BM029848.D
 Acq: 06 May 2021 04:43

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ2

Tot Ion:	163	Resp:	36818
Ion Ratio	Lower	Upper	
163	100		
194	3.4	3.4	5.0
164	10.7	7.9	11.9

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:52 PM

