

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029850.D
 Acq On : 06 May 2021 05:55
 Operator : CG/JU
 Sample : M2161-06
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AQ4

Manual Integrations
 APPROVED

mohammad
 5/6/2021 4:49:57 PM

Quant Time: May 06 07:04:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 04 14:23:48 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	107679	20.00	ng/ul	0.00
20) Naphthalene-d8	10.34	136	423892	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.21	164	268648	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.96	188	563769	20.00	ng/ul	0.00
79) Chrysene-d12	21.14	240	666547	20.00	ng/ul	-0.01
88) Perylene-d12	23.30	264	765394	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	2474m	0.85	ng/uL	0.00
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.75	99	38222	4.09	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.91	67	158438	27.43	ng/ul	0.00
11) 2-Chlorophenol-d4	7.10	132	150366	20.19	ng/ul	-0.01
15) 4-Methylphenol-d8	8.28	113	77460	10.38	ng/ul	0.00
21) Nitrobenzene-d5	8.72	128	105685	33.56	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.43	143	84042	24.44	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.97	165	141796	22.05	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.51	131	6805m	0.73	ng/ul	0.02
46) Dimethylphthalate-d6	13.63	166	594779	29.64	ng/ul	0.00
49) Acenaphthylene-d8	13.90	160	930559	35.46	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.47	143	6053m	1.96	ng/ul	0.02
60) Fluorene-d10	15.21	176	660536	38.69	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.34	200	56488	14.93	ng/ul	0.00
73) Anthracene-d10	17.06	188	1151760	41.31	ng/ul	0.00
81) Pyrene-d10	19.35	212	1406138	41.12	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.17	264	1676016	39.00	ng/ul	0.00

Target Compounds					Ovalue
47) Dimethylphthalate	13.67	163	29742	1.486 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029850.D
Acq On : 06 May 2021 05:55
Operator : CG/JU
Sample : M2161-06
Misc :
ALS Vial : 69 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AQ4

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:57 PM

Quant Time: May 06 07:04:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 04 14:23:48 2021
Response via : Initial Calibration

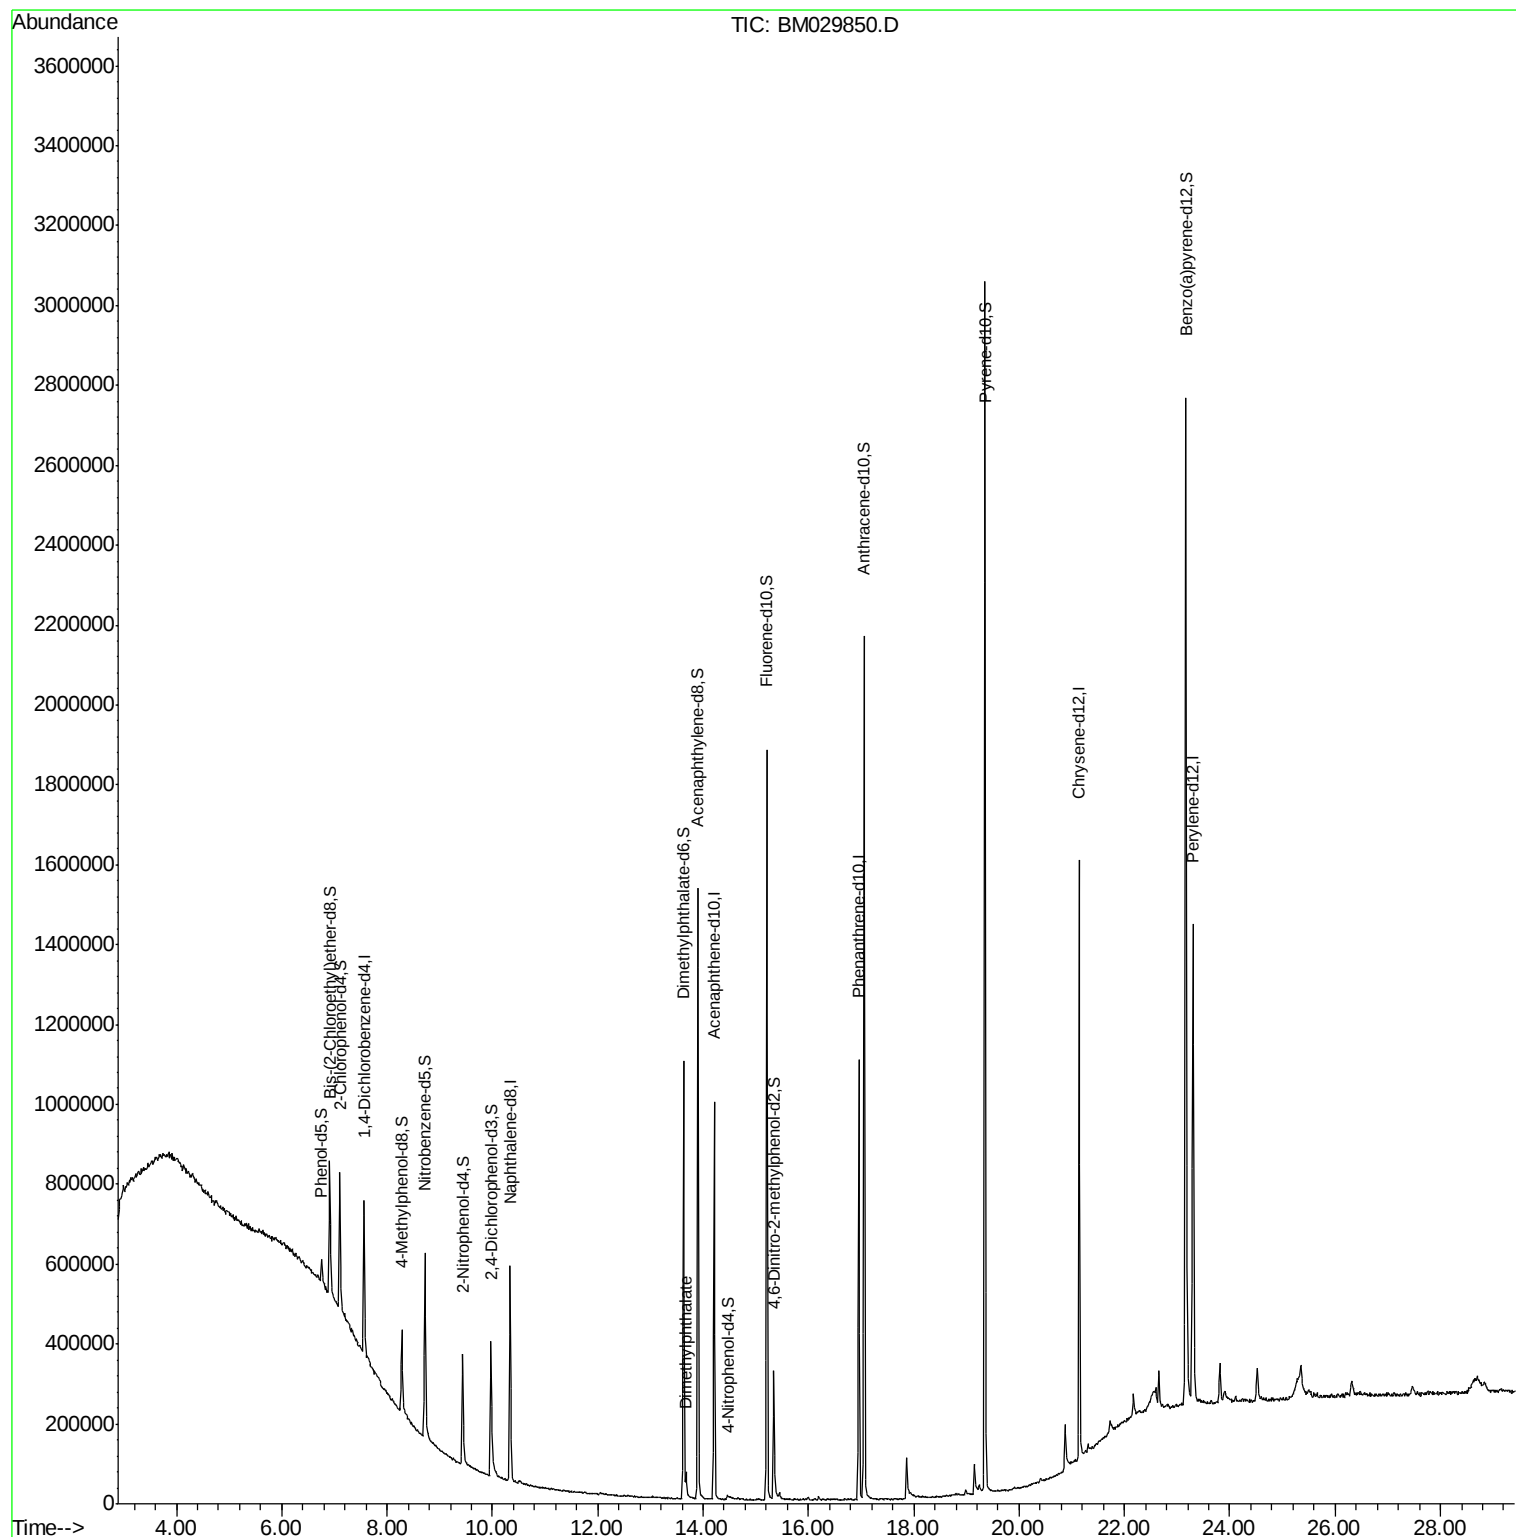

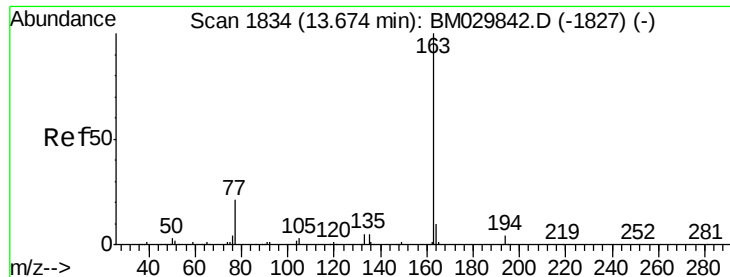

#47

Dimethylphthalate

Concen: 1.486 ng/ul

RT: 13.67 min Scan# 1834

Delta R.T. -0.01 min

Lab File: BM029850.D

Acq: 06 May 2021 05:55

Instrument :

BNA_M

ClientSampleId :

C0AQ4

Tot Ion:	163	Resp:	29742
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.4	5.0
164	9.2	7.9	11.9

Manual Integrations
APPROVED

mohammad
5/6/2021 4:49:57 PM

