

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029796.D
 Acq On : 04 May 2021 19:13
 Operator : CG/JU
 Sample : M2243-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	416	420	421	rBV2	2550	1901	0.14%	0.034%
2	5.869	503	507	510	rBV6	2006	3030	0.23%	0.053%
3	6.939	687	689	691	rBV3	1845	1680	0.13%	0.030%
4	7.139	721	723	727	rVB5	1917	1858	0.14%	0.033%
5	7.239	739	740	744	rVB3	2212	1494	0.11%	0.026%
6	7.334	755	756	759	rBV3	1736	1971	0.15%	0.035%
7	7.575	789	797	819	rBV	232672	501525	37.54%	8.842%
8	7.804	834	836	841	rVB5	1834	2722	0.20%	0.048%
9	8.257	909	913	914	rBV4	1573	1864	0.14%	0.033%
10	8.322	919	924	926	rBV5	1333	2587	0.19%	0.046%
11	8.592	967	970	971	rBV4	2077	1917	0.14%	0.034%
12	8.728	992	993	997	rVB5	2060	1723	0.13%	0.030%
13	8.810	1005	1007	1011	rVB5	1740	1496	0.11%	0.026%
14	8.869	1012	1017	1021	rVV4	2325	3922	0.29%	0.069%
15	9.028	1041	1044	1047	rVB3	1563	1837	0.14%	0.032%
16	9.151	1064	1065	1070	rVB5	2358	2044	0.15%	0.036%
17	9.257	1079	1083	1084	rBV4	2034	1986	0.15%	0.035%
18	9.269	1084	1085	1087	rVV2	2507	1748	0.13%	0.031%
19	9.316	1091	1093	1096	rVB4	1952	1440	0.11%	0.025%
20	9.416	1105	1110	1111	rBV4	1814	2537	0.19%	0.045%
21	9.516	1125	1127	1131	rVV4	1157	1551	0.12%	0.027%
22	9.580	1134	1138	1139	rVV4	1343	1635	0.12%	0.029%
23	9.839	1178	1182	1185	rVB4	1863	1759	0.13%	0.031%
24	9.963	1199	1203	1205	rBV5	916	1406	0.11%	0.025%
25	10.080	1220	1223	1224	rBV2	1503	1399	0.10%	0.025%
26	10.186	1239	1241	1244	rBV3	1216	1464	0.11%	0.026%
27	10.292	1255	1259	1262	rBV5	1144	2019	0.15%	0.036%
28	10.351	1262	1269	1280	rBV	286322	627535	46.97%	11.064%
29	10.522	1296	1298	1300	rVB3	2414	1700	0.13%	0.030%
30	10.792	1341	1344	1347	rBV4	1094	1682	0.13%	0.030%
31	10.880	1357	1359	1360	rBV2	1850	1654	0.12%	0.029%
32	11.104	1394	1397	1399	rVB4	1427	1567	0.12%	0.028%
33	11.145	1402	1404	1407	rVB4	1172	1354	0.10%	0.024%
34	11.633	1484	1487	1488	rVB4	2323	1701	0.13%	0.030%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029796.D
 Acq On : 04 May 2021 19:13
 Operator : CG/JU
 Sample : M2243-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

35	11.786	1508	1513	1515	rBV5	1436	2089	0.16%	0.037%
36	12.257	1592	1593	1597	rVB3	1453	1553	0.12%	0.027%
37	12.286	1597	1598	1602	rBV4	1670	1905	0.14%	0.034%
38	12.398	1615	1617	1620	rBV3	1634	1648	0.12%	0.029%
39	12.798	1682	1685	1688	rVB3	1935	1901	0.14%	0.034%
40	13.239	1756	1760	1762	rBV4	964	1411	0.11%	0.025%
41	13.592	1817	1820	1821	rVB3	1976	1568	0.12%	0.028%
42	13.610	1821	1823	1825	rBV2	2495	2112	0.16%	0.037%
43	13.698	1835	1838	1840	rBV3	1264	1419	0.11%	0.025%
44	13.986	1884	1887	1889	rVB3	1846	1638	0.12%	0.029%
45	14.004	1889	1890	1893	rBV3	1212	1470	0.11%	0.026%
46	14.057	1896	1899	1903	rBV6	1318	2100	0.16%	0.037%
47	14.215	1919	1926	1950	rBV	517284	888924	66.54%	15.673%
48	14.368	1950	1952	1955	rVB4	1673	1394	0.10%	0.025%
49	14.780	2020	2022	2024	rBV3	1598	1615	0.12%	0.028%
50	15.033	2062	2065	2066	rVB2	1439	1389	0.10%	0.024%
51	15.109	2076	2078	2079	rBV2	2167	1872	0.14%	0.033%
52	15.227	2095	2098	2101	rVB4	1106	1568	0.12%	0.028%
53	15.286	2107	2108	2111	rVB3	2105	1545	0.12%	0.027%
54	15.315	2111	2113	2117	rBV4	1391	1902	0.14%	0.034%
55	15.480	2136	2141	2143	rBV5	1761	2543	0.19%	0.045%
56	15.515	2143	2147	2150	rVV3	1140	1655	0.12%	0.029%
57	15.574	2154	2157	2159	rVB3	1619	1465	0.11%	0.026%
58	15.692	2175	2177	2181	rVB4	1454	1800	0.13%	0.032%
59	15.733	2181	2184	2186	rVB2	2013	1596	0.12%	0.028%
60	15.780	2186	2192	2193	rBV6	1700	3067	0.23%	0.054%
61	15.880	2207	2209	2213	rVV5	1953	2538	0.19%	0.045%
62	15.986	2223	2227	2230	rVB3	2589	2795	0.21%	0.049%
63	16.027	2233	2234	2237	rVB2	1657	1532	0.11%	0.027%
64	16.162	2254	2257	2261	rVB5	1458	2192	0.16%	0.039%
65	16.286	2274	2278	2279	rBV3	2509	1859	0.14%	0.033%
66	16.315	2282	2283	2286	rBV2	1999	1684	0.13%	0.030%
67	16.433	2297	2303	2306	rBV4	1330	2445	0.18%	0.043%
68	16.768	2356	2360	2361	rBV4	1572	1700	0.13%	0.030%
69	16.962	2387	2393	2409	rBV	526679	929536	69.58%	16.389%
70	17.251	2439	2442	2443	rVB3	1709	1780	0.13%	0.031%
71	17.398	2463	2467	2468	rVV3	1716	1503	0.11%	0.026%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029796.D
 Acq On : 04 May 2021 19:13
 Operator : CG/JU
 Sample : M2243-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

72	17.521	2486	2488	2491	rVB4	1717	1448	0.11%	0.026%
73	17.574	2494	2497	2500	rBV5	1940	2216	0.17%	0.039%
74	17.656	2507	2511	2513	rBV5	2075	3317	0.25%	0.058%
75	17.903	2546	2553	2557	rBV9	4403	10999	0.82%	0.194%
76	17.933	2557	2558	2562	rBV4	1496	2068	0.15%	0.036%
77	18.050	2575	2578	2580	rBV3	1399	1657	0.12%	0.029%
78	18.103	2584	2587	2588	rVV4	1678	1663	0.12%	0.029%
79	18.421	2639	2641	2642	rBV2	2653	1421	0.11%	0.025%
80	18.480	2649	2651	2653	rBV3	1594	1551	0.12%	0.027%
81	18.639	2676	2678	2679	rBV2	1857	1413	0.11%	0.025%
82	18.792	2700	2704	2706	rBV5	2399	2721	0.20%	0.048%
83	18.868	2715	2717	2718	rVB2	2711	1518	0.11%	0.027%
84	18.886	2718	2720	2722	rBV3	2797	2451	0.18%	0.043%
85	19.345	2796	2798	2799	rBV2	3037	1860	0.14%	0.033%
86	19.362	2799	2801	2802	rBV2	2817	2156	0.16%	0.038%
87	19.456	2815	2817	2820	rBV4	3147	3521	0.26%	0.062%
88	19.544	2830	2832	2835	rBV3	4016	4666	0.35%	0.082%
89	21.144	3100	3104	3121	rBV	751312	1216802	91.08%	21.453%
90	23.309	3466	3472	3488	rBV2	671376	1335993	100.00%	23.555%


Sum of corrected areas: 5671862

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029796.D
Acq On : 04 May 2021 19:13
Operator : CG/JU
Sample : M2243-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

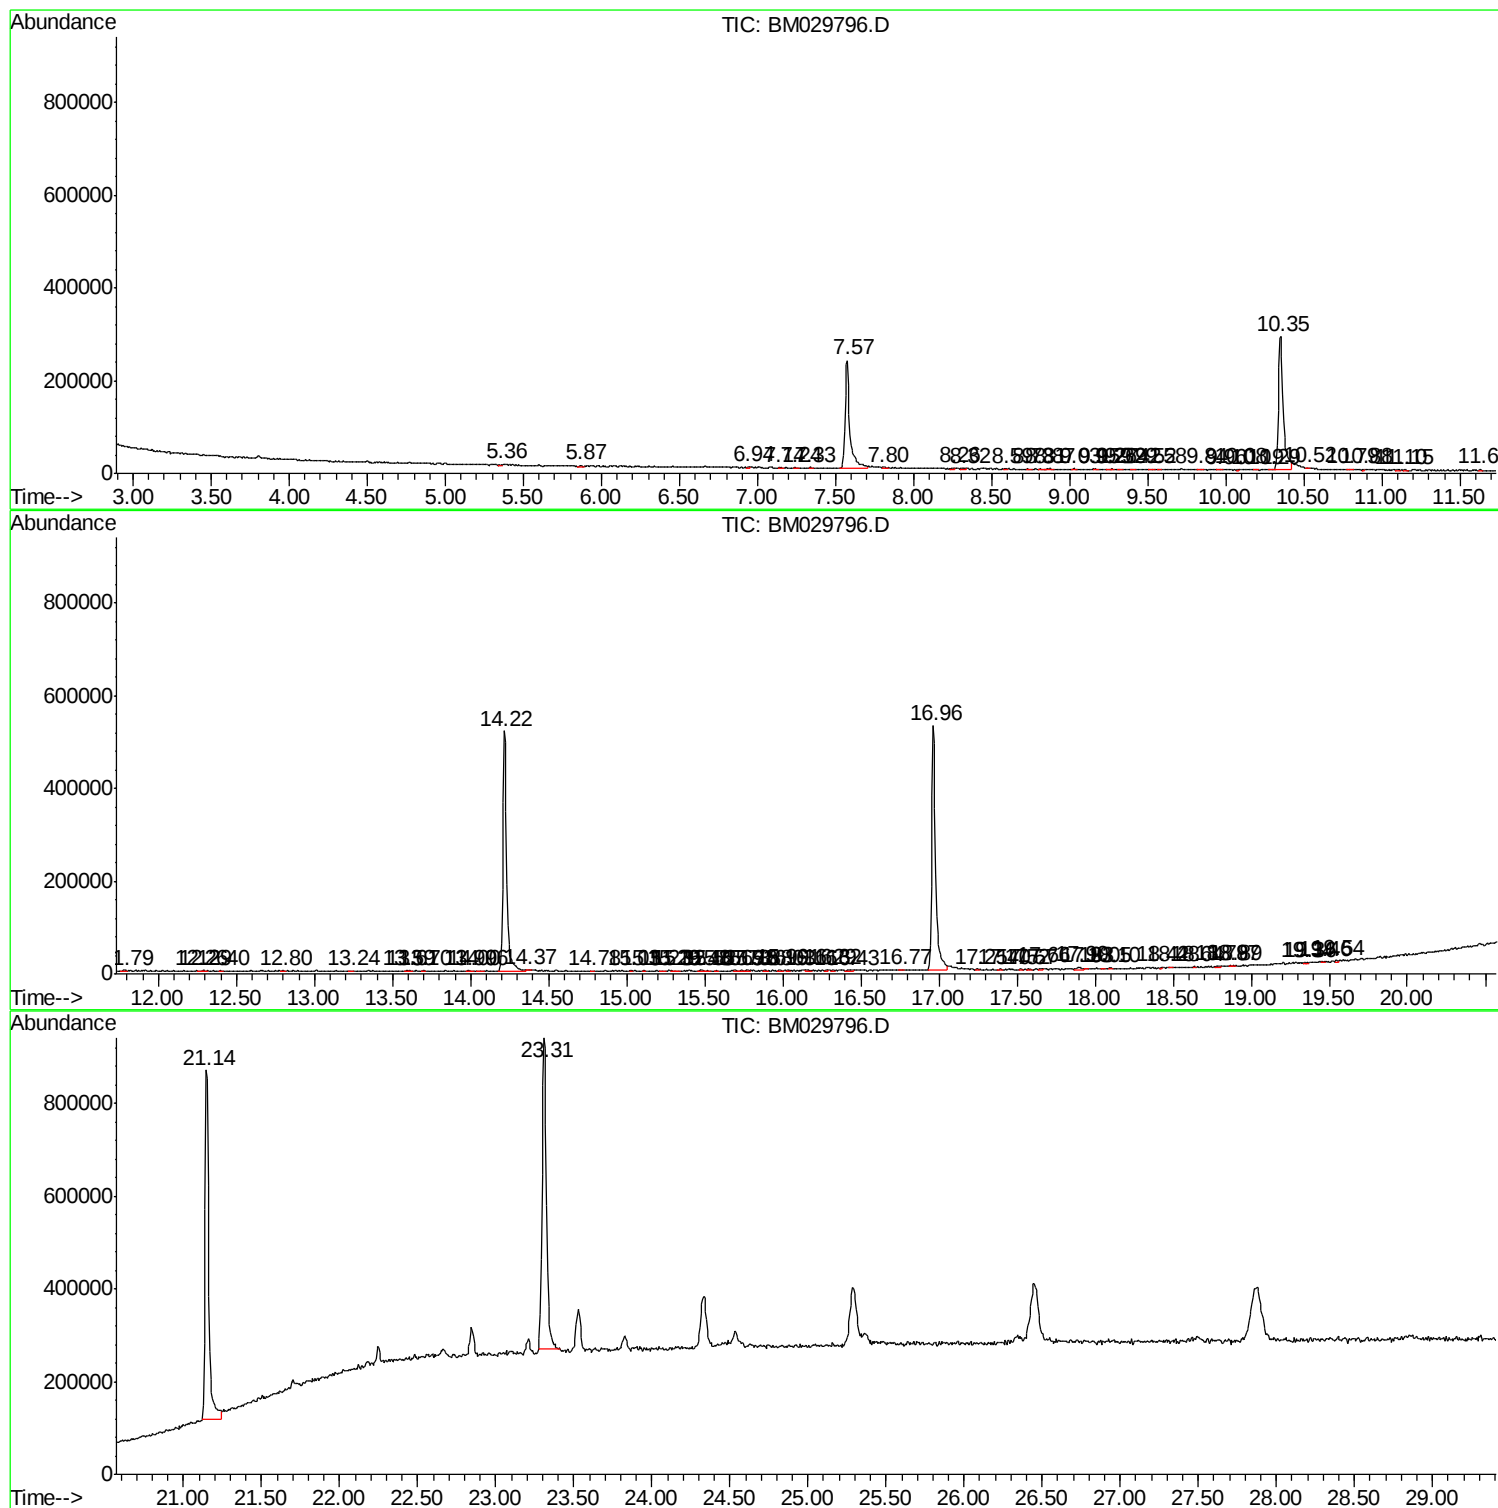

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029796.D
Acq On : 04 May 2021 19:13
Operator : CG/JU
Sample : M2243-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029796.D
Acq On : 04 May 2021 19:13
Operator : CG/JU
Sample : M2243-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc