

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029798.D
 Acq On : 04 May 2021 21:02
 Operator : CG/JU
 Sample : M2243-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.793	152	154	156	rBV3	5978	6161	0.42%	0.098%
2	5.704	477	479	481	rBV2	2585	2370	0.16%	0.038%
3	6.516	615	617	619	rBV2	2097	2289	0.16%	0.036%
4	6.963	689	693	694	rBV4	1615	1477	0.10%	0.023%
5	7.022	701	703	706	rBV3	1720	1886	0.13%	0.030%
6	7.069	709	711	714	rVB4	1728	1818	0.12%	0.029%
7	7.175	725	729	733	rBV5	1624	2920	0.20%	0.046%
8	7.569	789	796	812	rBV	247195	529358	36.11%	8.415%
9	7.863	845	846	850	rBV4	1624	1796	0.12%	0.029%
10	7.928	853	857	859	rBV5	1333	1889	0.13%	0.030%
11	8.169	897	898	903	rBV4	1577	2154	0.15%	0.034%
12	9.492	1120	1123	1126	rVB4	1673	2169	0.15%	0.034%
13	9.845	1182	1183	1186	rBV3	1359	1719	0.12%	0.027%
14	10.345	1261	1268	1292	rBV	339232	755743	51.55%	12.013%
15	10.569	1304	1306	1311	rVV5	2256	3132	0.21%	0.050%
16	10.604	1311	1312	1316	rVB4	2584	2344	0.16%	0.037%
17	10.739	1332	1335	1340	rVB6	1248	2013	0.14%	0.032%
18	10.845	1350	1353	1354	rVB3	2063	1814	0.12%	0.029%
19	10.869	1354	1357	1358	rBV3	1733	1800	0.12%	0.029%
20	11.069	1389	1391	1393	rVB2	1741	1548	0.11%	0.025%
21	11.216	1413	1416	1417	rBV3	1813	1512	0.10%	0.024%
22	11.275	1423	1426	1430	rVB5	1064	1494	0.10%	0.024%
23	11.316	1430	1433	1436	rVB4	1316	1593	0.11%	0.025%
24	11.469	1454	1459	1462	rVB5	1622	2304	0.16%	0.037%
25	11.969	1542	1544	1546	rBV3	1569	2085	0.14%	0.033%
26	12.033	1553	1555	1558	rBV4	1196	1548	0.11%	0.025%
27	12.974	1712	1715	1717	rBV3	1858	1550	0.11%	0.025%
28	13.374	1777	1783	1784	rVB4	1157	1887	0.13%	0.030%
29	13.539	1809	1811	1813	rVB3	1671	1544	0.11%	0.025%
30	13.574	1813	1817	1820	rBV4	2556	3624	0.25%	0.058%
31	14.216	1919	1926	1944	rBV	572594	999245	68.17%	15.884%
32	14.516	1972	1977	1979	rBV4	1101	1642	0.11%	0.026%
33	14.980	2052	2056	2058	rVB4	1576	1736	0.12%	0.028%
34	15.163	2084	2087	2089	rBV3	1521	1538	0.10%	0.024%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029798.D
 Acq On : 04 May 2021 21:02
 Operator : CG/JU
 Sample : M2243-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

35	15.251	2099	2102	2105	rVB4	1273	1495	0.10%	0.024%
36	15.451	2135	2136	2142	rVB5	1909	2636	0.18%	0.042%
37	15.504	2142	2145	2146	rBV3	1878	1782	0.12%	0.028%
38	15.686	2174	2176	2179	rVB3	1493	1724	0.12%	0.027%
39	15.898	2211	2212	2215	rBV3	1516	1691	0.12%	0.027%
40	16.115	2246	2249	2252	rVB5	1858	2031	0.14%	0.032%
41	16.145	2252	2254	2256	rBV3	1822	1609	0.11%	0.026%
42	16.415	2298	2300	2303	rBV4	1289	1550	0.11%	0.025%
43	16.457	2306	2307	2310	rVB3	1725	1551	0.11%	0.025%
44	16.498	2310	2314	2316	rBV4	1801	2933	0.20%	0.047%
45	16.757	2356	2358	2365	rVB7	2094	3754	0.26%	0.060%
46	16.962	2387	2393	2409	rBV	576506	1073321	73.22%	17.062%
47	17.298	2448	2450	2453	rVB3	1827	1658	0.11%	0.026%
48	17.392	2463	2466	2470	rBV5	1401	2470	0.17%	0.039%
49	17.733	2521	2524	2526	rVB3	1509	1719	0.12%	0.027%
50	17.768	2526	2530	2531	rBV2	2072	2271	0.15%	0.036%
51	17.898	2550	2552	2553	rBV2	1981	1980	0.14%	0.031%
52	18.121	2589	2590	2593	rBV2	1917	2314	0.16%	0.037%
53	18.221	2602	2607	2610	rBV4	2197	3870	0.26%	0.062%
54	18.409	2634	2639	2640	rBV4	1953	3484	0.24%	0.055%
55	18.856	2712	2715	2717	rBV4	3039	3195	0.22%	0.051%
56	19.174	2767	2769	2771	rVB2	3544	2403	0.16%	0.038%
57	19.198	2771	2773	2774	rBV2	3381	3318	0.23%	0.053%
58	19.456	2815	2817	2820	rBV4	3148	4276	0.29%	0.068%
59	21.150	3100	3105	3115	rBV	895744	1346191	91.83%	21.399%
60	23.309	3466	3472	3483	rBV	744949	1465900	100.00%	23.302%


Sum of corrected areas: 6290828

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029798.D
Acq On : 04 May 2021 21:02
Operator : CG/JU
Sample : M2243-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

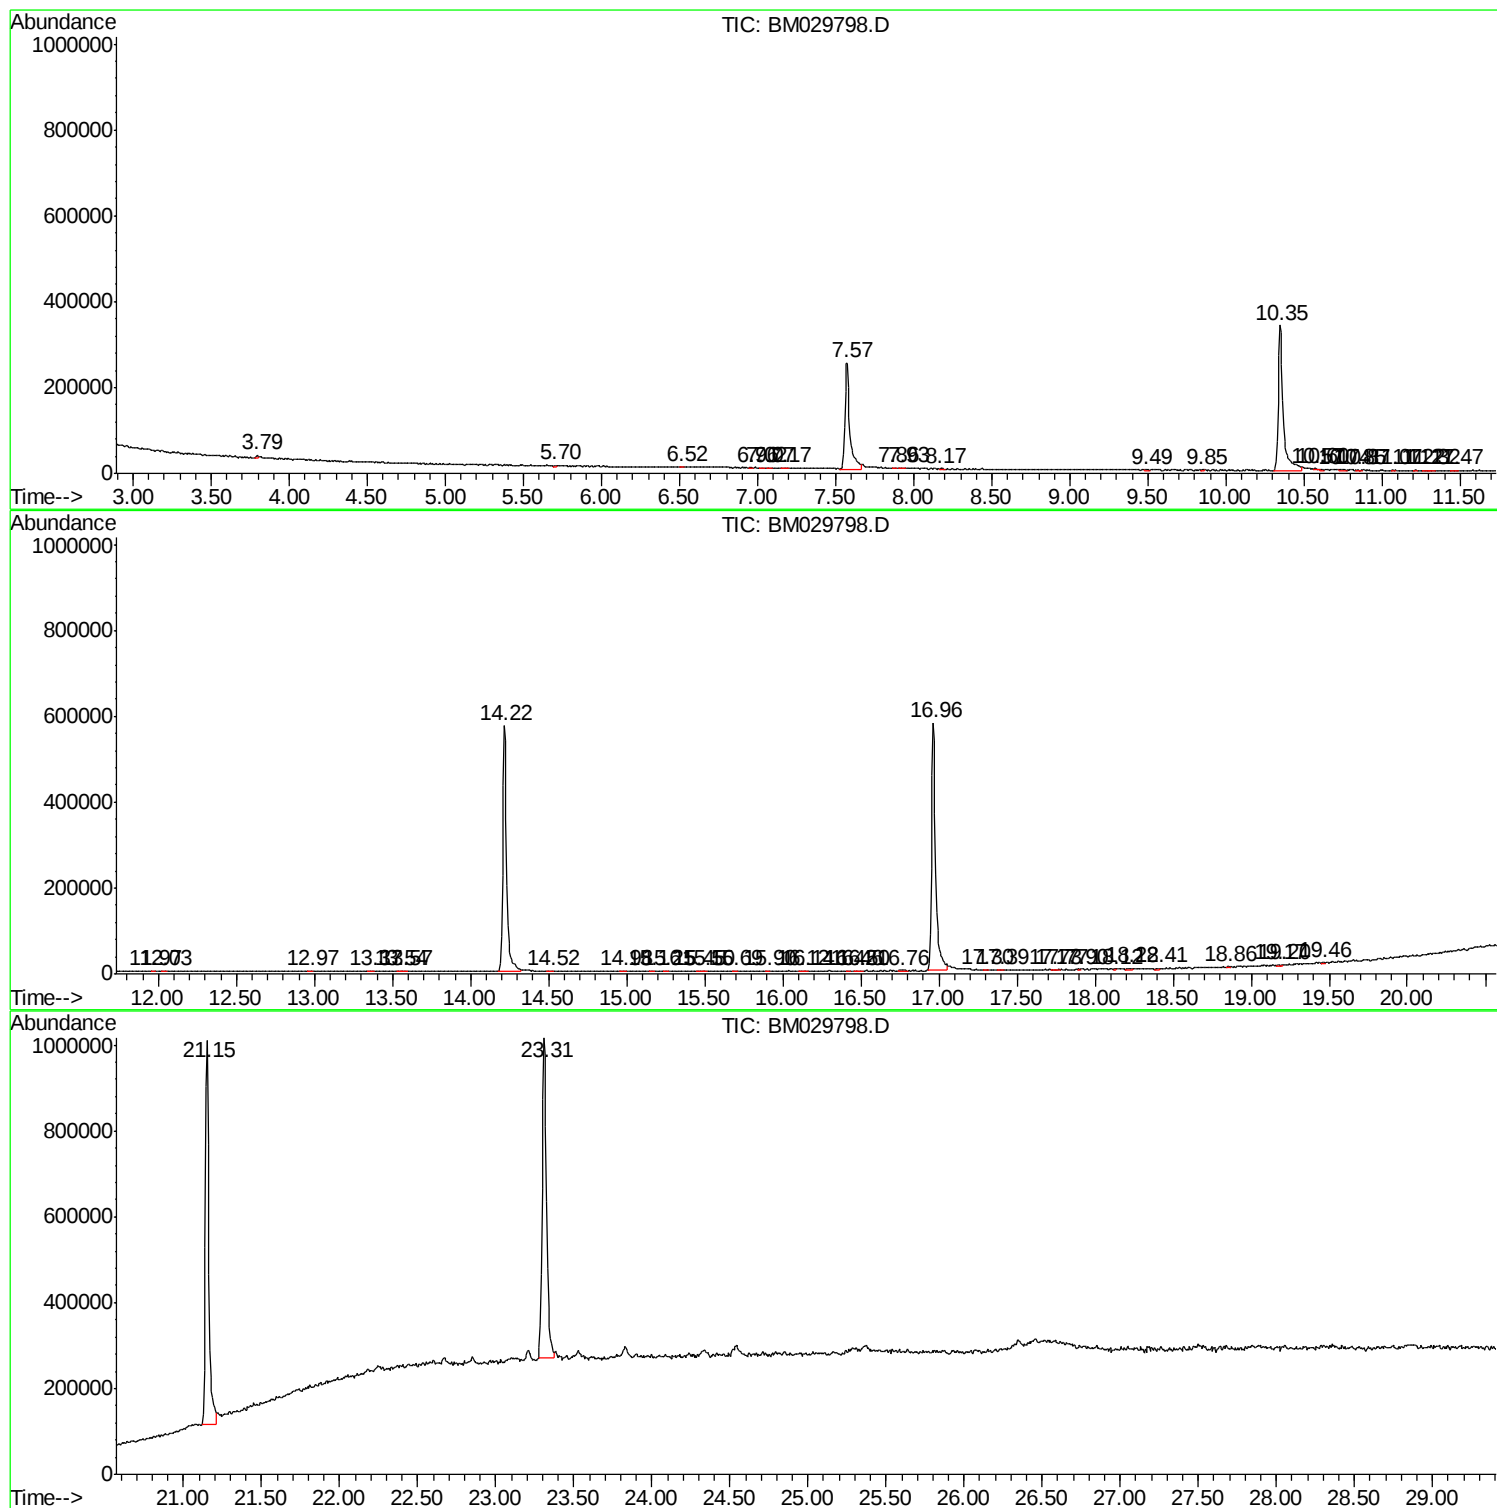

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029798.D
Acq On : 04 May 2021 21:02
Operator : CG/JU
Sample : M2243-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029798.D
Acq On : 04 May 2021 21:02
Operator : CG/JU
Sample : M2243-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc