

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029820.D
 Acq On : 05 May 2021 10:55
 Operator : CG/JU
 Sample : M2127-23
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.775	652	661	678	rVV2	213464	603574	14.16%	1.875%
2	6.910	679	684	706	rVB	422864	770180	18.07%	2.393%
3	7.104	711	717	730	rVB	516837	896118	21.02%	2.784%
4	7.569	789	796	805	rBV	372447	642162	15.06%	1.995%
5	8.280	911	917	934	rBV	335487	638756	14.98%	1.985%
6	8.722	985	992	1003	rBV	543266	978012	22.94%	3.039%
7	9.145	1059	1064	1068	rVB2	12231	21425	0.50%	0.067%
8	9.439	1106	1114	1127	rBV	442735	827426	19.41%	2.571%
9	9.975	1199	1205	1236	rBV	507337	1116255	26.18%	3.468%
10	10.339	1260	1267	1278	rBV	502387	882987	20.71%	2.743%
11	10.527	1293	1299	1305	rBV9	9291	25295	0.59%	0.079%
12	11.545	1467	1472	1477	rBV5	3790	6582	0.15%	0.020%
13	11.957	1534	1542	1548	rBV7	7901	16263	0.38%	0.051%
14	12.574	1639	1647	1649	rBV5	3320	5746	0.13%	0.018%
15	12.821	1684	1689	1693	rBV6	3467	5954	0.14%	0.018%
16	13.045	1721	1727	1733	rBV8	5481	12582	0.30%	0.039%
17	13.121	1733	1740	1747	rVV4	8391	17933	0.42%	0.056%
18	13.186	1747	1751	1755	rVB5	2867	4805	0.11%	0.015%
19	13.633	1820	1827	1832	rBV	1165514	1682601	39.47%	5.228%
20	13.680	1832	1835	1843	rVV	106844	163477	3.83%	0.508%
21	13.739	1843	1845	1852	rVB6	3824	7876	0.18%	0.024%
22	13.904	1862	1873	1888	rBV	1516715	2268344	53.21%	7.048%
23	14.127	1906	1911	1915	rBV5	5000	6611	0.16%	0.021%
24	14.215	1919	1926	1935	rBV	770038	1137656	26.69%	3.535%
25	14.468	1965	1969	1970	rBV	15490	17888	0.42%	0.056%
26	14.857	2031	2035	2039	rVB3	7498	9446	0.22%	0.029%
27	15.027	2059	2064	2067	rBV2	8327	13221	0.31%	0.041%
28	15.086	2071	2074	2079	rVB4	4702	6181	0.14%	0.019%
29	15.209	2089	2095	2112	rBV	1789411	2606160	61.13%	8.097%
30	15.345	2112	2118	2133	rVV	542484	842625	19.76%	2.618%
31	15.457	2133	2137	2142	rVB2	19168	29950	0.70%	0.093%
32	15.592	2157	2160	2164	rVB6	3121	4323	0.10%	0.013%
33	15.786	2187	2193	2198	rBV8	4610	9804	0.23%	0.030%
34	15.898	2208	2212	2216	rBV3	6726	9106	0.21%	0.028%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029820.D
 Acq On : 05 May 2021 10:55
 Operator : CG/JU
 Sample : M2127-23
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0AA4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

35	15.945	2216	2220	2223	rVV5	5396	7762	0.18%	0.024%
36	15.998	2226	2229	2233	rVB5	9820	13769	0.32%	0.043%
37	16.115	2243	2249	2254	rVB7	3912	8315	0.20%	0.026%
38	16.198	2259	2263	2268	rVB3	6786	10214	0.24%	0.032%
39	16.645	2334	2339	2343	rBV8	2199	4360	0.10%	0.014%
40	16.703	2344	2349	2352	rVV4	6666	9642	0.23%	0.030%
41	16.745	2352	2356	2359	rVV4	6275	10334	0.24%	0.032%
42	16.956	2386	2392	2402	rBV	876301	1302129	30.54%	4.046%
43	17.056	2403	2409	2426	rVV	1955101	2888487	67.75%	8.974%
44	17.286	2445	2448	2451	rVB4	4990	6511	0.15%	0.020%
45	17.639	2505	2508	2511	rVV5	4095	5990	0.14%	0.019%
46	17.815	2535	2538	2541	rBV5	3509	4913	0.12%	0.015%
47	17.868	2542	2547	2556	rBV	65098	112610	2.64%	0.350%
48	18.162	2593	2597	2600	rBV6	2720	5051	0.12%	0.016%
49	18.356	2627	2630	2635	rVB4	5619	7663	0.18%	0.024%
50	18.627	2671	2676	2681	rBV2	26745	35414	0.83%	0.110%
51	18.992	2733	2738	2741	rBV	20213	32383	0.76%	0.101%
52	19.156	2761	2766	2776	rBV3	44774	81079	1.90%	0.252%
53	19.244	2777	2781	2787	rVB2	17202	30502	0.72%	0.095%
54	19.356	2794	2800	2818	rBV	2682195	3583049	84.04%	11.132%
55	19.768	2868	2870	2872	rBV3	5036	5478	0.13%	0.017%
56	20.409	2975	2979	2985	rBV8	13495	30560	0.72%	0.095%
57	20.874	3055	3058	3068	rBV3	57629	97437	2.29%	0.303%
58	21.144	3099	3104	3114	rBV	1120885	1576634	36.98%	4.899%
59	23.174	3442	3449	3463	rBV	2289546	4263278	100.00%	13.246%
60	23.309	3465	3472	3483	rVB	935042	1765041	41.40%	5.484%


Sum of corrected areas: 32185929

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029820.D
Acq On : 05 May 2021 10:55
Operator : CG/JU
Sample : M2127-23
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AA4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

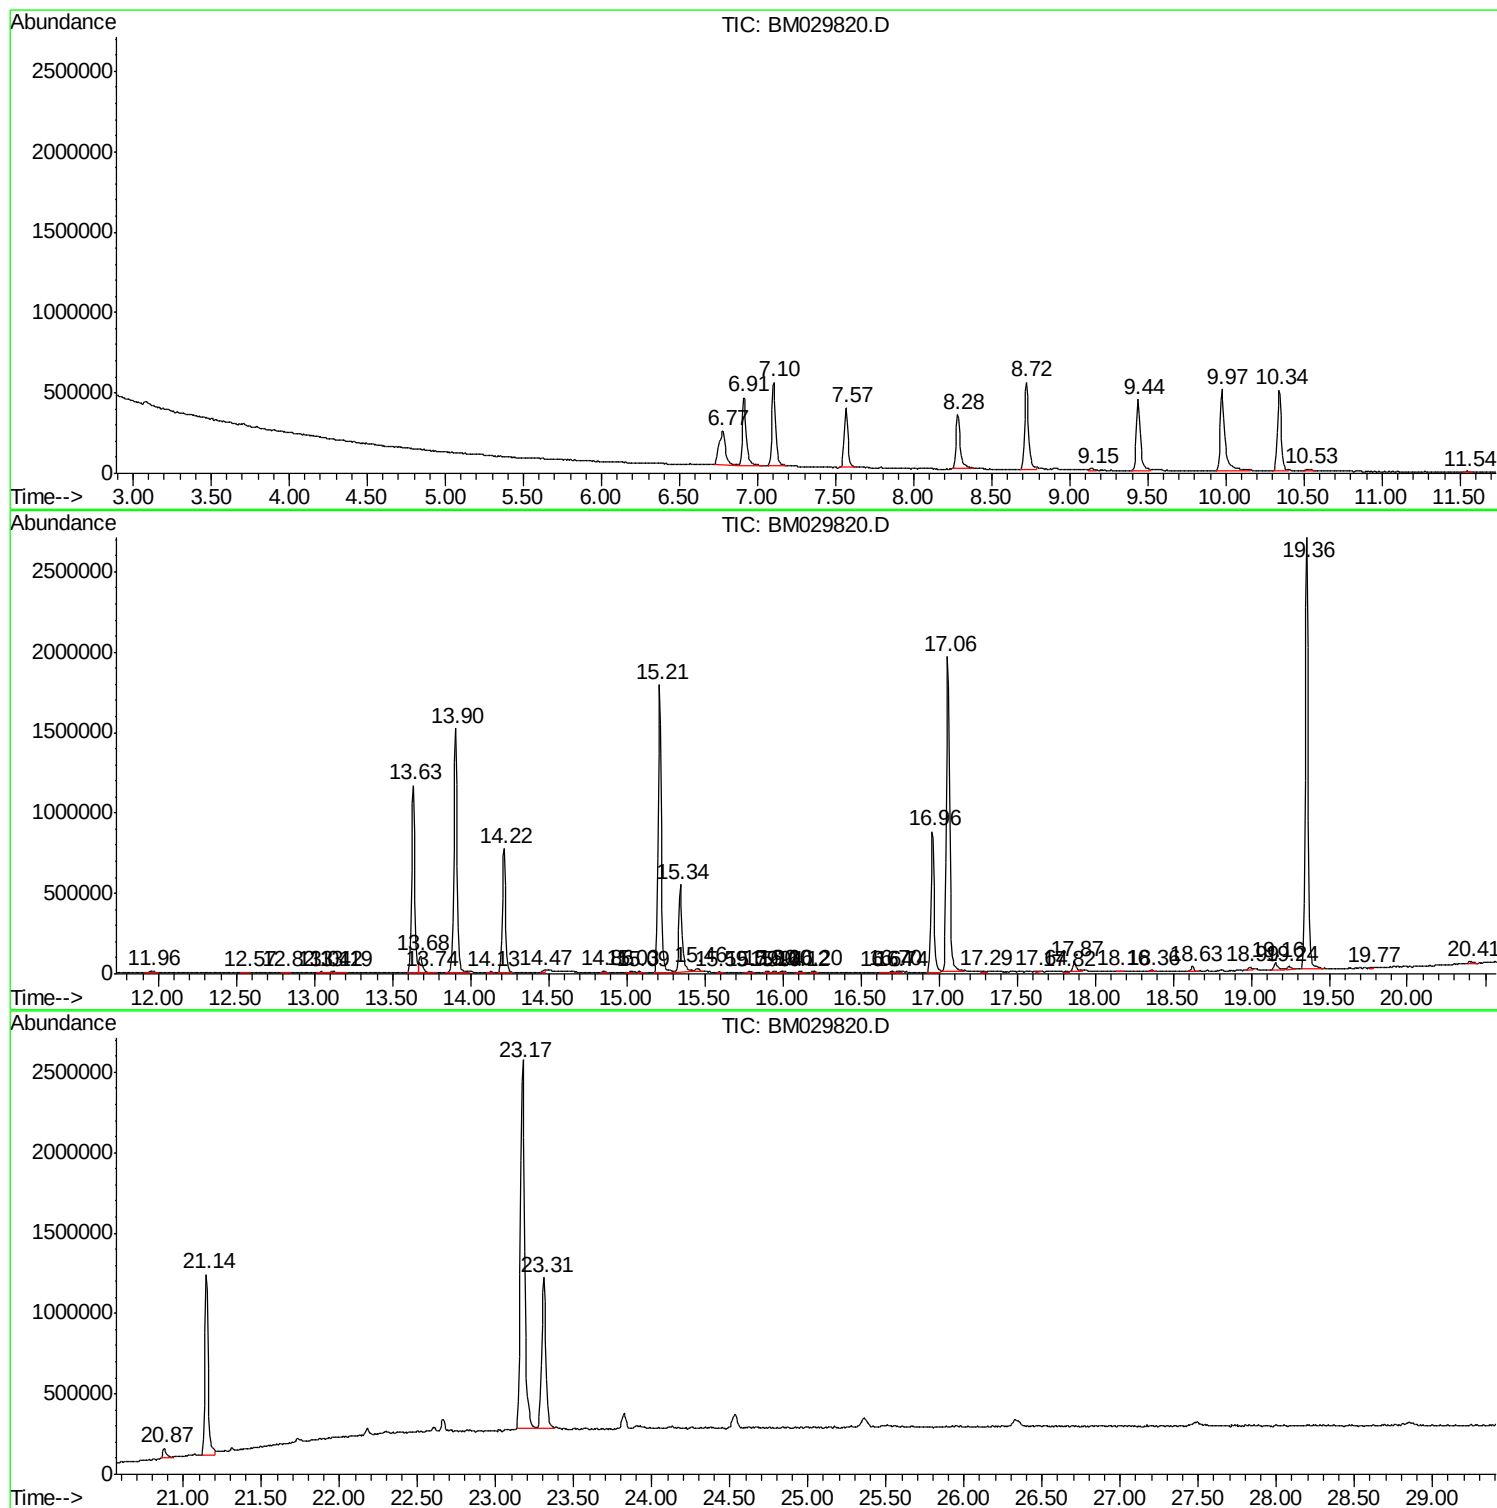

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029820.D
Acq On : 05 May 2021 10:55
Operator : CG/JU
Sample : M2127-23
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AA4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029820.D
Acq On : 05 May 2021 10:55
Operator : CG/JU
Sample : M2127-23
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0AA4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc