

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029827.D
 Acq On : 05 May 2021 15:18
 Operator : CG/JU
 Sample : PB135972BL
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK972

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.499	102	104	119	rBV2	148714	304565	11.98%	1.340%
2	6.751	652	657	670	rBV	346962	626586	24.64%	2.756%
3	6.916	680	685	704	rVB	266259	518378	20.38%	2.280%
4	7.104	711	717	731	rVB	401732	715958	28.15%	3.149%
5	7.563	790	795	807	rVB	324333	557841	21.93%	2.454%
6	8.281	911	917	935	rBV	404900	763441	30.02%	3.358%
7	8.722	986	992	1010	rBV	339002	624955	24.57%	2.749%
8	9.439	1108	1114	1126	rBV	268083	502488	19.76%	2.210%
9	9.975	1199	1205	1228	rBV	339033	720245	28.32%	3.168%
10	10.339	1261	1267	1276	rBV	458644	769792	30.27%	3.386%
11	10.492	1287	1293	1317	rBV	273142	703491	27.66%	3.094%
12	11.963	1540	1543	1547	rVB5	2503	3607	0.14%	0.016%
13	13.633	1821	1827	1844	rBV	711168	1088336	42.79%	4.787%
14	13.904	1864	1873	1883	rBV	913100	1351972	53.16%	5.947%
15	14.004	1888	1890	1895	rVB4	2878	3782	0.15%	0.017%
16	14.210	1919	1925	1935	rBV	641874	963997	37.90%	4.240%
17	14.333	1944	1946	1950	rBV3	2254	2635	0.10%	0.012%
18	14.457	1960	1967	1991	rBV3	65731	300905	11.83%	1.324%
19	14.851	2032	2034	2040	rVB6	2602	3534	0.14%	0.016%
20	15.210	2086	2095	2110	rBV	1097318	1606261	63.16%	7.065%
21	15.345	2113	2118	2132	rVV	231840	403977	15.88%	1.777%
22	15.457	2132	2137	2142	rVB3	13356	24354	0.96%	0.107%
23	15.998	2226	2229	2235	rBV5	4442	7447	0.29%	0.033%
24	16.751	2352	2357	2360	rBV4	2211	3685	0.14%	0.016%
25	16.957	2386	2392	2403	rBV	715126	1057656	41.59%	4.652%
26	17.057	2403	2409	2423	rVV	1142533	1706366	67.09%	7.506%
27	18.780	2701	2702	2705	rBV3	2851	2840	0.11%	0.012%
28	18.992	2735	2738	2745	rVB2	8020	13261	0.52%	0.058%
29	19.245	2777	2781	2785	rVV2	8961	13048	0.51%	0.057%
30	19.356	2793	2800	2813	rBV	1469993	2092606	82.28%	9.205%
31	19.562	2833	2835	2838	rBV4	3120	3772	0.15%	0.017%
32	19.603	2840	2842	2844	rBV2	3732	2643	0.10%	0.012%
33	21.145	3099	3104	3113	rBV	890488	1237921	48.67%	5.445%
34	23.168	3442	3448	3462	rBV	1307842	2543336	100.00%	11.187%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029827.D
Acq On : 05 May 2021 15:18
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Title : SVOA CALIBRATION

35	23.303	3465	3471	3485	rVB2	754557	1488857	58.54%	6.549%
----	--------	------	------	------	------	--------	---------	--------	--------


Sum of corrected areas: 22734538

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029827.D
Acq On : 05 May 2021 15:18
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

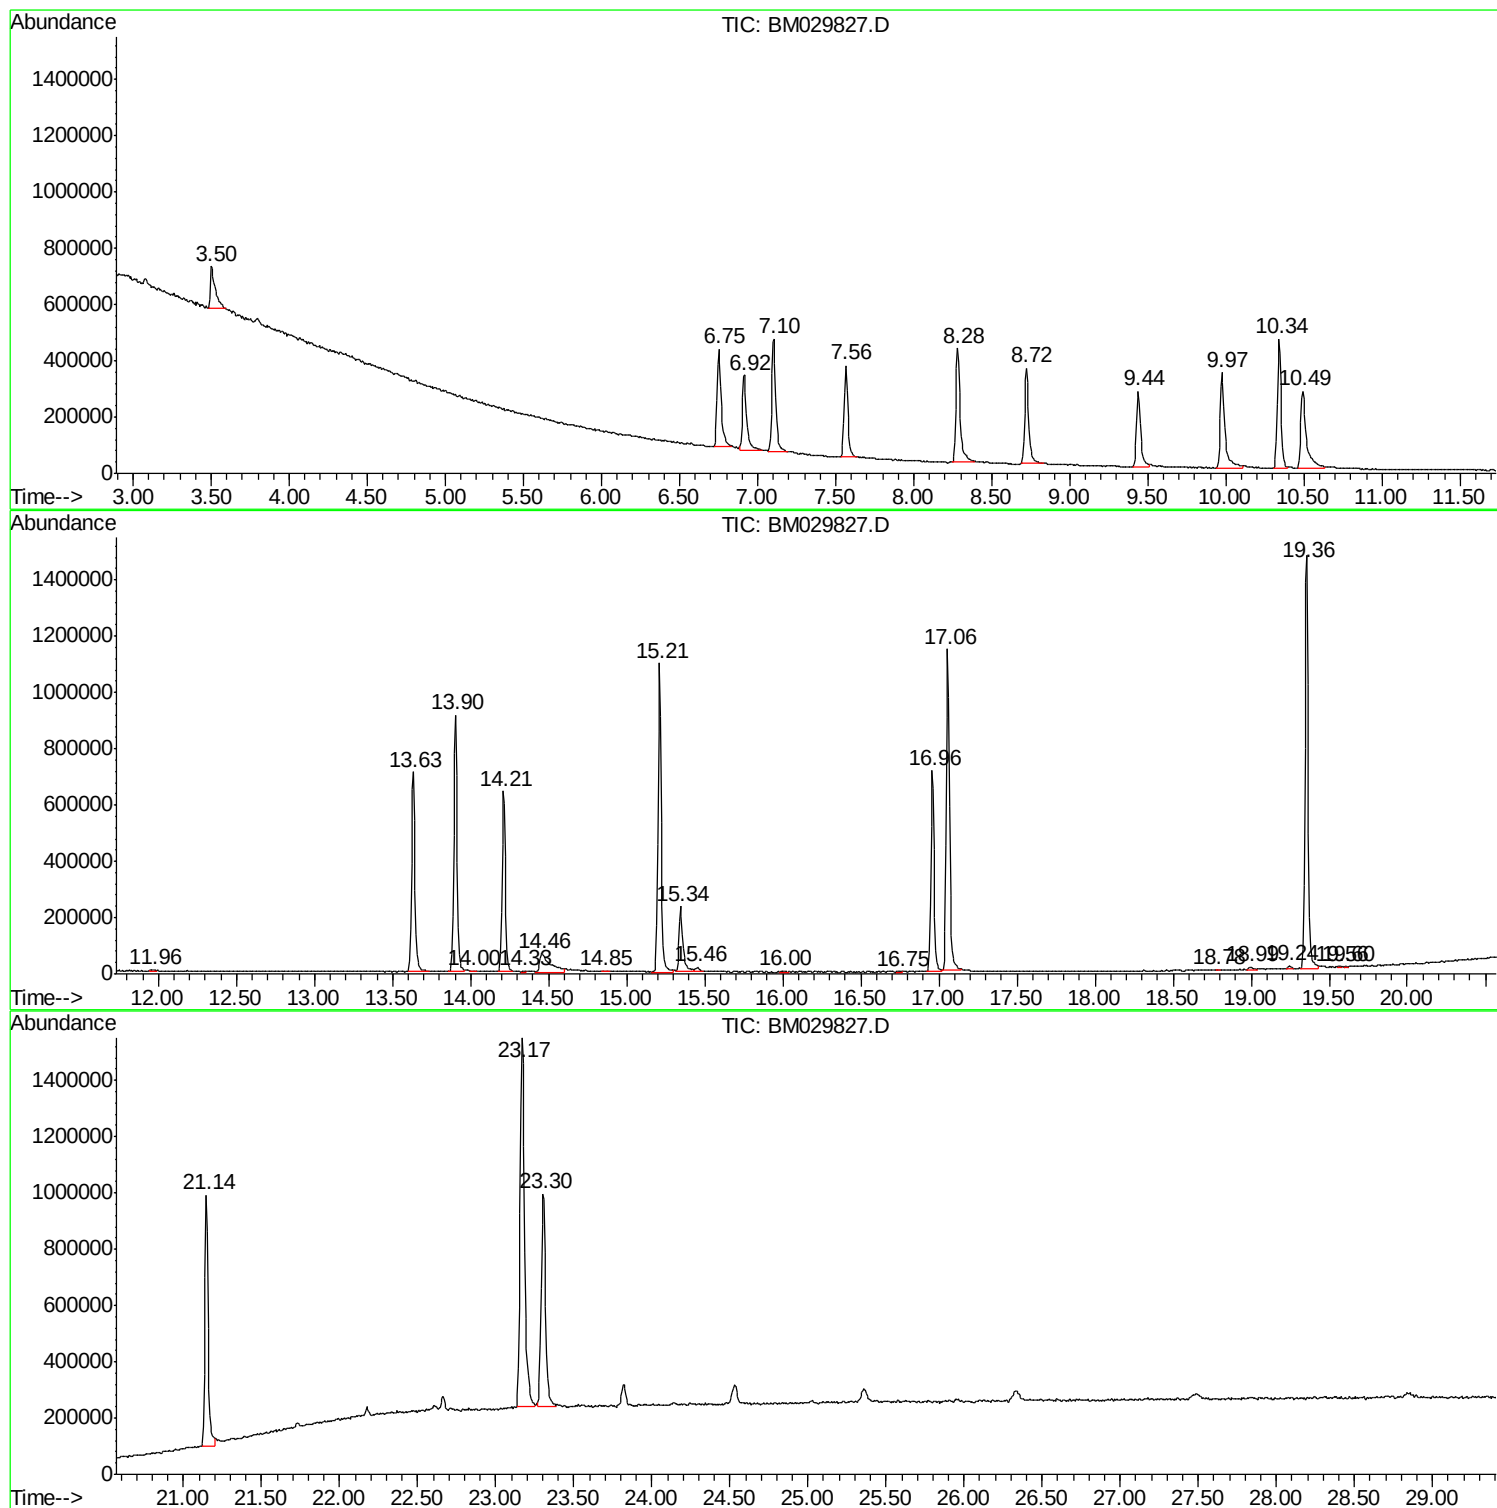

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029827.D
Acq On : 05 May 2021 15:18
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029827.D
Acq On : 05 May 2021 15:18
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc