

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
 Data File : BM029843.D
 Acq On : 06 May 2021 01:43
 Operator : CG/JU
 Sample : PB136016BL
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK016

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.751	653	657	670	rVB	322546	571674	21.56%	2.685%
2	6.910	680	684	695	rVB2	302524	532276	20.08%	2.500%
3	7.098	712	716	730	rVB2	378728	654846	24.70%	3.076%
4	7.563	790	795	805	rVB	341134	564812	21.31%	2.653%
5	8.281	912	917	928	rVB	352690	593245	22.38%	2.786%
6	8.722	986	992	1015	rVB	335838	646461	24.39%	3.036%
7	9.439	1108	1114	1126	rVB2	181662	327576	12.36%	1.539%
8	9.975	1199	1205	1220	rBV	286856	546718	20.62%	2.568%
9	10.339	1260	1267	1276	rBV	445714	715640	26.99%	3.361%
10	10.492	1287	1293	1317	rVB	260197	568391	21.44%	2.670%
11	13.633	1821	1827	1840	rBV	685968	952262	35.92%	4.473%
12	13.904	1866	1873	1887	rBV	925787	1300663	49.06%	6.109%
13	14.210	1919	1925	1935	rBV	718996	984866	37.15%	4.626%
14	14.445	1960	1965	1980	rBV3	44254	161321	6.09%	0.758%
15	15.210	2089	2095	2107	rBV	1177655	1593906	60.12%	7.486%
16	15.286	2107	2108	2112	rVV4	4765	4403	0.17%	0.021%
17	15.345	2112	2118	2132	rVV	157722	266131	10.04%	1.250%
18	15.451	2132	2136	2144	rVB5	9003	17143	0.65%	0.081%
19	16.957	2386	2392	2403	rBV	757897	981881	37.04%	4.612%
20	17.057	2403	2409	2424	rVB2	1305561	1779981	67.14%	8.360%
21	17.504	2481	2485	2487	rBV4	2054	3141	0.12%	0.015%
22	18.574	2663	2667	2669	rBV5	1928	2853	0.11%	0.013%
23	18.998	2734	2739	2742	rBV4	5633	8045	0.30%	0.038%
24	19.239	2778	2780	2786	rVB5	4261	7085	0.27%	0.033%
25	19.350	2794	2799	2813	rBV	1659376	2119288	79.94%	9.954%
26	21.144	3099	3104	3116	rBV	919850	1290355	48.67%	6.061%
27	23.168	3441	3448	3463	rBV	1400766	2651044	100.00%	12.452%
28	23.303	3465	3471	3479	rVV2	779976	1444845	54.50%	6.786%


Sum of corrected areas: 21290852

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050421\
Data File : BM029843.D
Acq On : 06 May 2021 01:43
Operator : CG/JU
Sample : PB136016BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK016

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

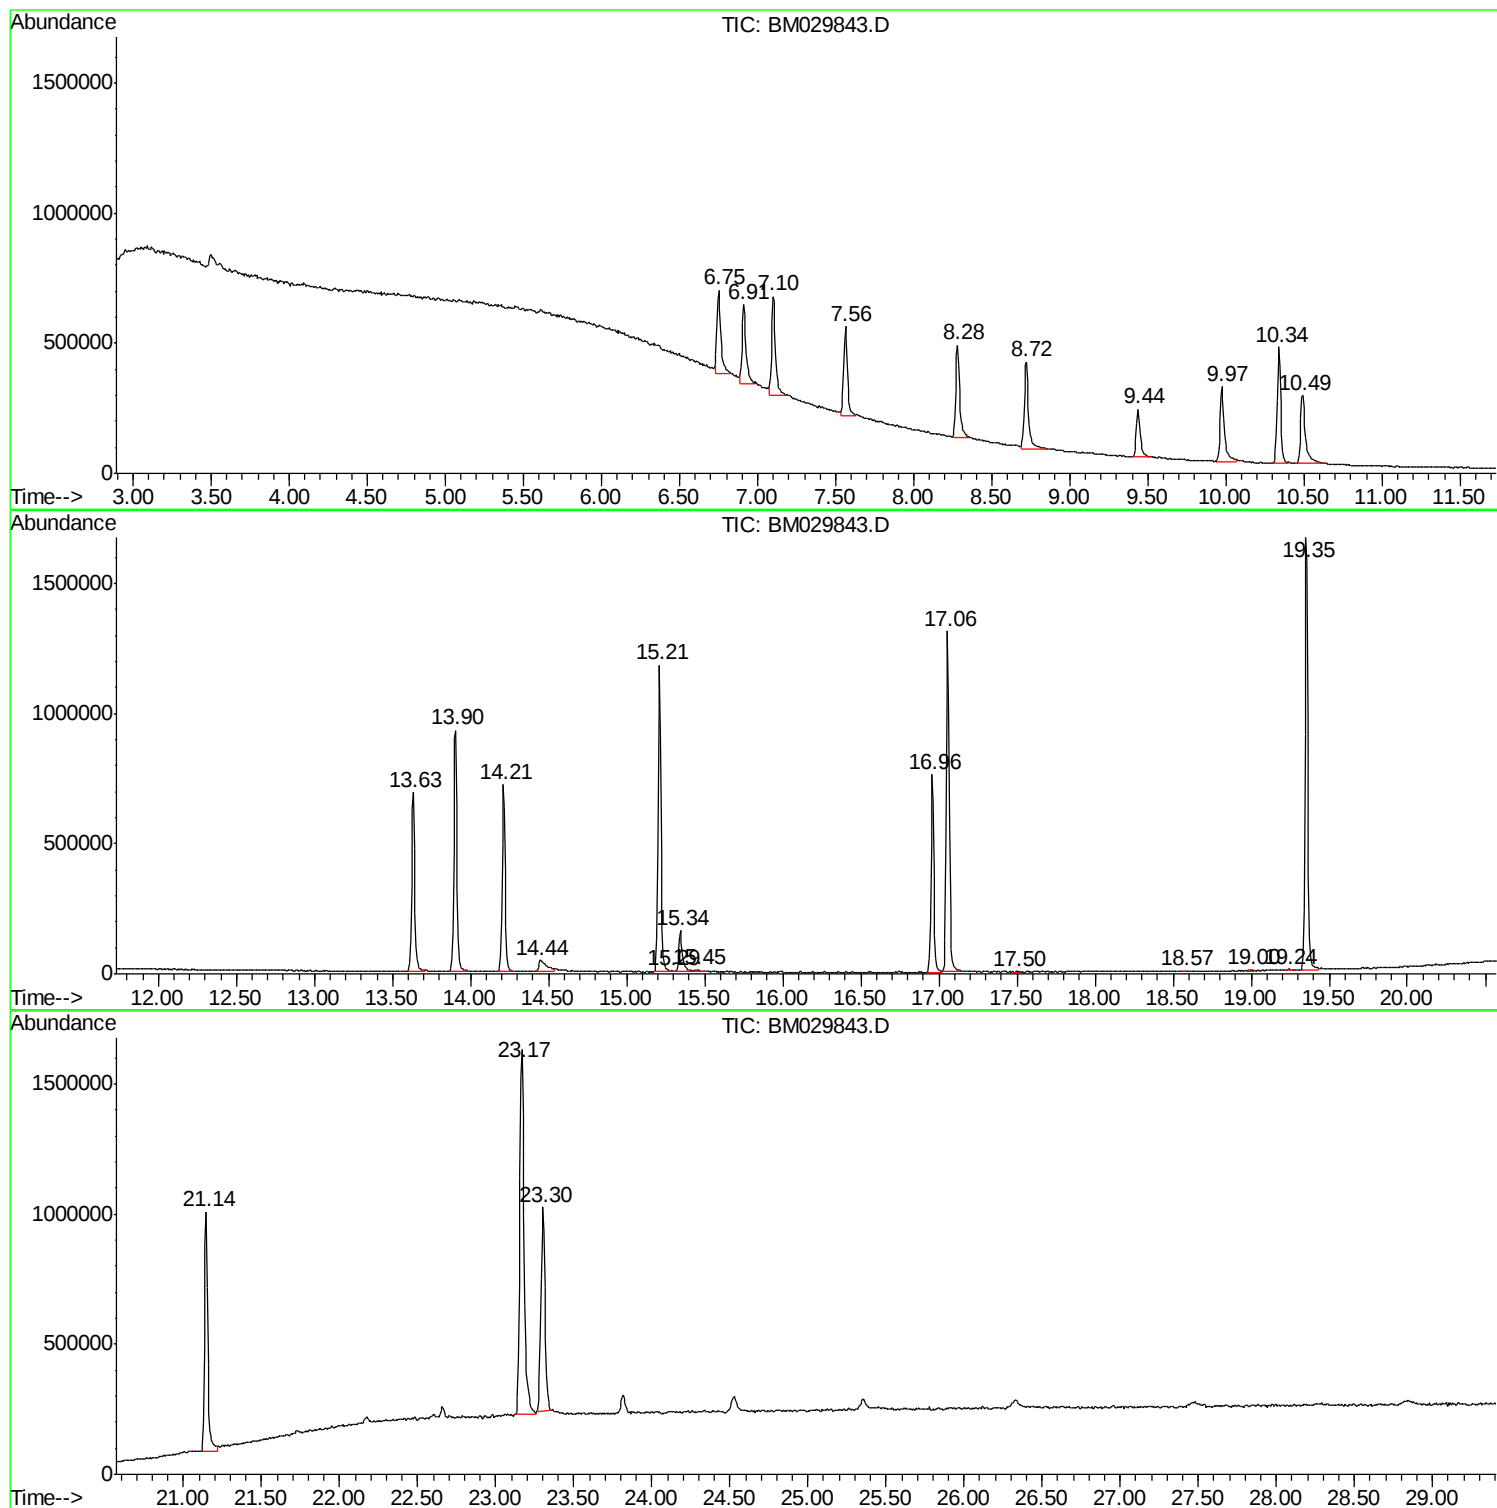

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029843.D
Acq On : 06 May 2021 01:43
Operator : CG/JU
Sample : PB136016BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK016

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050421\
Data File : BM029843.D
Acq On : 06 May 2021 01:43
Operator : CG/JU
Sample : PB136016BL
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK016

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc